

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037727.D
 Acq On : 26 Nov 2022 11:12
 Operator : CG/JU
 Sample : N5592-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB2

Quant Time: Nov 27 21:26:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	186957	20.000	ng/ul	0.00
20) Naphthalene-d8	10.934	136	924745	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.733	164	578095	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.468	188	1151783	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1040066	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1005274	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	23998	5.323	ng/uL	0.00
4) Pyridine-d5	3.875	84	165107	11.252	ng/ul	0.00
7) Phenol-d5	7.257	99	152044	8.152	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	479274	38.520	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	381848	29.462	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	277955	18.727	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	278509	38.417	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	253214	35.447	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.545	165	410352	31.391	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	533976	24.616	ng/ul	-0.01
46) Dimethylphthalate-d6	14.139	166	1687572	41.213	ng/ul	0.00
49) Acenaphthylene-d8	14.433	160	1913386	39.588	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	63684	7.061	ng/ul	-0.01
60) Fluorene-d10	15.721	176	1465830	40.874	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.833	200	206139	33.270	ng/ul	0.00
73) Anthracene-d10	17.568	188	2420321	44.936	ng/ul	0.00
81) Pyrene-d10	19.851	212	2608362	49.351	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2308694	44.617	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.145	165	13210	1.572	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037727.D
Acq On : 26 Nov 2022 11:12
Operator : CG/JU
Sample : N5592-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB2


Quant Time: Nov 27 21:26:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration

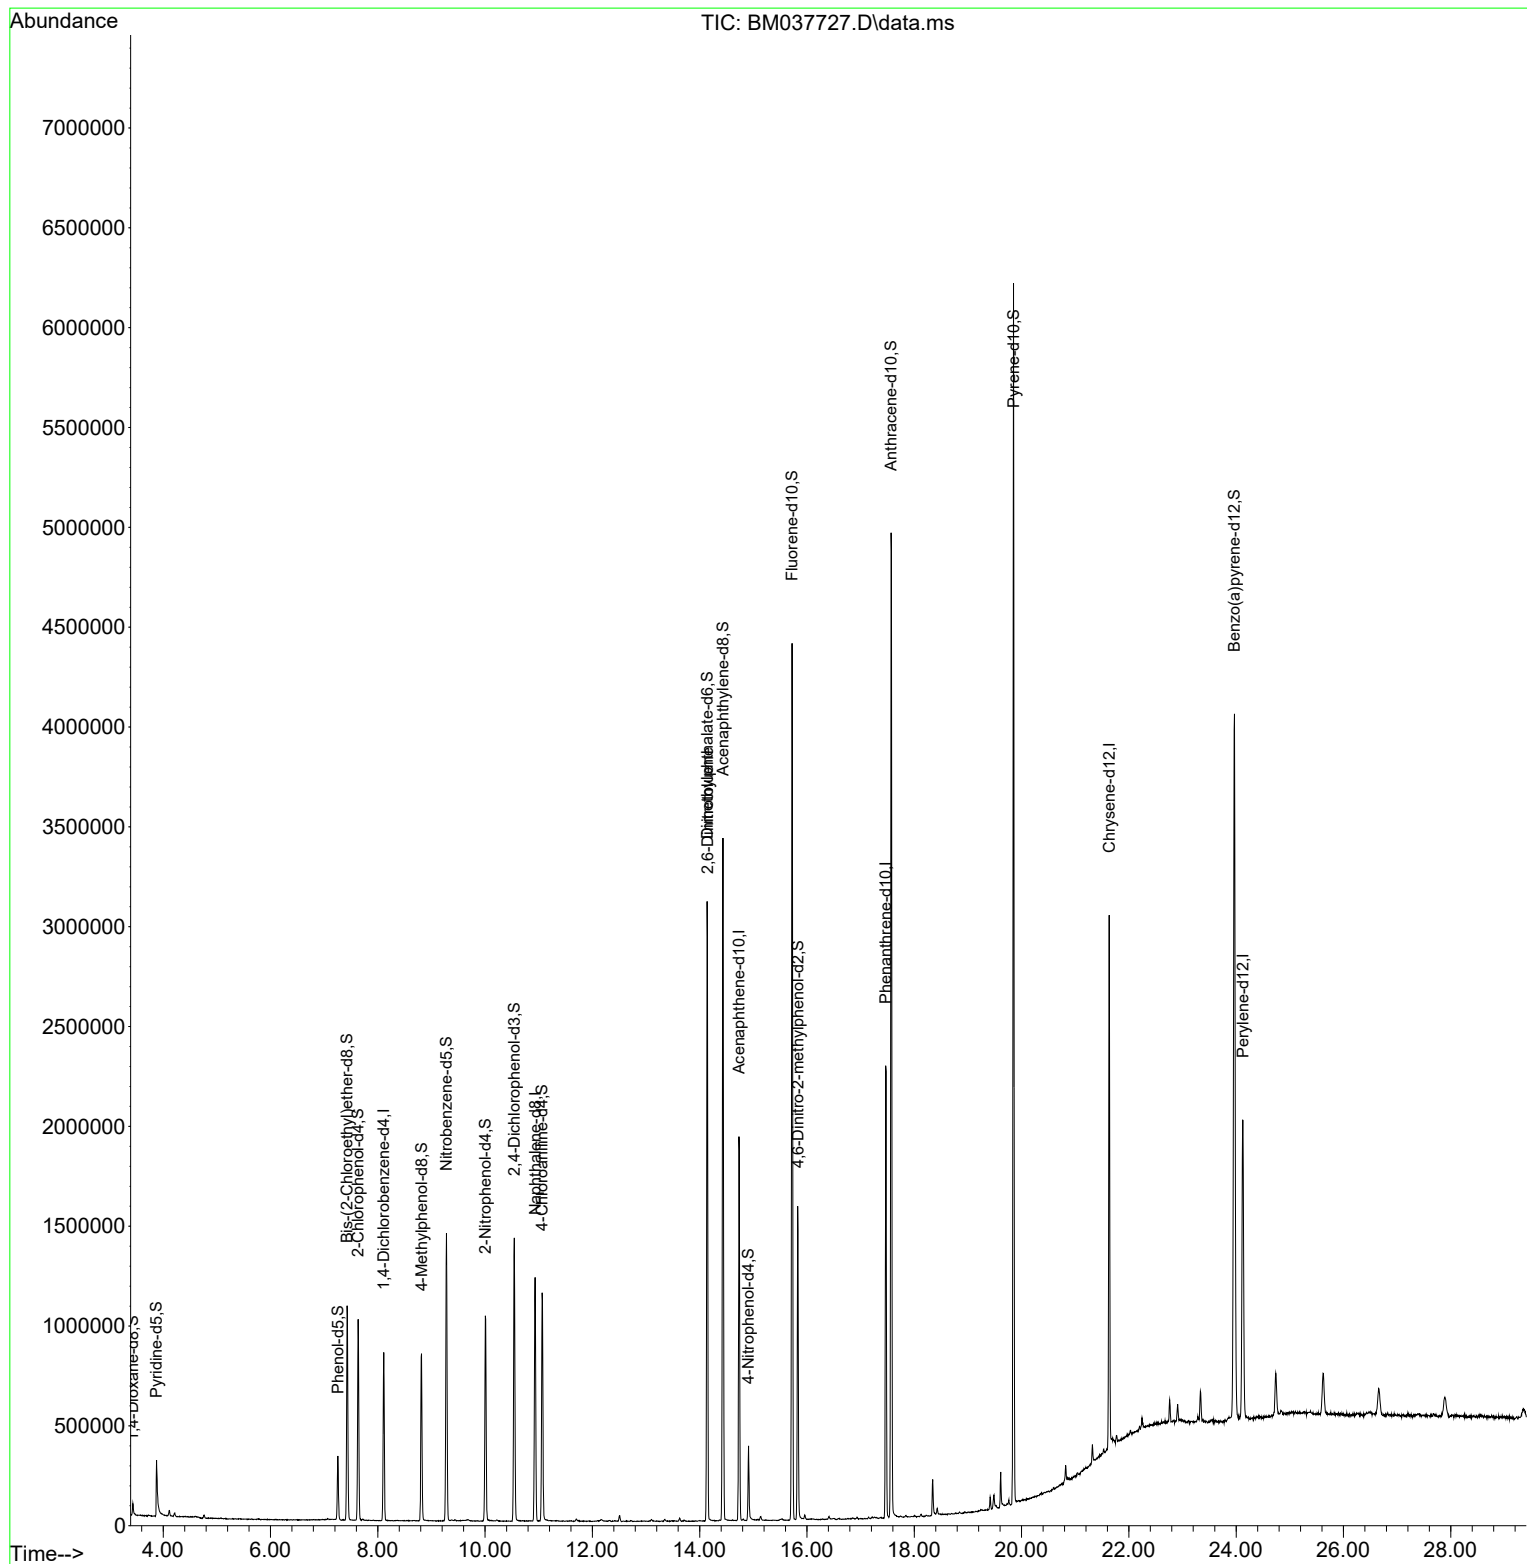

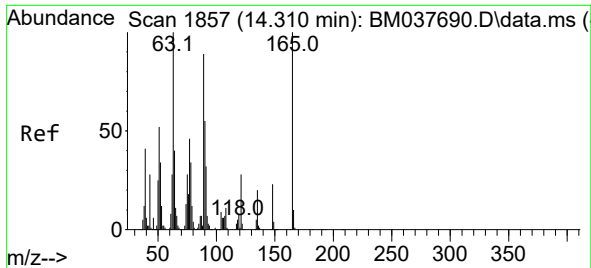

#48
 2,6-Dinitrotoluene
 Concen: 1.572 ng/ul
 RT: 14.145 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BM037727.D
 Acq: 26 Nov 2022 11:12

Instrument :
 BNA_M
 ClientSampleId :
 H0AB2

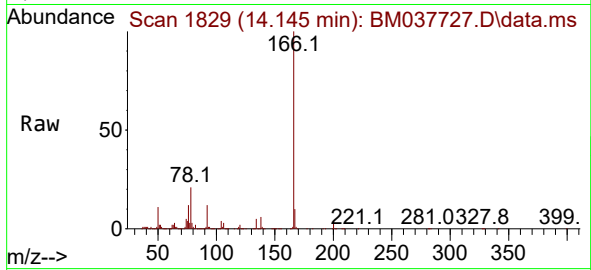

Tgt Ion:165 Resp: 13210
 Ion Ratio Lower Upper
 165 100
 89 2.3 56.4 84.6#
 121 33.6 18.9 28.3#

