

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037731.D
 Acq On : 26 Nov 2022 13:40
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020055

Quant Time: Nov 27 21:27:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	212178	20.000	ng/u1	0.00
20) Naphthalene-d8	10.933	136	1076590	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.739	164	690326	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.474	188	1409378	20.000	ng/u1	0.00
79) Chrysene-d12	21.639	240	1310363	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	1215779	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	45784	8.949	ng/uL	0.00
4) Pyridine-d5	3.869	84	377204	22.650	ng/u1	0.00
7) Phenol-d5	7.257	99	443996	20.975	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	304902	21.593	ng/u1	0.00
11) 2-Chlorophenol-d4	7.634	132	318907	21.681	ng/u1	0.00
15) 4-Methylphenol-d8	8.816	113	356146	21.143	ng/u1	0.00
21) Nitrobenzene-d5	9.281	128	178903	21.197	ng/u1	0.00
24) 2-Nitrophenol-d4	10.010	143	171571	20.631	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.545	165	315972	20.762	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	537464	21.282	ng/u1	0.00
46) Dimethylphthalate-d6	14.139	166	1016153	20.781	ng/u1	0.00
49) Acenaphthylene-d8	14.433	160	1229782	21.308	ng/u1	0.00
54) 4-Nitrophenol-d4	14.916	143	214148	19.883	ng/u1	0.00
60) Fluorene-d10	15.721	176	894329	20.884	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.833	200	136652	18.024	ng/u1	0.00
73) Anthracene-d10	17.574	188	1407182	21.351	ng/u1	0.00
81) Pyrene-d10	19.851	212	1505740	22.612	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.962	264	1324205	21.160	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.469	88	49086	8.727	ng/uL#	91
5) Pyridine	3.893	79	382412	22.582	ng/u1	99
6) Benzaldehyde	7.240	77	235721	21.217	ng/u1	98
8) Phenol	7.287	94	472840	21.310	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.522	93	381150	21.189	ng/u1	99
12) 2-Chlorophenol	7.669	128	351987	21.906	ng/u1	99
13) 2-Methylphenol	8.551	108	361900	21.380	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.639	45	700395	21.556	ng/u1	99
16) Acetophenone	8.939	105	601593	21.695	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.928	70	359241	22.104	ng/u1	99
18) 4-Methylphenol	8.881	108	400026	21.390	ng/u1	97
19) Hexachloroethane	9.204	117	155718	22.407	ng/u1	94
22) Nitrobenzene	9.322	77	510196	22.170	ng/u1	96
23) Isophorone	9.851	82	974914	21.019	ng/u1	100
25) 2-Nitrophenol	10.039	139	200600	21.327	ng/u1	97
26) 2,4-Dimethylphenol	10.092	107	463706	22.448	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.334	93	555593	20.881	ng/u1	100
29) 2,4-Dichlorophenol	10.575	162	327593	21.041	ng/u1	98
30) Naphthalene	10.986	128	1263411	21.463	ng/u1	100
32) 4-Chloroaniline	11.092	127	561765	21.346	ng/u1	99
33) Hexachlorobutadiene	11.269	225	168273	20.588	ng/u1	98
34) Caprolactam	11.869	113	91355	14.089	ng/u1	96
35) 4-Chloro-3-methylphenol	12.198	107	433663	21.789	ng/u1	96
36) 2-Methylnaphthalene	12.580	142	858910	21.004	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037731.D
 Acq On : 26 Nov 2022 13:40
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 43 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SSTD020055


Quant Time: Nov 27 21:27:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.798	142	863588	20.992	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.945	216	335565	19.797	ng/ul	95
40) Hexachlorocyclopentadiene	12.922	237	193310	18.314	ng/ul	96
41) 2,4,6-Trichlorophenol	13.174	196	243424	19.943	ng/ul	97
42) 2,4,5-Trichlorophenol	13.245	196	266893	20.436	ng/ul	97
43) 1,1'-Biphenyl	13.574	154	1112118	21.215	ng/ul	99
44) 2-Chloronaphthalene	13.622	162	857233	21.039	ng/ul	98
45) 2-Nitroaniline	13.822	65	349772	22.643	ng/ul	97
47) Dimethylphthalate	14.186	163	1078712	20.754	ng/ul	99
48) 2,6-Dinitrotoluene	14.310	165	213440	21.266	ng/ul	89
50) Acenaphthylene	14.463	152	1403822	21.518	ng/ul	99
51) 3-Nitroaniline	14.639	138	244700	20.093	ng/ul	98
52) Acenaphthene	14.798	153	1012749	21.706	ng/ul	99
53) 2,4-Dinitrophenol	14.839	184	94372	16.026	ng/ul	91
55) 4-Nitrophenol	14.933	109	216497	22.431	ng/ul	92
56) Dibenzofuran	15.133	168	1290876	21.198	ng/ul	96
57) 2,4-Dinitrotoluene	15.086	165	317546	21.562	ng/ul	90
58) 2,3,4,6-Tetrachlorophenol	15.351	232	213667	19.941	ng/ul	92
59) Diethylphthalate	15.545	149	1208430	21.541	ng/ul	99
61) Fluorene	15.780	166	1113764	21.113	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.768	204	470062	20.427	ng/ul	94
63) 4-Nitroaniline	15.792	138	245977	21.251	ng/ul	87
66) 4,6-Dinitro-2-methylph...	15.851	198	149453	18.574	ng/ul	96
67) N-Nitrosodiphenylamine	15.980	169	949011	21.671	ng/ul	98
68) 4-Bromophenyl-phenylether	16.663	248	209780	18.505	ng/ul	96
69) Hexachlorobenzene	16.780	284	294465	20.225	ng/ul	99
70) Atrazine	16.921	200	291080	19.583	ng/ul	98
71) Pentachlorophenol	17.121	266	179133	18.582	ng/ul	97
72) Phenanthrene	17.515	178	1763257	21.357	ng/ul	99
74) Anthracene	17.604	178	1800030	21.476	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.545	216	343424	20.369	ng/uL	99
76) Pentachlorobenzene	15.051	250	362317	20.205	ng/uL	98
77) Carbazole	17.874	167	1700569	21.341	ng/ul	98
78) Di-n-butylphthalate	18.427	149	2194733	19.027	ng/ul	99
80) Fluoranthene	19.515	202	1921701	22.591	ng/ul	98
82) Pyrene	19.880	202	2054291	22.865	ng/ul	99
83) Butylbenzylphthalate	20.762	149	1007760	24.078	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.545	252	517191	19.652	ng/ul	99
85) Benzo(a)anthracene	21.621	228	1863128	21.253	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.527	149	1469460	23.238	ng/ul	99
87) Chrysene	21.674	228	1734305	21.023	ng/ul	98
89) Di-n-octyl phthalate	22.480	149	2511756	24.185	ng/ul	100
90) Benzo(b)fluoranthene	23.362	252	1745498	21.119	ng/ul	100
91) Benzo(k)fluoranthene	23.409	252	1704765	21.151	ng/ul	99
93) Benzo(a)pyrene	24.015	252	1505888	20.963	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.732	276	1596744	19.375	ng/ul	99
95) Dibenzo(a,h)anthracene	26.750	278	1434743	19.390	ng/ul	98
96) Benzo(g,h,i)perylene	27.538	276	1399875	19.507	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 27 21:27:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration




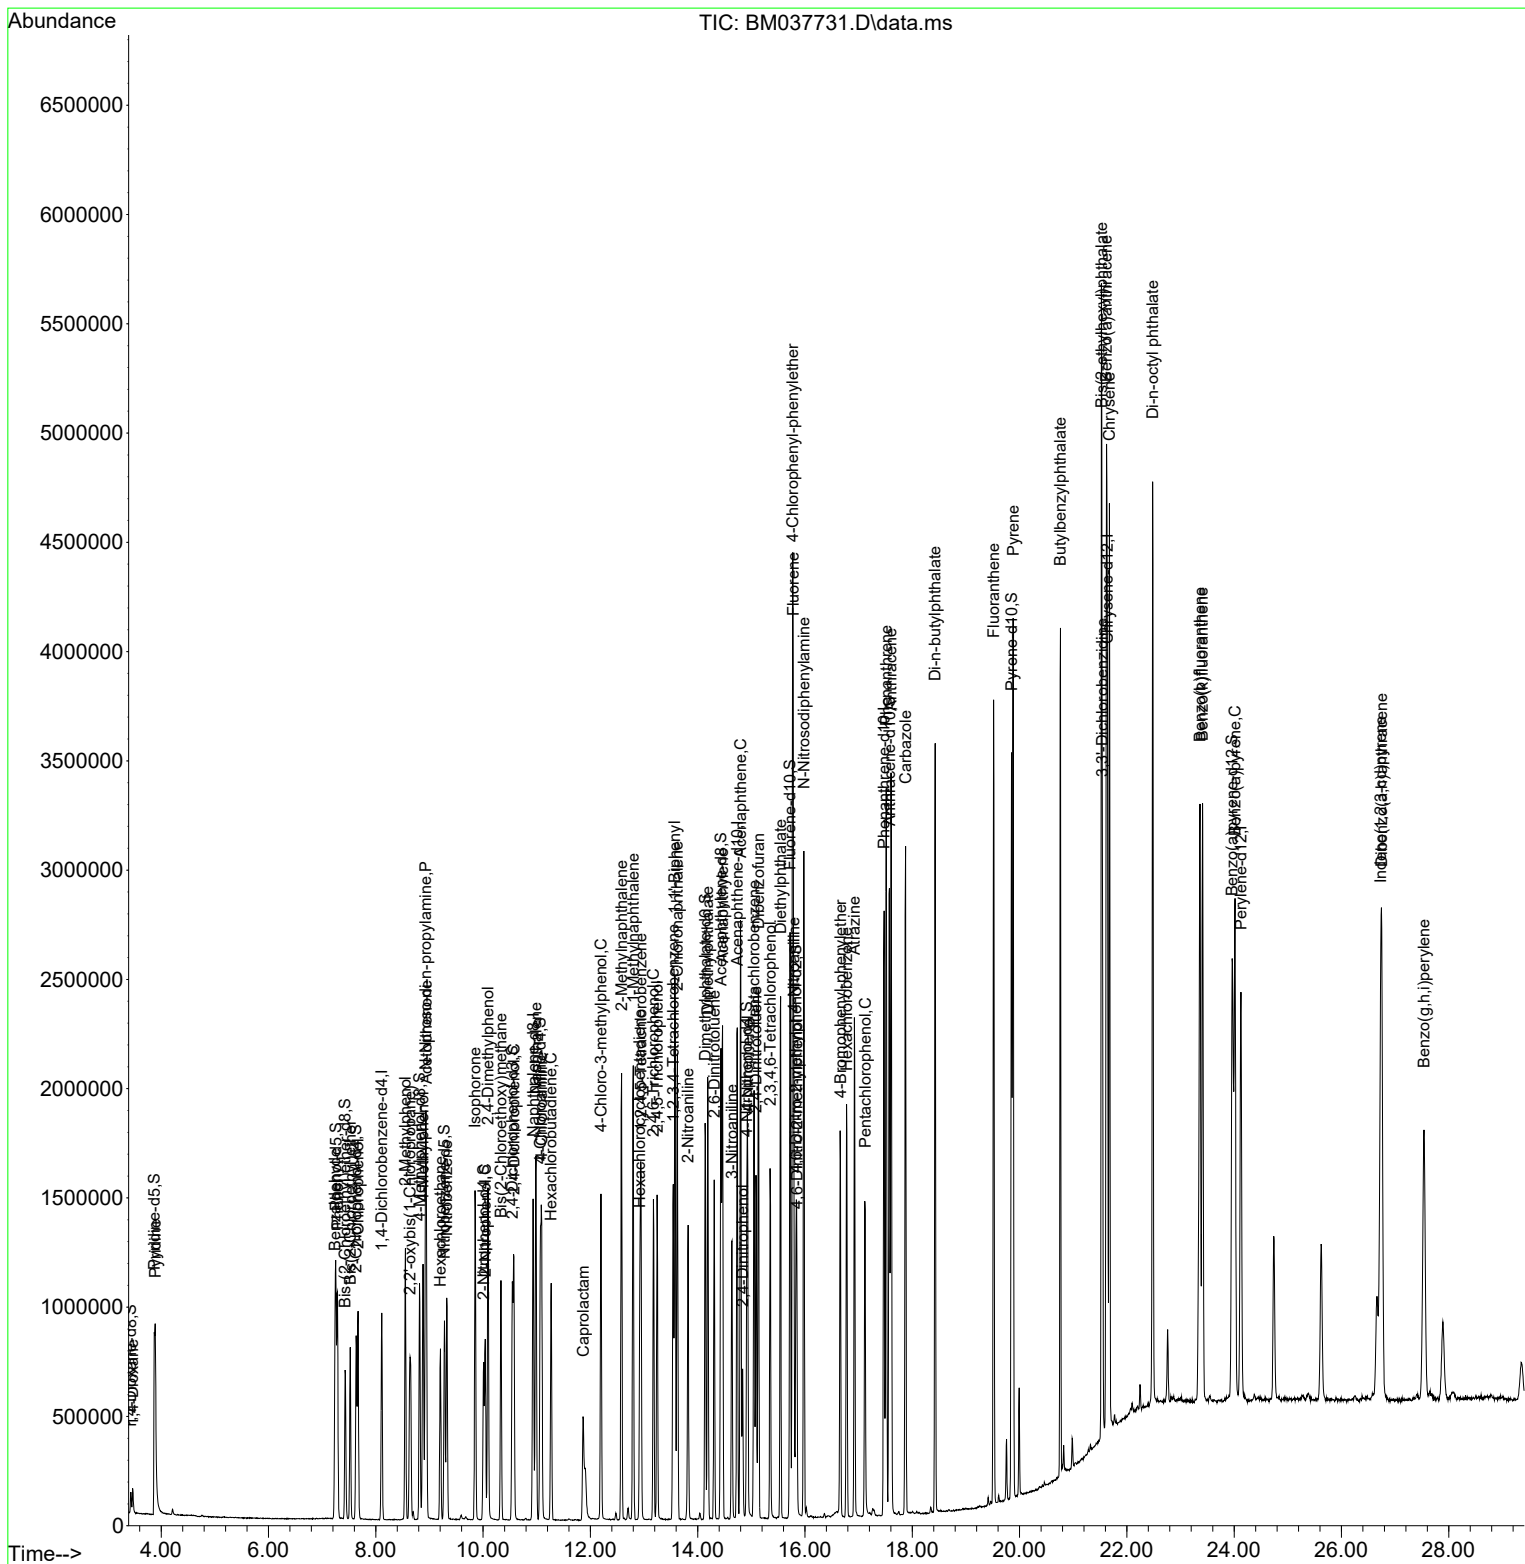




#2
1,4-Dioxane
Concen: 8.727 ng/uL
RT: 3.469 min Scan# 14
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion: 88 Resp: 49086
Ion Ratio Lower Upper
88 100
43 42.1 42.8 64.2#
58 81.9 62.6 94.0

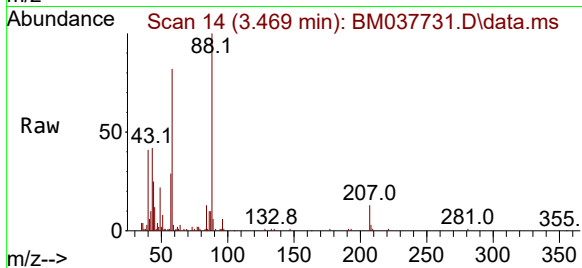

#5
Pyridine
Concen: 22.582 ng/uL
RT: 3.893 min Scan# 86
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion: 79 Resp: 382412
Ion Ratio Lower Upper
79 100
52 84.7 68.2 102.4
51 41.9 32.4 48.6




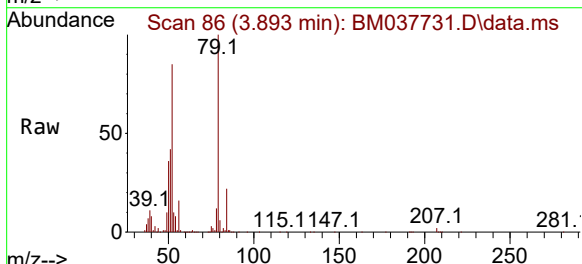




#6
Benzaldehyde
Concen: 21.217 ng/ul
RT: 7.240 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion: 77 Resp: 235721
Ion Ratio Lower Upper
77 100
105 88.3 73.4 110.0
106 86.9 70.2 105.2

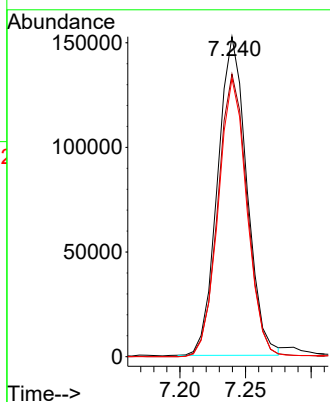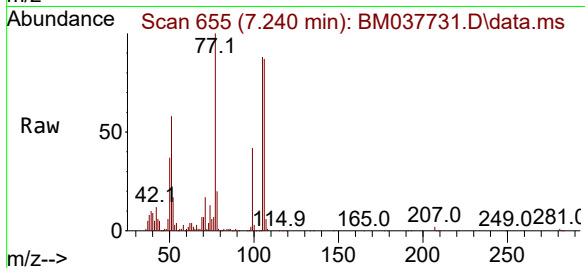

#8
Phenol
Concen: 21.310 ng/ul
RT: 7.287 min Scan# 663
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion: 94 Resp: 472840
Ion Ratio Lower Upper
94 100
65 32.4 25.0 37.4
66 43.2 31.0 46.6



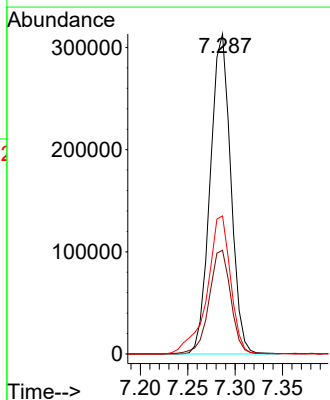
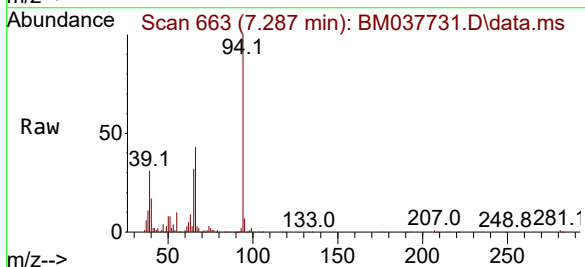




#10
Bis(2-Chloroethyl)ether
Concen: 21.189 ng/ul
RT: 7.522 min Scan# 704
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion: 93 Resp: 381150
Ion Ratio Lower Upper
93 100
63 85.8 68.6 103.0
95 32.3 27.1 40.7

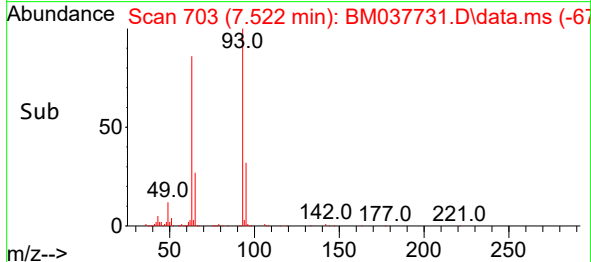

#12
2-Chlorophenol
Concen: 21.906 ng/ul
RT: 7.669 min Scan# 728
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:128 Resp: 351987
Ion Ratio Lower Upper
128 100
64 53.3 42.2 63.4
130 33.6 26.1 39.1




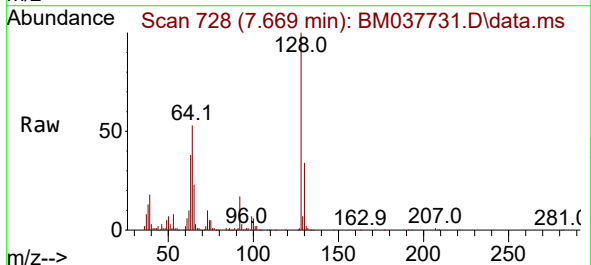




#13
2-Methylphenol
Concen: 21.380 ng/ul
RT: 8.551 min Scan# 81
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:108 Resp: 361900
Ion Ratio Lower Upper
108 100
107 86.8 70.6 106.0

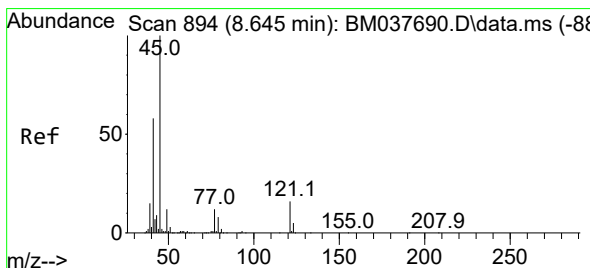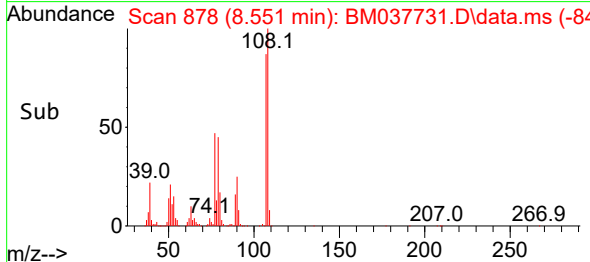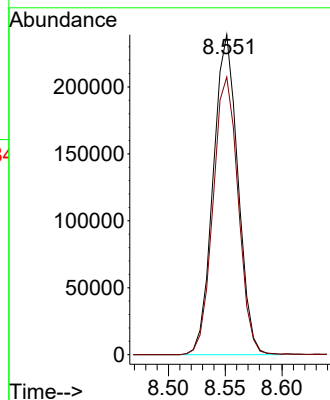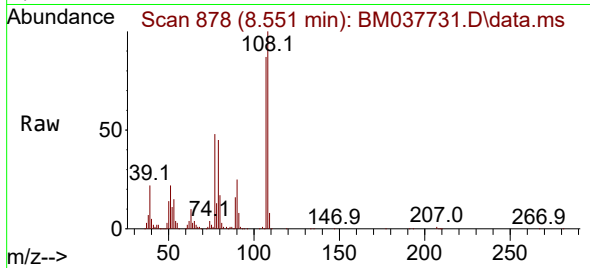

#14
2,2'-oxybis(1-Chloropropane)
Concen: 21.556 ng/ul
RT: 8.639 min Scan# 893
Delta R.T. -0.012 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion: 45 Resp: 700395
Ion Ratio Lower Upper
45 100
77 11.8 9.4 14.0
79 8.8 7.3 10.9


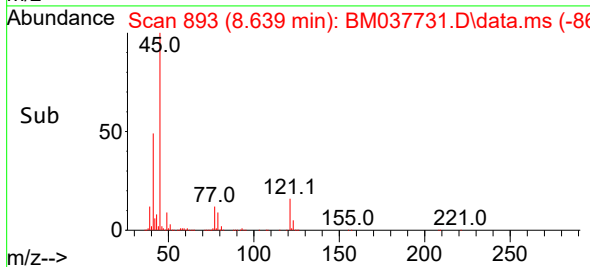
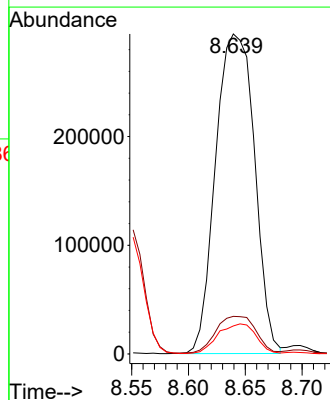
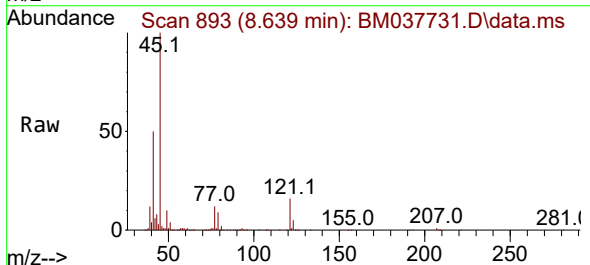




#16
Acetophenone
Concen: 21.695 ng/ul
RT: 8.939 min Scan# 945
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:105 Resp: 601593
Ion Ratio Lower Upper
105 100
77 86.0 66.6 99.8
51 36.9 27.3 40.9

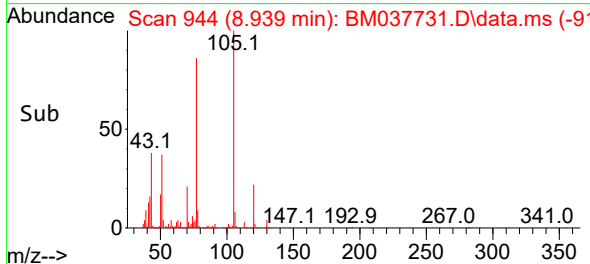

#17
N-Nitroso-di-n-propylamine
Concen: 22.104 ng/ul
RT: 8.928 min Scan# 942
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion: 70 Resp: 359241
Ion Ratio Lower Upper
70 100
42 72.5 57.1 85.7
101 8.8 7.0 10.6
130 18.0 14.8 22.2

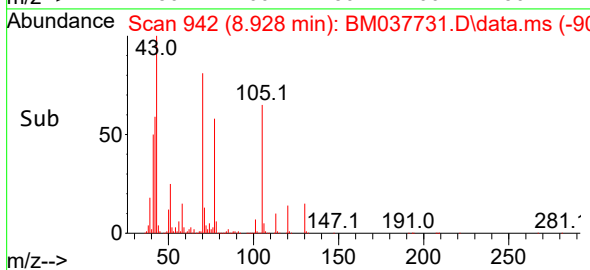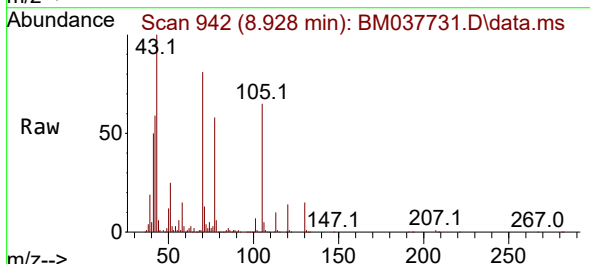



#18

4-Methylphenol

Concen: 21.390 ng/ul

RT: 8.881 min Scan# 91

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :





SSTD020055

Tgt Ion:108 Resp: 400026

Ion Ratio Lower Upper

108 100

107 109.8 90.4 135.6

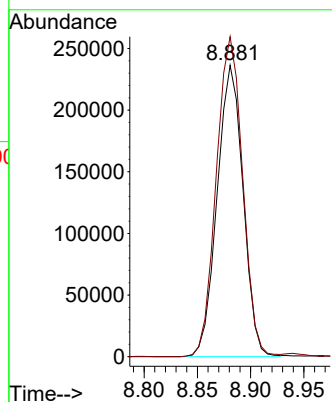

#19

Hexachloroethane

Concen: 22.407 ng/ul

RT: 9.204 min Scan# 989

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40




Tgt Ion:117 Resp: 155718


Ion Ratio Lower Upper

117 100

201 71.1 60.4 90.6

199 43.0 38.1 57.1









#22
Nitrobenzene
Concen: 22.170 ng/ul
RT: 9.322 min Scan# 1009
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion: 77 Resp: 510196
Ion Ratio Lower Upper
77 100
123 37.5 32.4 48.6
65 14.0 11.4 17.0

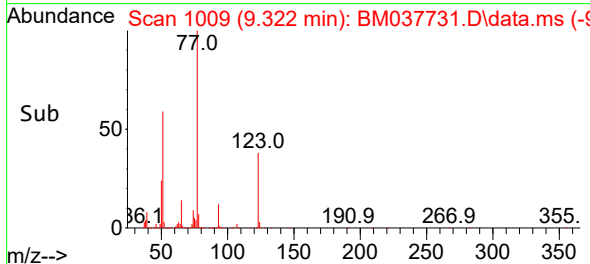

#23
Isophorone
Concen: 21.019 ng/ul
RT: 9.851 min Scan# 1099
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion: 82 Resp: 974914
Ion Ratio Lower Upper
82 100
95 6.9 5.3 7.9
138 15.5 12.5 18.7


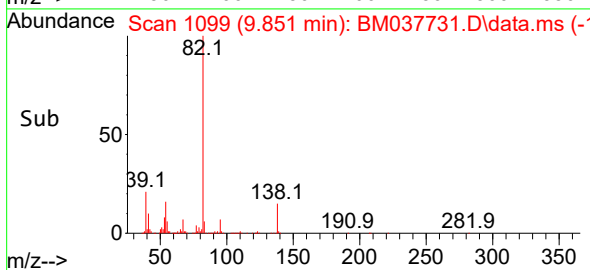

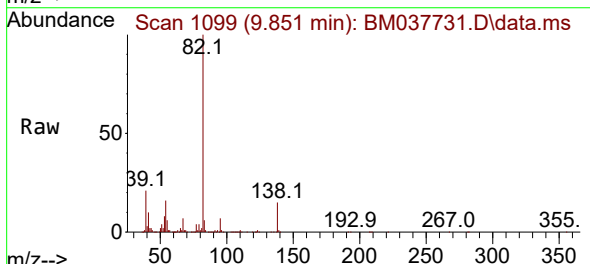


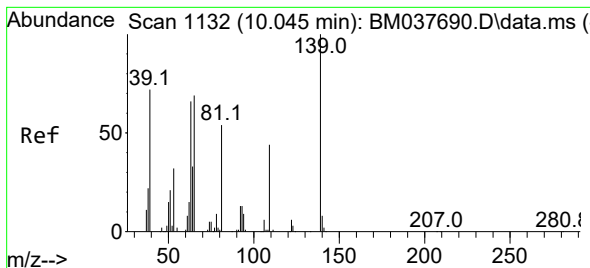

#25
2-Nitrophenol
Concen: 21.327 ng/ul
RT: 10.039 min Scan# 1132
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:139 Resp: 200600
Ion Ratio Lower Upper
139 100
65 64.2 49.6 74.4
109 34.8 25.8 38.6

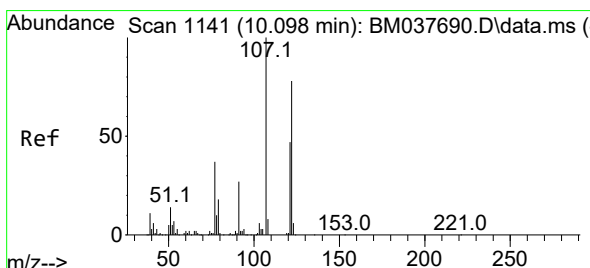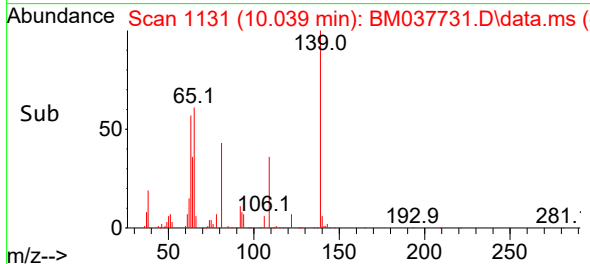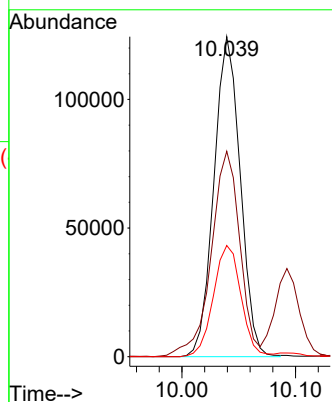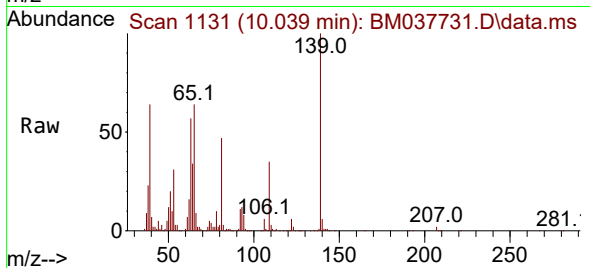

#26
2,4-Dimethylphenol
Concen: 22.448 ng/ul
RT: 10.092 min Scan# 1140
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:107 Resp: 463706
Ion Ratio Lower Upper
107 100
121 47.6 39.6 59.4
122 81.6 69.0 103.6


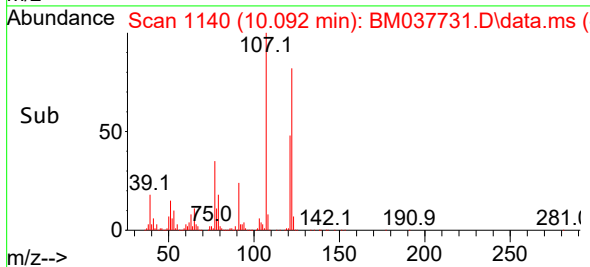
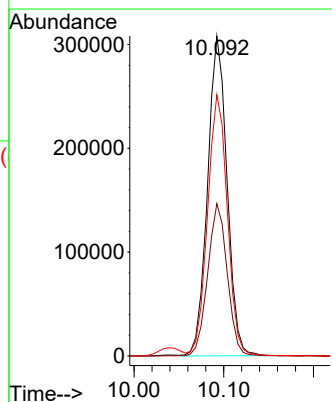
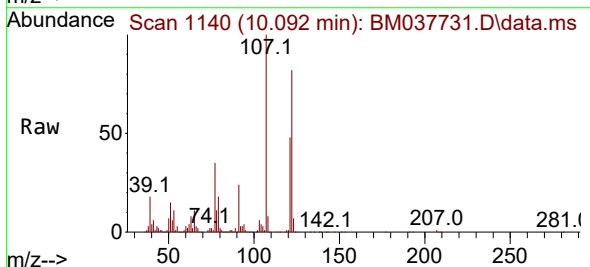




#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.881 ng/ul
 RT: 10.334 min Scan# 1181
 Delta R.T. -0.006 min
 Lab File: BM037731.D
 Acq: 26 Nov 2022 13:40




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020055


Tgt Ion: 93 Resp: 555593
 Ion Ratio Lower Upper
 93 100
 95 32.7 26.4 39.6
 123 10.8 8.6 13.0

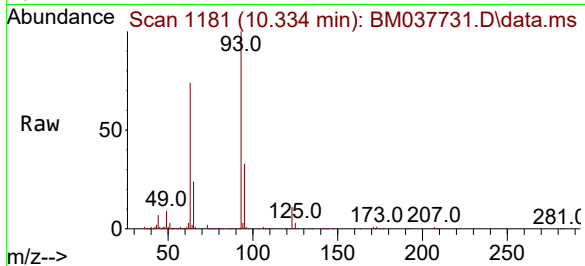

#29
 2,4-Dichlorophenol
 Concen: 21.041 ng/ul
 RT: 10.575 min Scan# 1222
 Delta R.T. -0.006 min
 Lab File: BM037731.D
 Acq: 26 Nov 2022 13:40

Tgt Ion:162 Resp: 327593
 Ion Ratio Lower Upper
 162 100
 164 63.5 52.6 79.0
 98 41.6 33.6 50.4




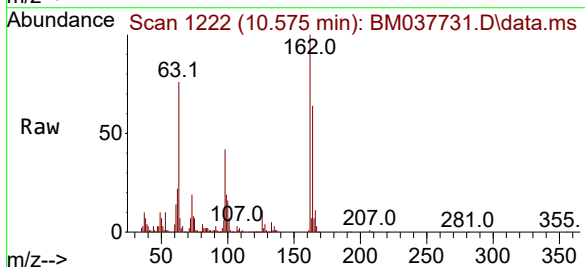




#30
Naphthalene
Concen: 21.463 ng/ul
RT: 10.986 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:128 Resp: 1263411
Ion Ratio Lower Upper
128 100
129 10.8 8.6 12.8
127 13.0 10.4 15.6

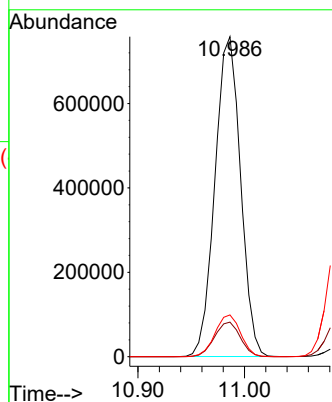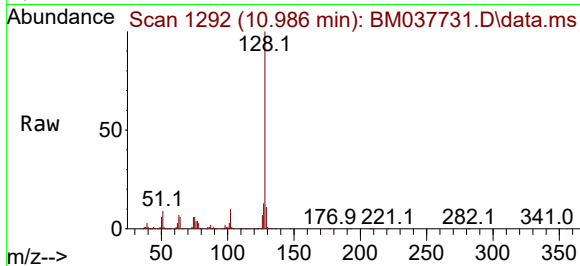

#32
4-Chloroaniline
Concen: 21.346 ng/ul
RT: 11.092 min Scan# 1310
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:127 Resp: 561765
Ion Ratio Lower Upper
127 100
129 32.0 26.1 39.1

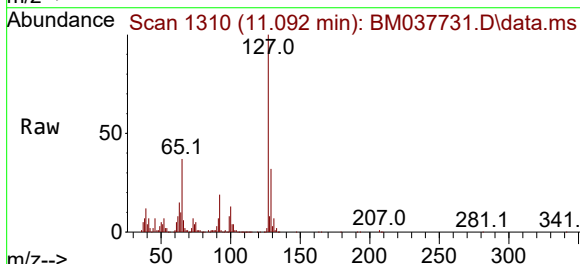



#33

Hexachlorobutadiene

Concen: 20.588 ng/ul

RT: 11.269 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :

SSTD020055





Tgt Ion:225 Resp: 168273

Ion Ratio Lower Upper

225 100

223 62.7 51.1 76.7

227 65.4 50.7 76.1

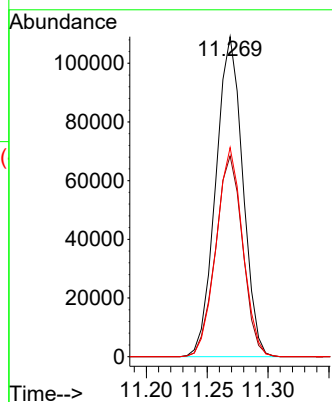

#34

Caprolactam

Concen: 14.089 ng/ul

RT: 11.869 min Scan# 1442

Delta R.T. 0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40




Tgt Ion:113 Resp: 91355


Ion Ratio Lower Upper

113 100

55 194.3 163.3 244.9

56 148.5 120.3 180.5




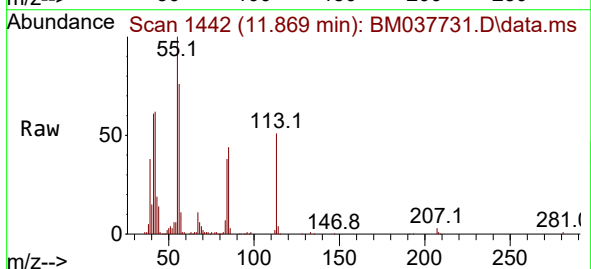




#35
4-Chloro-3-methylphenol
Concen: 21.789 ng/ul
RT: 12.198 min Scan# 1498
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:107 Resp: 433663
Ion Ratio Lower Upper
107 100
144 24.1 20.2 30.4
142 74.3 62.6 93.8

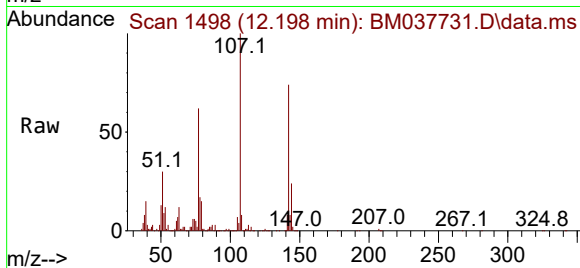

#36
2-Methylnaphthalene
Concen: 21.004 ng/ul
RT: 12.580 min Scan# 1563
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:142 Resp: 858910
Ion Ratio Lower Upper
142 100
141 89.2 72.2 108.4




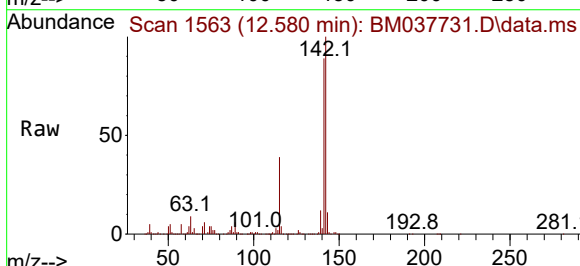




#37
1-Methylnaphthalene
Concen: 20.992 ng/ul
RT: 12.798 min Scan# 1600
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:142 Resp: 863588
Ion Ratio Lower Upper
142 100
141 93.5 73.3 109.9
116 4.3 3.2 4.8

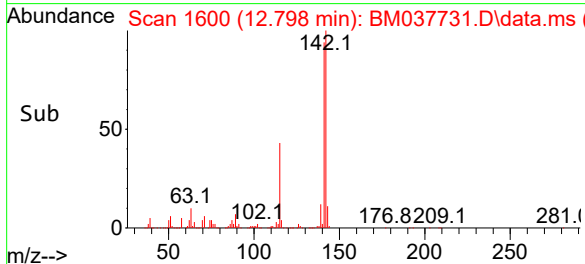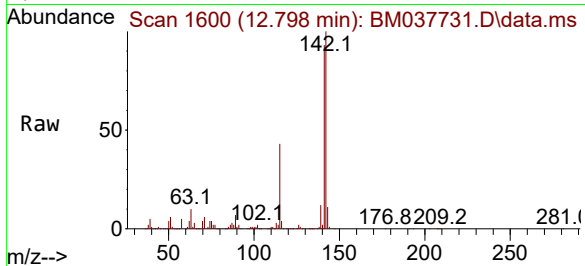

#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.797 ng/ul
RT: 12.945 min Scan# 1625
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:216 Resp: 335565
Ion Ratio Lower Upper
216 100
214 79.2 60.2 90.4
179 24.1 18.6 27.8
108 27.5 18.3 27.5

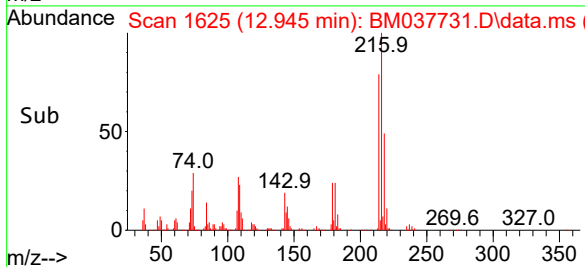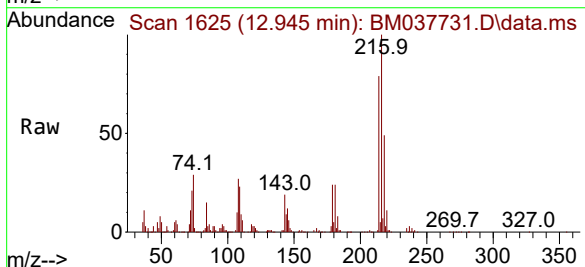



#40

Hexachlorocyclopentadiene

Concen: 18.314 ng/ul

RT: 12.922 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :

SSTD020055





Tgt Ion:237 Resp: 193310

Ion Ratio Lower Upper

237 100

235 65.2 49.1 73.7

272 12.6 9.5 14.3

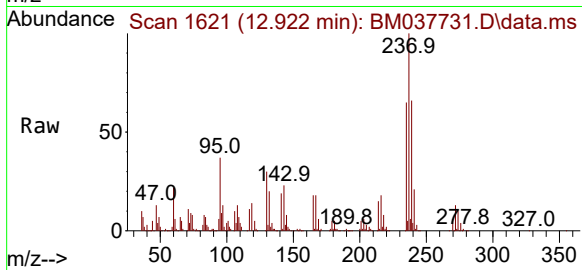

#41

2,4,6-Trichlorophenol

Concen: 19.943 ng/ul

RT: 13.174 min Scan# 1664

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40




Tgt Ion:196 Resp: 243424


Ion Ratio Lower Upper

196 100

198 92.6 76.9 115.3

200 30.2 24.1 36.1



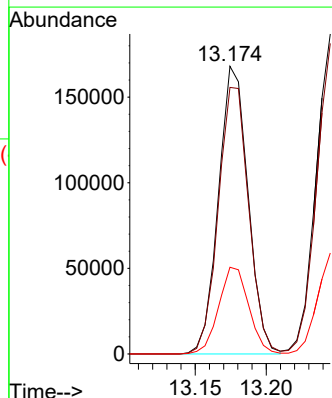
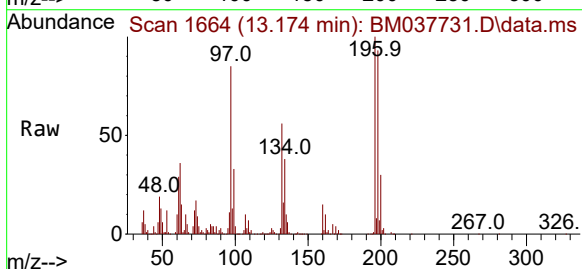




#42
2,4,5-Trichlorophenol
Concen: 20.436 ng/ul
RT: 13.245 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:196 Resp: 266893
Ion Ratio Lower Upper
196 100
198 97.1 75.4 113.2
200 31.5 23.7 35.5

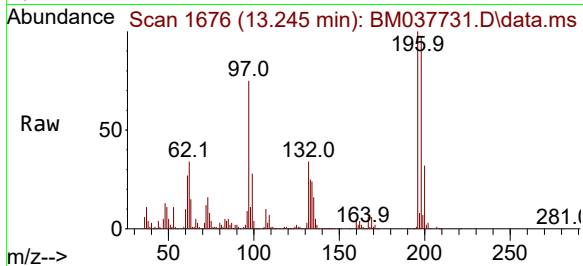

#43
1,1'-Biphenyl
Concen: 21.215 ng/ul
RT: 13.574 min Scan# 1732
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:154 Resp: 1112118
Ion Ratio Lower Upper
154 100
153 40.9 32.1 48.1
76 15.5 12.4 18.6




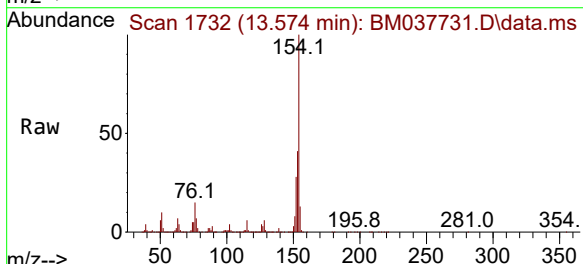




#44
2-Chloronaphthalene
Concen: 21.039 ng/ul
RT: 13.622 min Scan# 1740
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:162 Resp: 857233
Ion Ratio Lower Upper
162 100
164 32.8 26.5 39.7
127 43.0 32.4 48.6

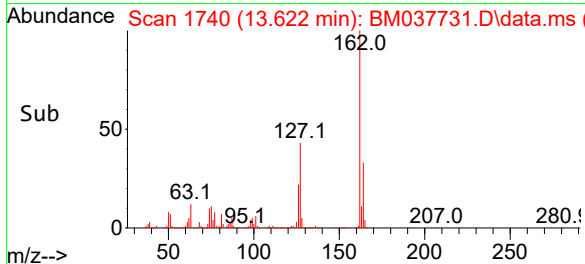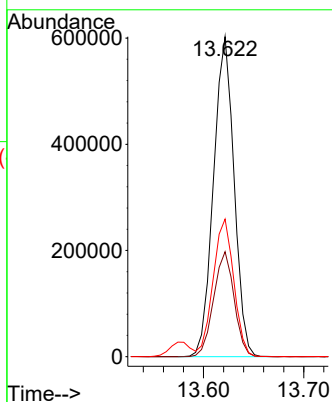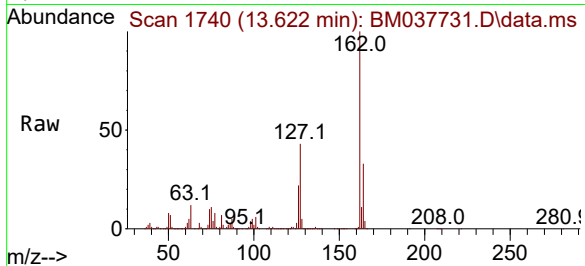

#45
2-Nitroaniline
Concen: 22.643 ng/ul
RT: 13.822 min Scan# 1774
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion: 65 Resp: 349772
Ion Ratio Lower Upper
65 100
92 63.4 48.6 73.0
138 85.7 67.0 100.4


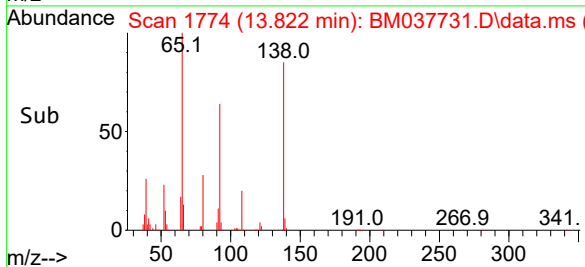
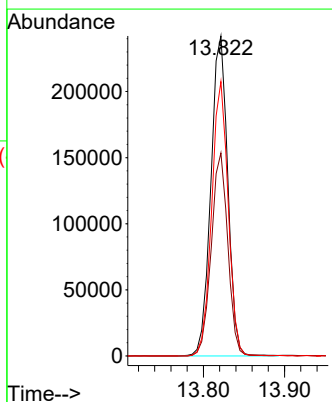
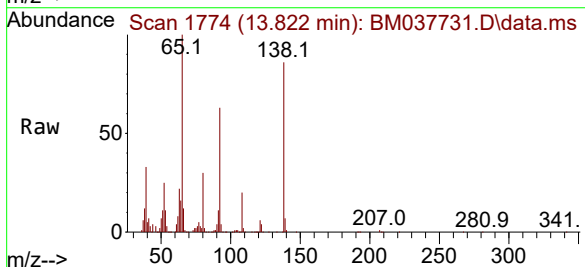




#47
Dimethylphthalate
Concen: 20.754 ng/ul
RT: 14.186 min Scan# 1836
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:163 Resp: 1078712
Ion Ratio Lower Upper
163 100
194 3.4 2.9 4.3
164 10.4 8.2 12.2

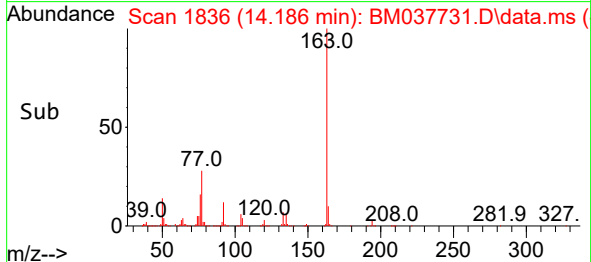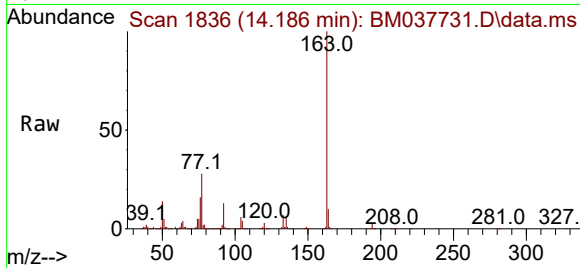

#48
2,6-Dinitrotoluene
Concen: 21.266 ng/ul
RT: 14.310 min Scan# 1857
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:165 Resp: 213440
Ion Ratio Lower Upper
165 100
89 80.3 56.4 84.6
121 26.9 18.9 28.3




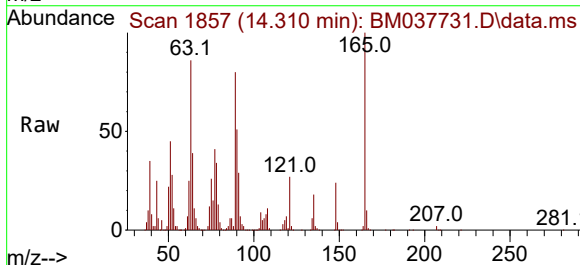




#50
Acenaphthylene
Concen: 21.518 ng/ul
RT: 14.463 min Scan# 1883
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:152 Resp: 1403822
Ion Ratio Lower Upper
152 100
151 20.1 16.3 24.5
153 12.7 10.3 15.5

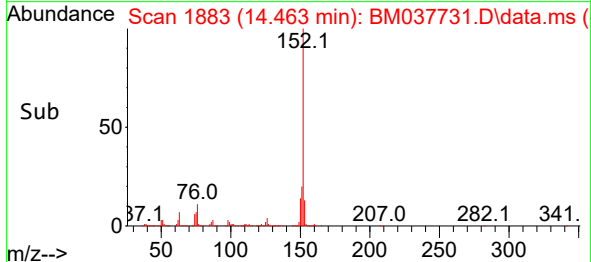

#51
3-Nitroaniline
Concen: 20.093 ng/ul
RT: 14.639 min Scan# 1913
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:138 Resp: 244700
Ion Ratio Lower Upper
138 100
108 10.8 8.4 12.6
92 127.0 104.0 156.0




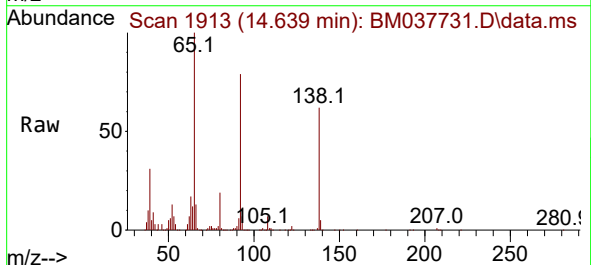




#52
Acenaphthene
Concen: 21.706 ng/ul
RT: 14.798 min Scan# 1940
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:153 Resp: 1012749
Ion Ratio Lower Upper
153 100
152 48.1 38.4 57.6
154 87.5 70.7 106.1

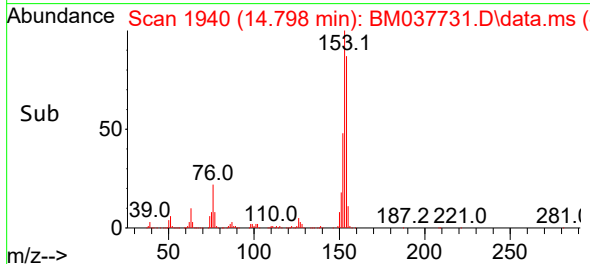

#53
2,4-Dinitrophenol
Concen: 16.026 ng/ul
RT: 14.839 min Scan# 1947
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:184 Resp: 94372
Ion Ratio Lower Upper
184 100
63 103.5 74.9 112.3
154 79.3 57.8 86.6


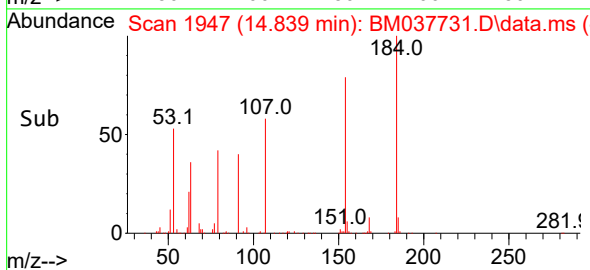

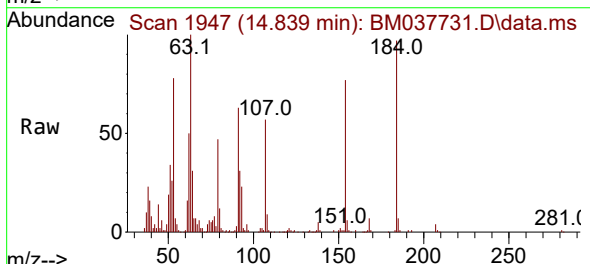




#55
4-Nitrophenol
Concen: 22.431 ng/ul
RT: 14.933 min Scan# 1963
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:109 Resp: 216497
Ion Ratio Lower Upper
109 100
139 116.7 102.4 153.6
65 142.4 119.6 179.4

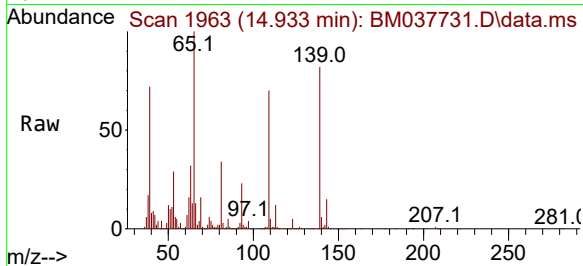

#56
Dibenzofuran
Concen: 21.198 ng/ul
RT: 15.133 min Scan# 1997
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:168 Resp: 1290876
Ion Ratio Lower Upper
168 100
139 42.9 32.2 48.2




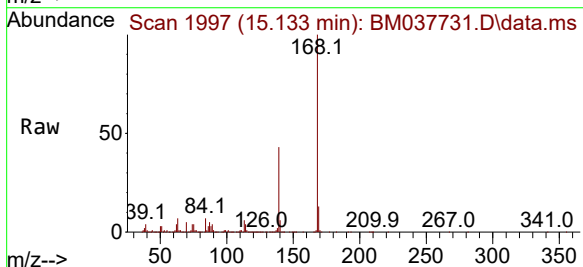




#57
2,4-Dinitrotoluene
Concen: 21.562 ng/ul
RT: 15.086 min Scan# 1990
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:165 Resp: 317546
Ion Ratio Lower Upper
165 100
63 65.9 46.6 70.0
182 2.3 1.9 2.9

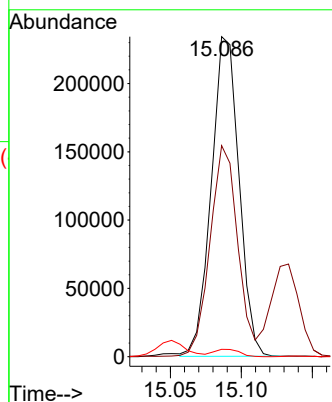

#58
2,3,4,6-Tetrachlorophenol
Concen: 19.941 ng/ul
RT: 15.351 min Scan# 2034
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:232 Resp: 213667
Ion Ratio Lower Upper
232 100
131 70.1 50.2 75.4
130 4.0 2.8 4.2
166 42.9 31.2 46.8


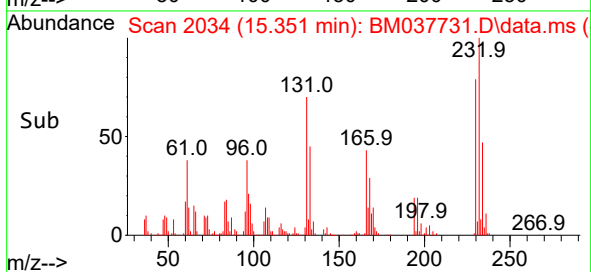

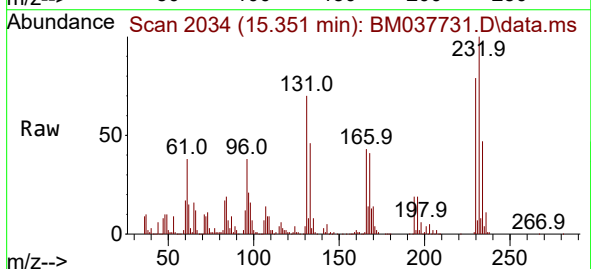




#59
Diethylphthalate
Concen: 21.541 ng/ul
RT: 15.545 min Scan# 2067
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:149 Resp: 1208430
Ion Ratio Lower Upper
149 100
177 19.5 16.1 24.1
150 12.4 9.4 14.0

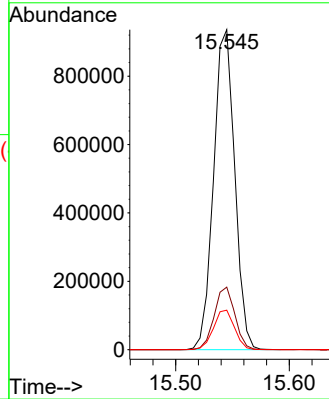

#61
Fluorene
Concen: 21.113 ng/ul
RT: 15.780 min Scan# 2107
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:166 Resp: 1113764
Ion Ratio Lower Upper
166 100
165 98.9 79.3 118.9
167 13.6 10.6 15.8


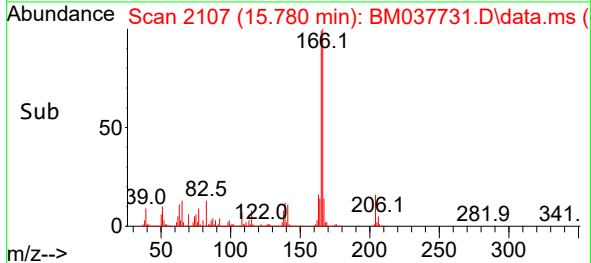
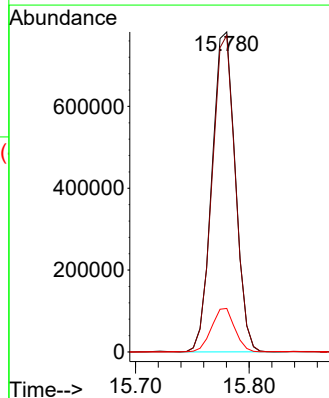





#62
4-Chlorophenyl-phenylether
Concen: 20.427 ng/ul
RT: 15.768 min Scan# 2105
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:204 Resp: 470062
Ion Ratio Lower Upper
204 100
206 32.0 25.8 38.8
141 74.7 54.3 81.5



#63
4-Nitroaniline
Concen: 21.251 ng/ul
RT: 15.792 min Scan# 2109
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:138 Resp: 245977
Ion Ratio Lower Upper
138 100
92 58.4 43.7 65.5
108 101.1 68.1 102.1









#66
 4,6-Dinitro-2-methylphenol
 Concen: 18.574 ng/ul
 RT: 15.851 min Scan# 2119
 Delta R.T. -0.000 min
 Lab File: BM037731.D
 Acq: 26 Nov 2022 13:40




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020055


Tgt Ion:198 Resp: 149453
 Ion Ratio Lower Upper
 198 100
 182 4.2 4.0 6.0
 77 37.3 27.9 41.9

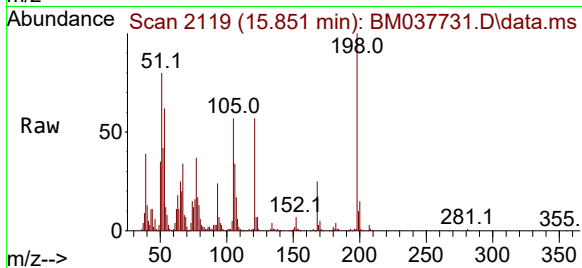

#67
 N-Nitrosodiphenylamine
 Concen: 21.671 ng/ul
 RT: 15.980 min Scan# 2141
 Delta R.T. -0.006 min
 Lab File: BM037731.D
 Acq: 26 Nov 2022 13:40

Tgt Ion:169 Resp: 949011
 Ion Ratio Lower Upper
 169 100
 168 69.4 54.0 81.0
 167 37.8 29.3 43.9




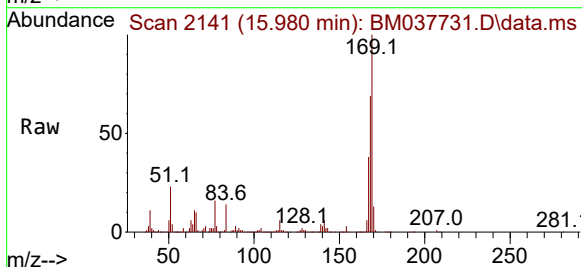




#68
4-Bromophenyl-phenylether
Concen: 18.505 ng/ul
RT: 16.663 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:248 Resp: 209780
Ion Ratio Lower Upper
248 100
250 97.3 78.5 117.7
141 105.2 78.9 118.3

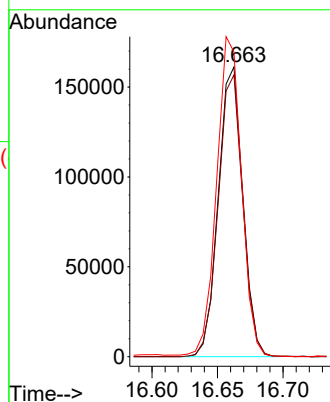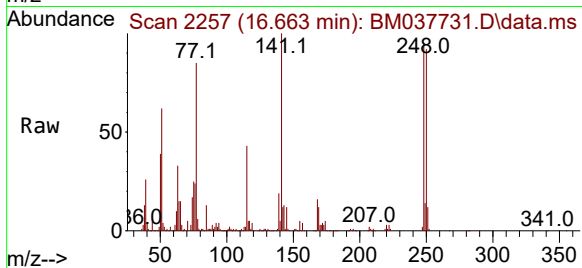

#69
Hexachlorobenzene
Concen: 20.225 ng/ul
RT: 16.780 min Scan# 2277
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:284 Resp: 294465
Ion Ratio Lower Upper
284 100
142 51.5 40.4 60.6
249 31.2 24.5 36.7



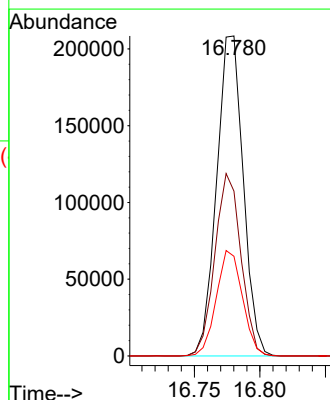
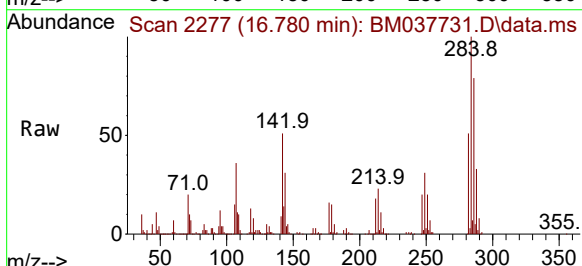




#70
Atrazine
Concen: 19.583 ng/ul
RT: 16.921 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:200 Resp: 291080
Ion Ratio Lower Upper
200 100
173 28.3 22.6 34.0
215 44.2 36.6 55.0

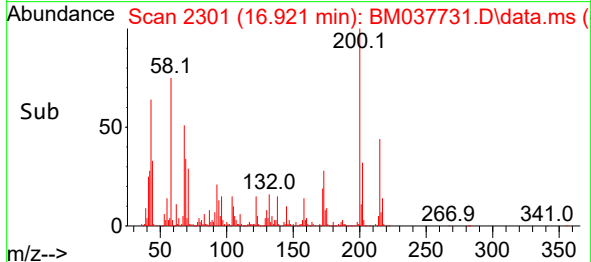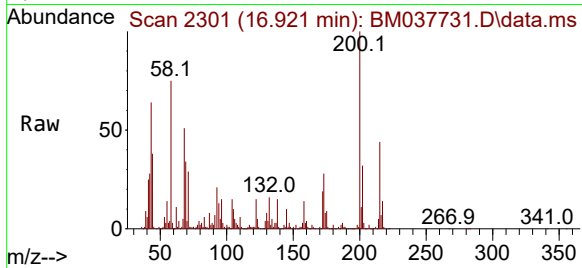

#71
Pentachlorophenol
Concen: 18.582 ng/ul
RT: 17.121 min Scan# 2335
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:266 Resp: 179133
Ion Ratio Lower Upper
266 100
264 63.0 52.0 78.0
268 62.0 52.2 78.2

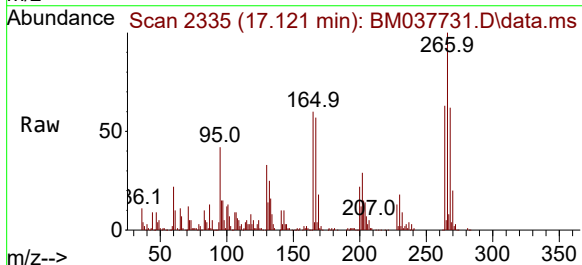



#72

Phenanthrene

Concen: 21.357 ng/ul

RT: 17.515 min Scan# 2402

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :

SSTD020055





Tgt Ion:178 Resp: 1763257

Ion Ratio Lower Upper

178 100

179 15.4 12.0 18.0

176 19.9 15.4 23.2



#74

Anthracene

Concen: 21.476 ng/ul

RT: 17.604 min Scan# 2417

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40




Tgt Ion:178 Resp: 1800030


Ion Ratio Lower Upper

178 100

179 15.7 12.6 18.8

176 18.7 15.0 22.4





#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.369 ng/uL

RT: 13.545 min Scan# 11

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :

SSTD020055





Tgt Ion:216 Resp: 343424

Ion Ratio Lower Upper

216 100

214 77.4 63.3 94.9

218 47.9 38.6 58.0

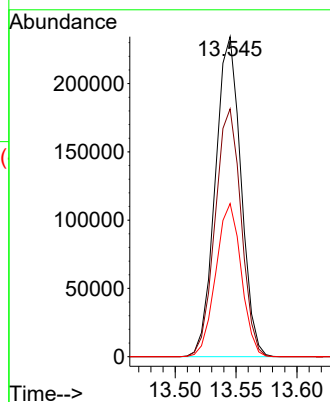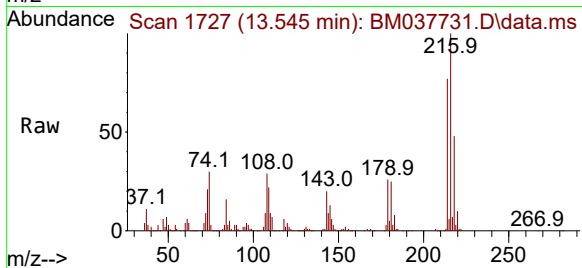

#76

Pentachlorobenzene

Concen: 20.205 ng/uL

RT: 15.051 min Scan# 1983

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40




Tgt Ion:250 Resp: 362317


Ion Ratio Lower Upper

250 100

248 63.5 50.1 75.1

252 64.1 49.9 74.9


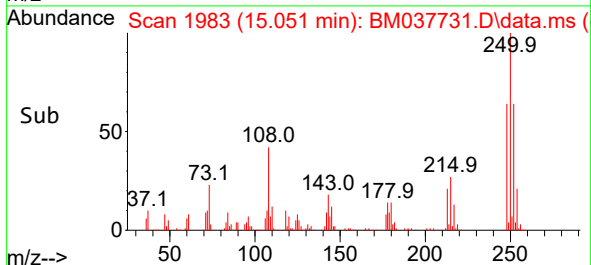
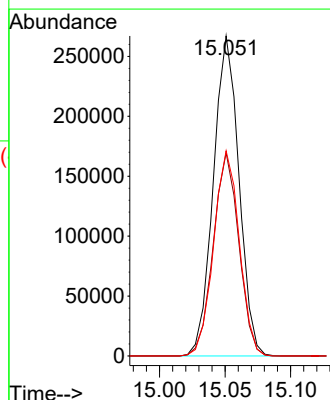
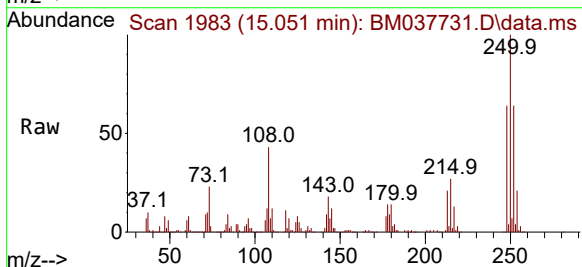




#77
 Carbazole
 Concen: 21.341 ng/ul
 RT: 17.874 min Scan# 2463
 Delta R.T. -0.000 min
 Lab File: BM037731.D
 Acq: 26 Nov 2022 13:40




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020055


Tgt Ion:167 Resp: 1700569
 Ion Ratio Lower Upper
 167 100
 166 22.9 17.5 26.3
 139 14.1 10.9 16.3

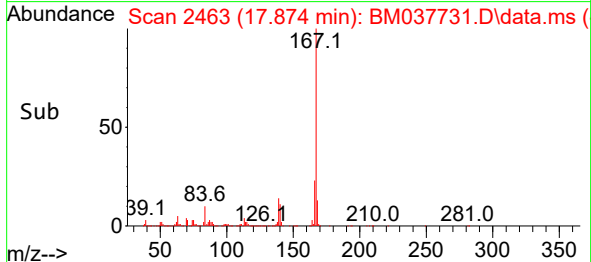

#78
 Di-n-butylphthalate
 Concen: 19.027 ng/ul
 RT: 18.427 min Scan# 2557
 Delta R.T. -0.006 min
 Lab File: BM037731.D
 Acq: 26 Nov 2022 13:40

Tgt Ion:149 Resp: 2194733
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.4 11.0
 104 6.2 4.4 6.6




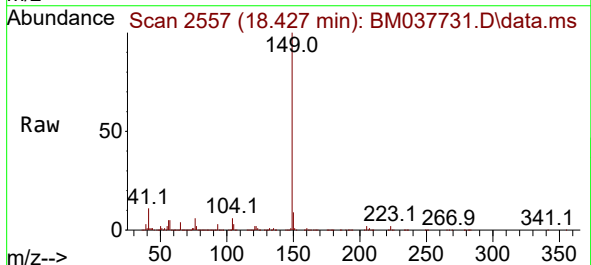




#80
Fluoranthene
Concen: 22.591 ng/ul
RT: 19.515 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:202 Resp: 1921701
Ion Ratio Lower Upper
202 100
101 14.3 10.6 16.0
100 11.2 8.2 12.4

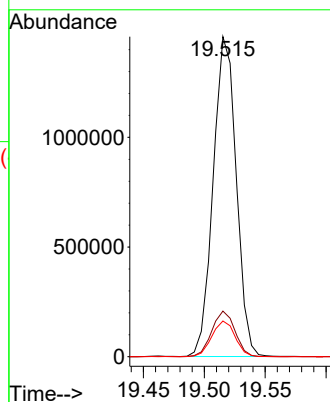

#82
Pyrene
Concen: 22.865 ng/ul
RT: 19.880 min Scan# 2804
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:202 Resp: 2054291
Ion Ratio Lower Upper
202 100
101 15.6 12.2 18.4
100 13.1 10.2 15.2



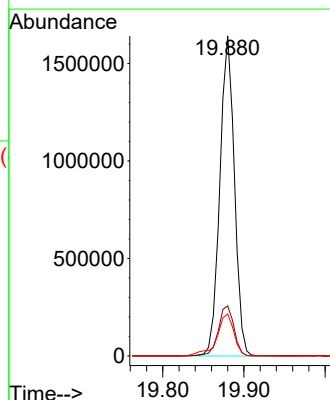





#83
Butylbenzylphthalate
Concen: 24.078 ng/ul
RT: 20.762 min Scan# 2954
Delta R.T. -0.000 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:149 Resp: 1007760
Ion Ratio Lower Upper
149 100
91 82.4 65.9 98.9
206 16.0 13.4 20.2

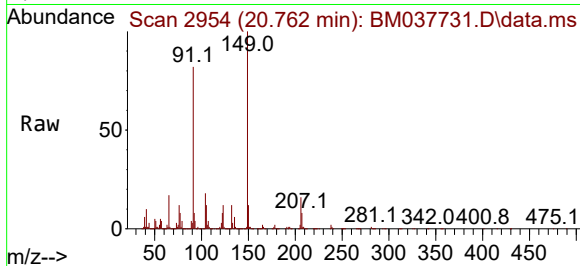

#84
3,3'-Dichlorobenzidine
Concen: 19.652 ng/ul
RT: 21.545 min Scan# 3087
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:252 Resp: 517191
Ion Ratio Lower Upper
252 100
254 63.8 51.0 76.4
126 16.7 12.2 18.4




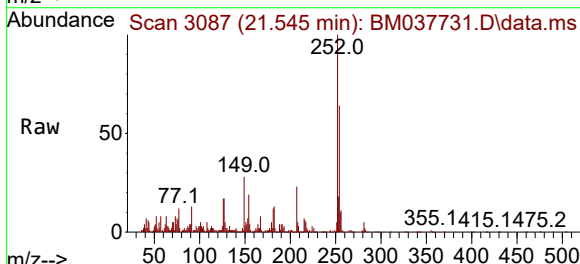




#85
Benzo(a)anthracene
Concen: 21.253 ng/ul
RT: 21.621 min Scan# 3100
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:228 Resp: 1863128
Ion Ratio Lower Upper
228 100
229 19.4 15.6 23.4
226 28.1 22.2 33.2

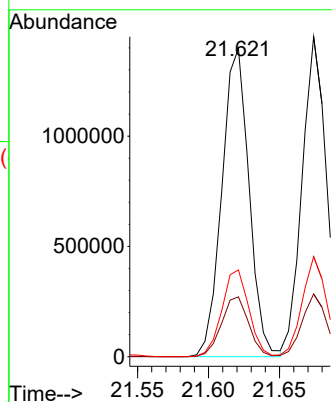

#86
Bis(2-ethylhexyl)phthalate
Concen: 23.238 ng/ul
RT: 21.527 min Scan# 3084
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:149 Resp: 1469460
Ion Ratio Lower Upper
149 100
167 24.5 20.2 30.4
279 2.9 2.2 3.4





#87

Chrysene

Concen: 21.023 ng/ul

RT: 21.674 min Scan# 3109

Delta R.T. -0.006 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :

SSTD020055





Tgt Ion:228 Resp: 1734305

Ion Ratio Lower Upper

228 100

226 31.3 24.2 36.4

229 19.6 16.1 24.1

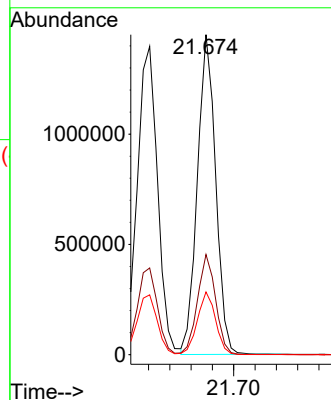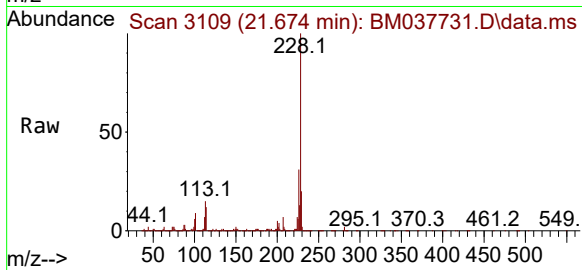

#89

Di-n-octyl phthalate

Concen: 24.185 ng/ul




RT: 22.480 min Scan# 3246


Delta R.T. -0.012 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Tgt Ion:149 Resp: 2511756



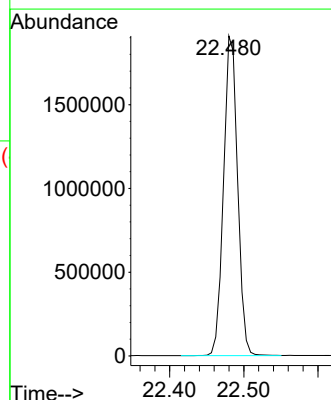
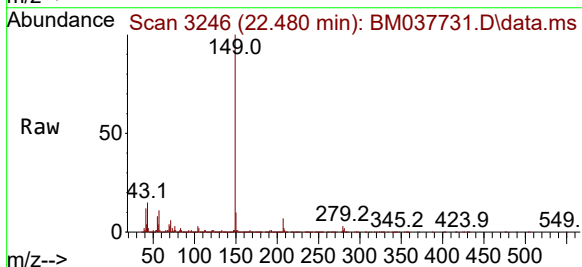




#90
Benzo(b)fluoranthene
Concen: 21.119 ng/ul
RT: 23.362 min Scan# 31
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:252 Resp: 1745498
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 13.9 11.0 16.4



#91
Benzo(k)fluoranthene
Concen: 21.151 ng/ul
RT: 23.409 min Scan# 3404
Delta R.T. -0.012 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:252 Resp: 1704765
Ion Ratio Lower Upper
252 100
253 22.1 17.5 26.3
125 14.3 10.6 16.0









#93
Benzo(a)pyrene
Concen: 20.963 ng/ul
RT: 24.015 min Scan# 31
Delta R.T. -0.006 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40




Instrument :
BNA_M
ClientSampleId :
SSTD020055


Tgt Ion:252 Resp: 1505888
Ion Ratio Lower Upper
252 100
253 21.3 17.3 25.9
125 15.1 12.0 18.0



#94
Indeno(1,2,3-cd)pyrene
Concen: 19.375 ng/ul
RT: 26.732 min Scan# 3969
Delta R.T. -0.012 min
Lab File: BM037731.D
Acq: 26 Nov 2022 13:40

Tgt Ion:276 Resp: 1596744
Ion Ratio Lower Upper
276 100
138 33.1 26.9 40.3
277 25.2 19.9 29.9





#95

Dibenzo(a,h)anthracene

Concen: 19.390 ng/ul

RT: 26.750 min Scan# 3972

Delta R.T. -0.012 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Instrument :

BNA_M

ClientSampleId :

SSTD020055





Tgt Ion:278 Resp: 1434743

Ion Ratio Lower Upper

278 100

139 21.9 16.6 25.0

279 23.1 19.3 28.9

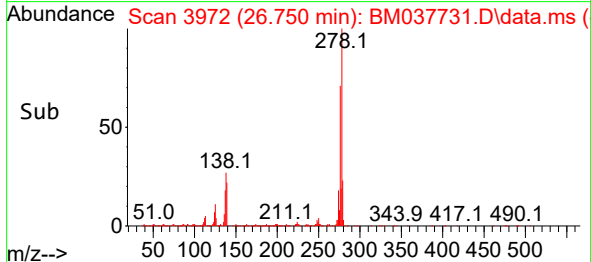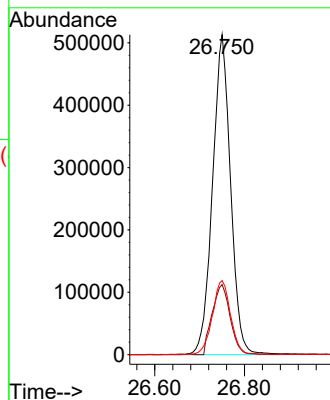

#96

Benzo(g,h,i)perylene

Concen: 19.507 ng/ul

RT: 27.538 min Scan# 4106

Delta R.T. -0.012 min

Lab File: BM037731.D

Acq: 26 Nov 2022 13:40

Tgt Ion:276 Resp: 1399875

Ion Ratio Lower Upper

276 100

138 29.2 23.4 35.2

277 23.4 19.1 28.7

