

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037736.D
 Acq On : 26 Nov 2022 16:52
 Operator : CG/JU
 Sample : N5602-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG5

Quant Time: Nov 27 21:29:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	173661	20.000	ng/ul	0.00
20) Naphthalene-d8	10.934	136	831931	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.734	164	547883	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.475	188	1136949	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.633	240	1121398	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1039486	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	25608	6.115	ng/uL	0.00
4) Pyridine-d5	3.875	84	125100	9.178	ng/ul	0.00
7) Phenol-d5	7.258	99	185723	10.720	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	458283	39.653	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	416603	34.605	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	323393	23.457	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	287313	44.053	ng/ul	0.00
24) 2-Nitrophenol-d4	10.010	143	287231	44.695	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	476292	40.500	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	511522	26.212	ng/ul	-0.01
46) Dimethylphthalate-d6	14.139	166	1800721	46.401	ng/ul	0.00
49) Acenaphthylene-d8	14.434	160	2061271	45.000	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	86471	10.116	ng/ul	-0.01
60) Fluorene-d10	15.722	176	1582826	46.570	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.833	200	245306	40.108	ng/ul	0.00
73) Anthracene-d10	17.575	188	2567973	48.299	ng/ul	0.00
81) Pyrene-d10	19.851	212	2993897	52.537	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2610350	48.787	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.145	165	12733	1.599	ng/ul#	Qvalue 31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037736.D
Acq On : 26 Nov 2022 16:52
Operator : CG/JU
Sample : N5602-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG5

Quant Time: Nov 27 21:29:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration

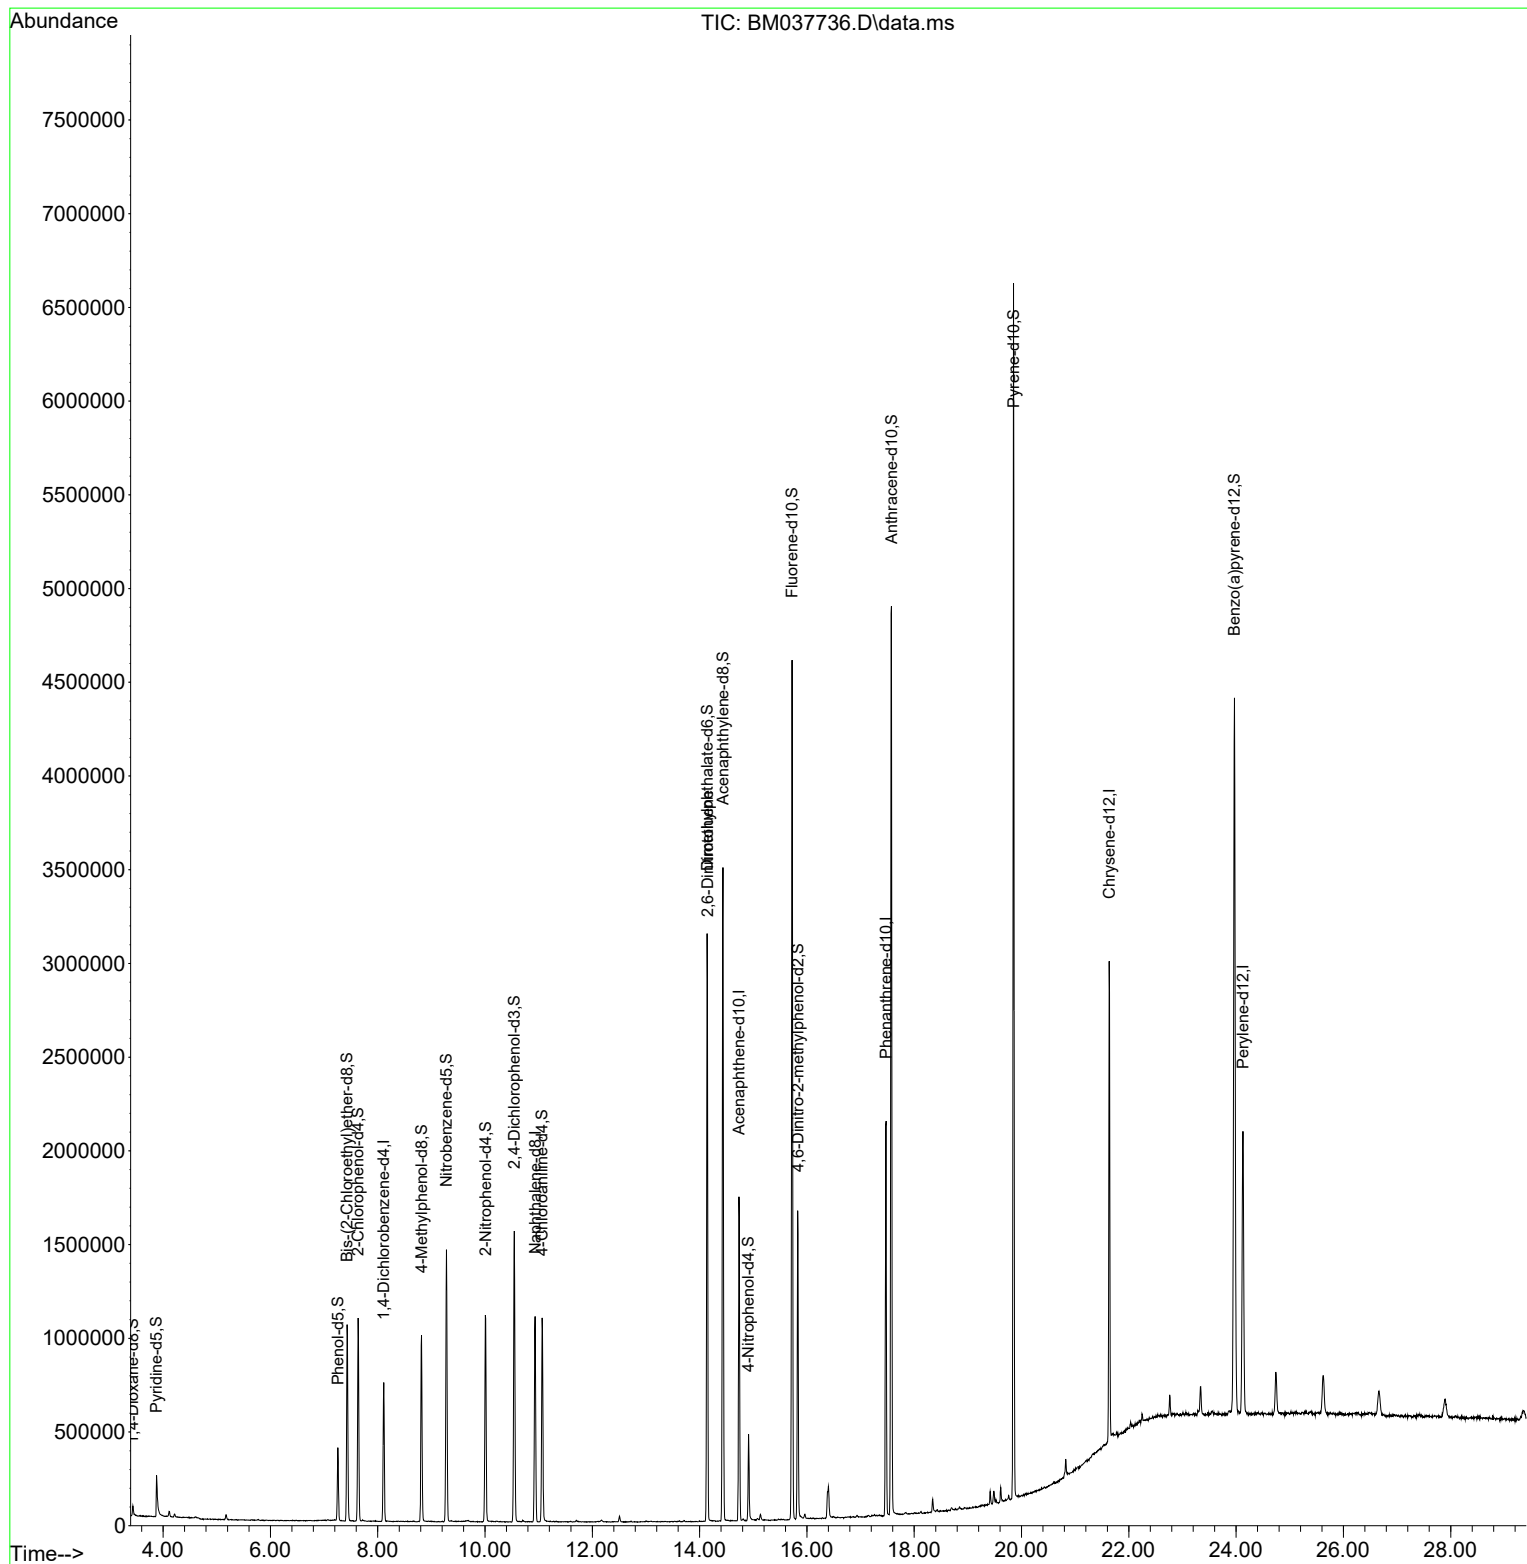

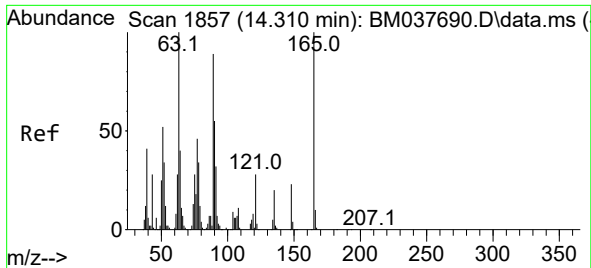

#48
 2,6-Dinitrotoluene
 Concen: 1.599 ng/ul
 RT: 14.145 min Scan# 11
 Delta R.T. -0.170 min
 Lab File: BM037736.D
 Acq: 26 Nov 2022 16:52

Instrument :
 BNA_M
 ClientSampleId :
 C0AG5

Tgt Ion:165 Resp: 12733
 Ion Ratio Lower Upper
 165 100
 89 0.0 56.4 84.6#
 121 33.6 18.9 28.3#

