

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037744.D
 Acq On : 26 Nov 2022 21:47
 Operator : CG/JU
 Sample : N5694-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHB38

Quant Time: Nov 27 21:30:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	245940	20.000	ng/ul	0.00
20) Naphthalene-d8	10.933	136	1110821	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.733	164	732373	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.468	188	1536513	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1478190	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1284098	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	26785	4.517	ng/uL	0.00
4) Pyridine-d5	3.881	84	147555	7.644	ng/ul	0.01
7) Phenol-d5	7.257	99	312211	12.724	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	487844	29.806	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	447714	26.260	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	392620	20.109	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	312826	35.923	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	175551	20.459	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.545	165	467041	29.743	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	809729	31.075	ng/ul	-0.01
46) Dimethylphthalate-d6	14.139	166	2084887	40.190	ng/ul	0.00
49) Acenaphthylene-d8	14.433	160	2332751	38.098	ng/ul	0.00
54) 4-Nitrophenol-d4	14.915	143	93923	8.220	ng/ul	0.00
60) Fluorene-d10	15.721	176	1866346	41.079	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	22003	2.662	ng/ul	-0.01
73) Anthracene-d10	17.568	188	3170832	44.130	ng/ul	0.00
81) Pyrene-d10	19.850	212	3613634	48.106	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2924087	44.240	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.198	107	36331	1.769	ng/ul	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037744.D
Acq On : 26 Nov 2022 21:47
Operator : CG/JU
Sample : N5694-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHB38

Quant Time: Nov 27 21:30:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration

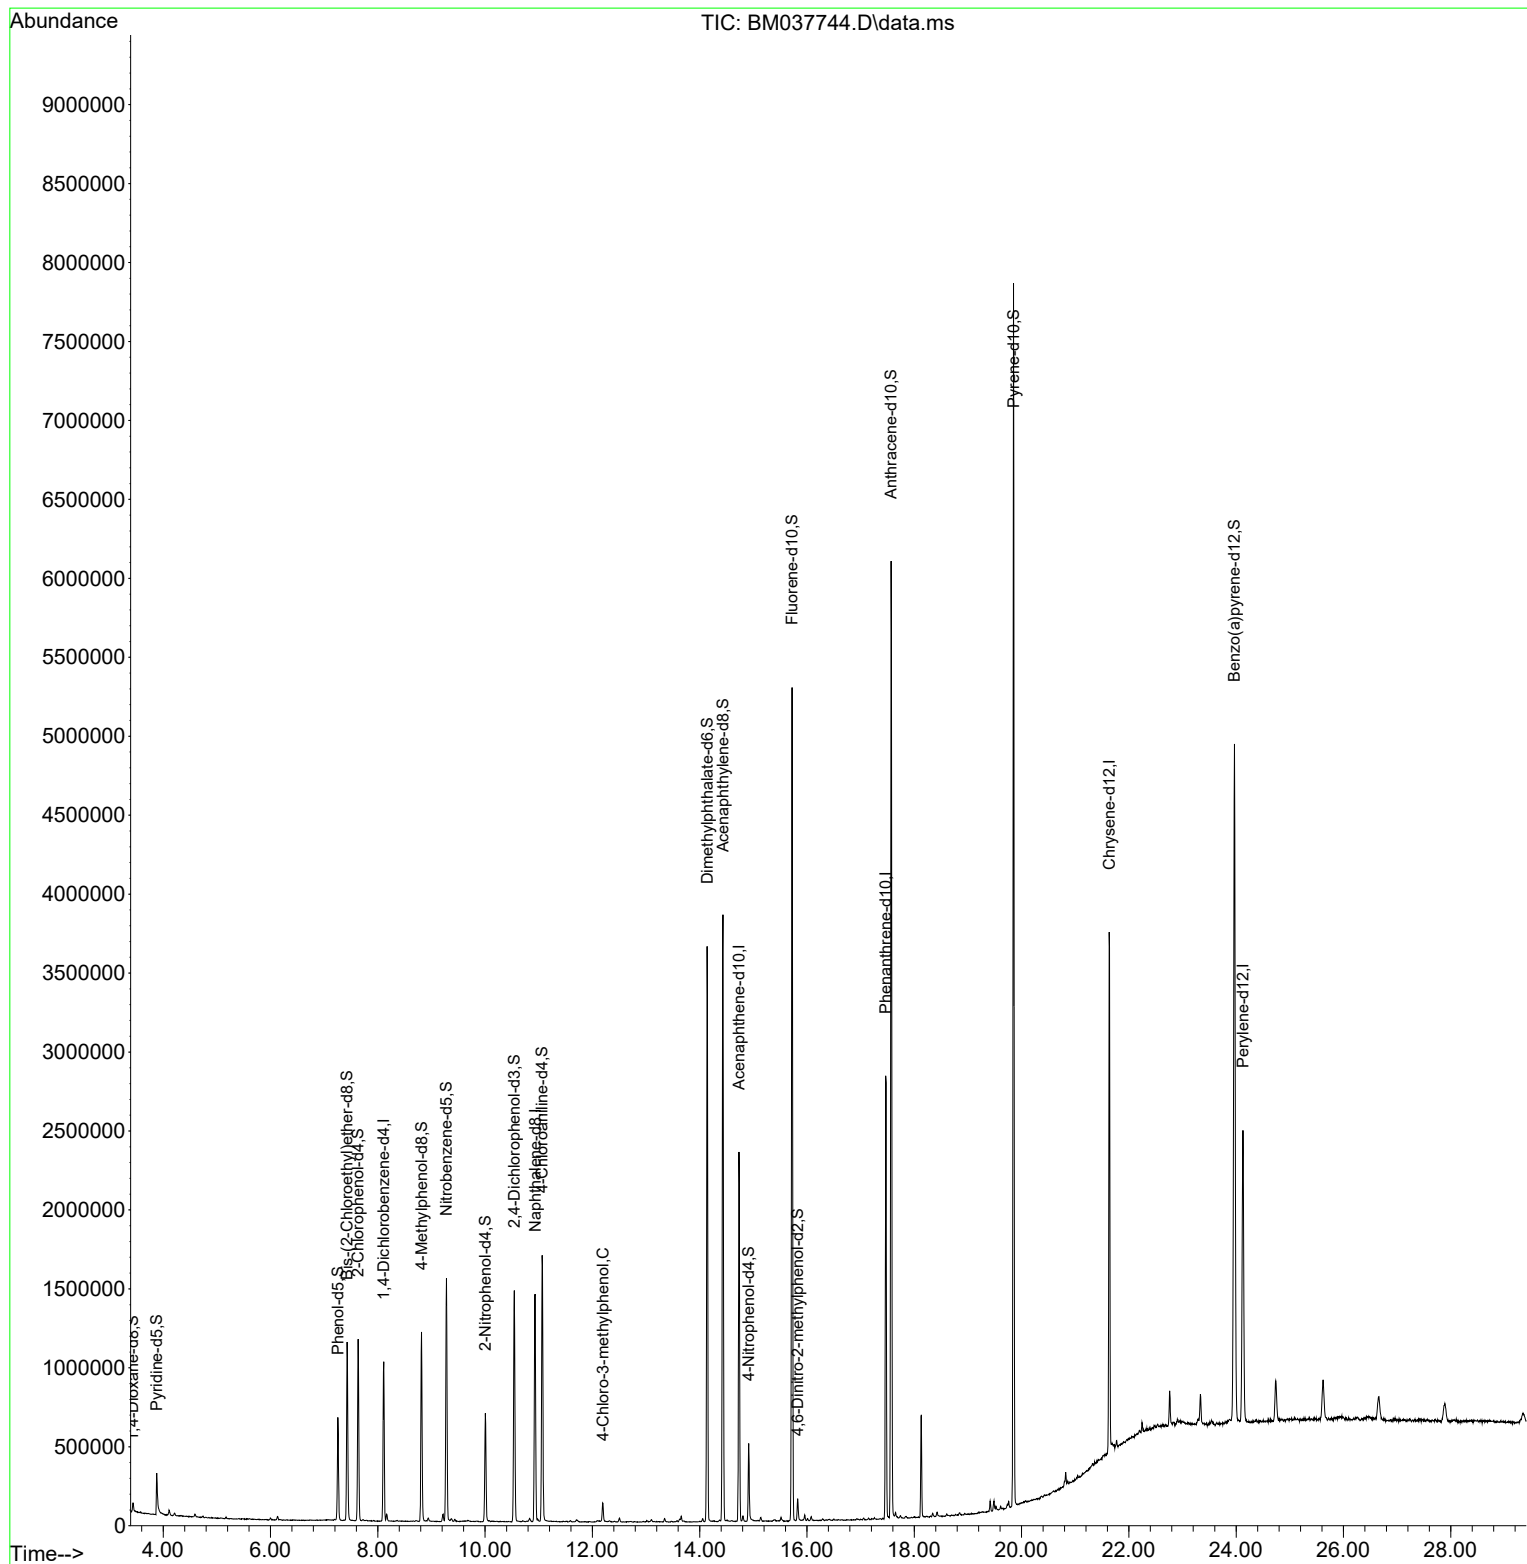

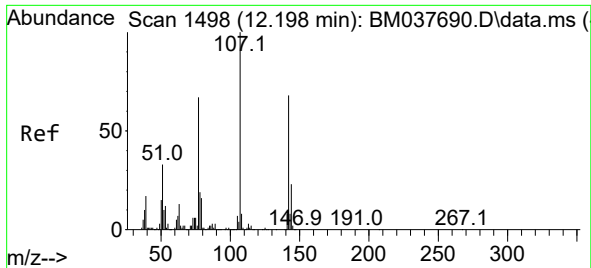

#35
 4-Chloro-3-methylphenol
 Concen: 1.769 ng/ul
 RT: 12.198 min Scan# 1498
 Delta R.T. -0.006 min
 Lab File: BM037744.D
 Acq: 26 Nov 2022 21:47

Instrument :
 BNA_M
 ClientSampleId :
 BHB38

Tgt Ion:107 Resp: 36331
 Ion Ratio Lower Upper
 107 100
 144 21.4 20.2 30.4
 142 68.5 62.6 93.8

