

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037745.D
 Acq On : 26 Nov 2022 22:23
 Operator : CG/JU
 Sample : N5694-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHB39

Quant Time: Nov 27 21:30:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	222340	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	1023839	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.733	164	682044	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.468	188	1403257	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1312823	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1167760	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	21222	3.958	ng/uL	0.00
4) Pyridine-d5	3.881	84	112451	6.444	ng/ul	0.01
7) Phenol-d5	7.257	99	263878	11.896	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	446338	30.164	ng/ul	0.00
11) 2-Chlorophenol-d4	7.634	132	411960	26.727	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	344445	19.514	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	282918	35.248	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	200825	25.393	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.545	165	458124	31.653	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	718230	29.905	ng/ul	-0.01
46) Dimethylphthalate-d6	14.139	166	1789022	37.032	ng/ul	0.00
49) Acenaphthylene-d8	14.427	160	2037826	35.737	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.916	143	64670	6.077	ng/ul	0.00
60) Fluorene-d10	15.721	176	1581845	37.386	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	21585	2.859	ng/ul	-0.01
73) Anthracene-d10	17.568	188	2726697	41.552	ng/ul	0.00
81) Pyrene-d10	19.851	212	2992384	44.854	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	2482679	41.304	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.192	107	33190	1.754	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037745.D
Acq On : 26 Nov 2022 22:23
Operator : CG/JU
Sample : N5694-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHB39

Quant Time: Nov 27 21:30:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration

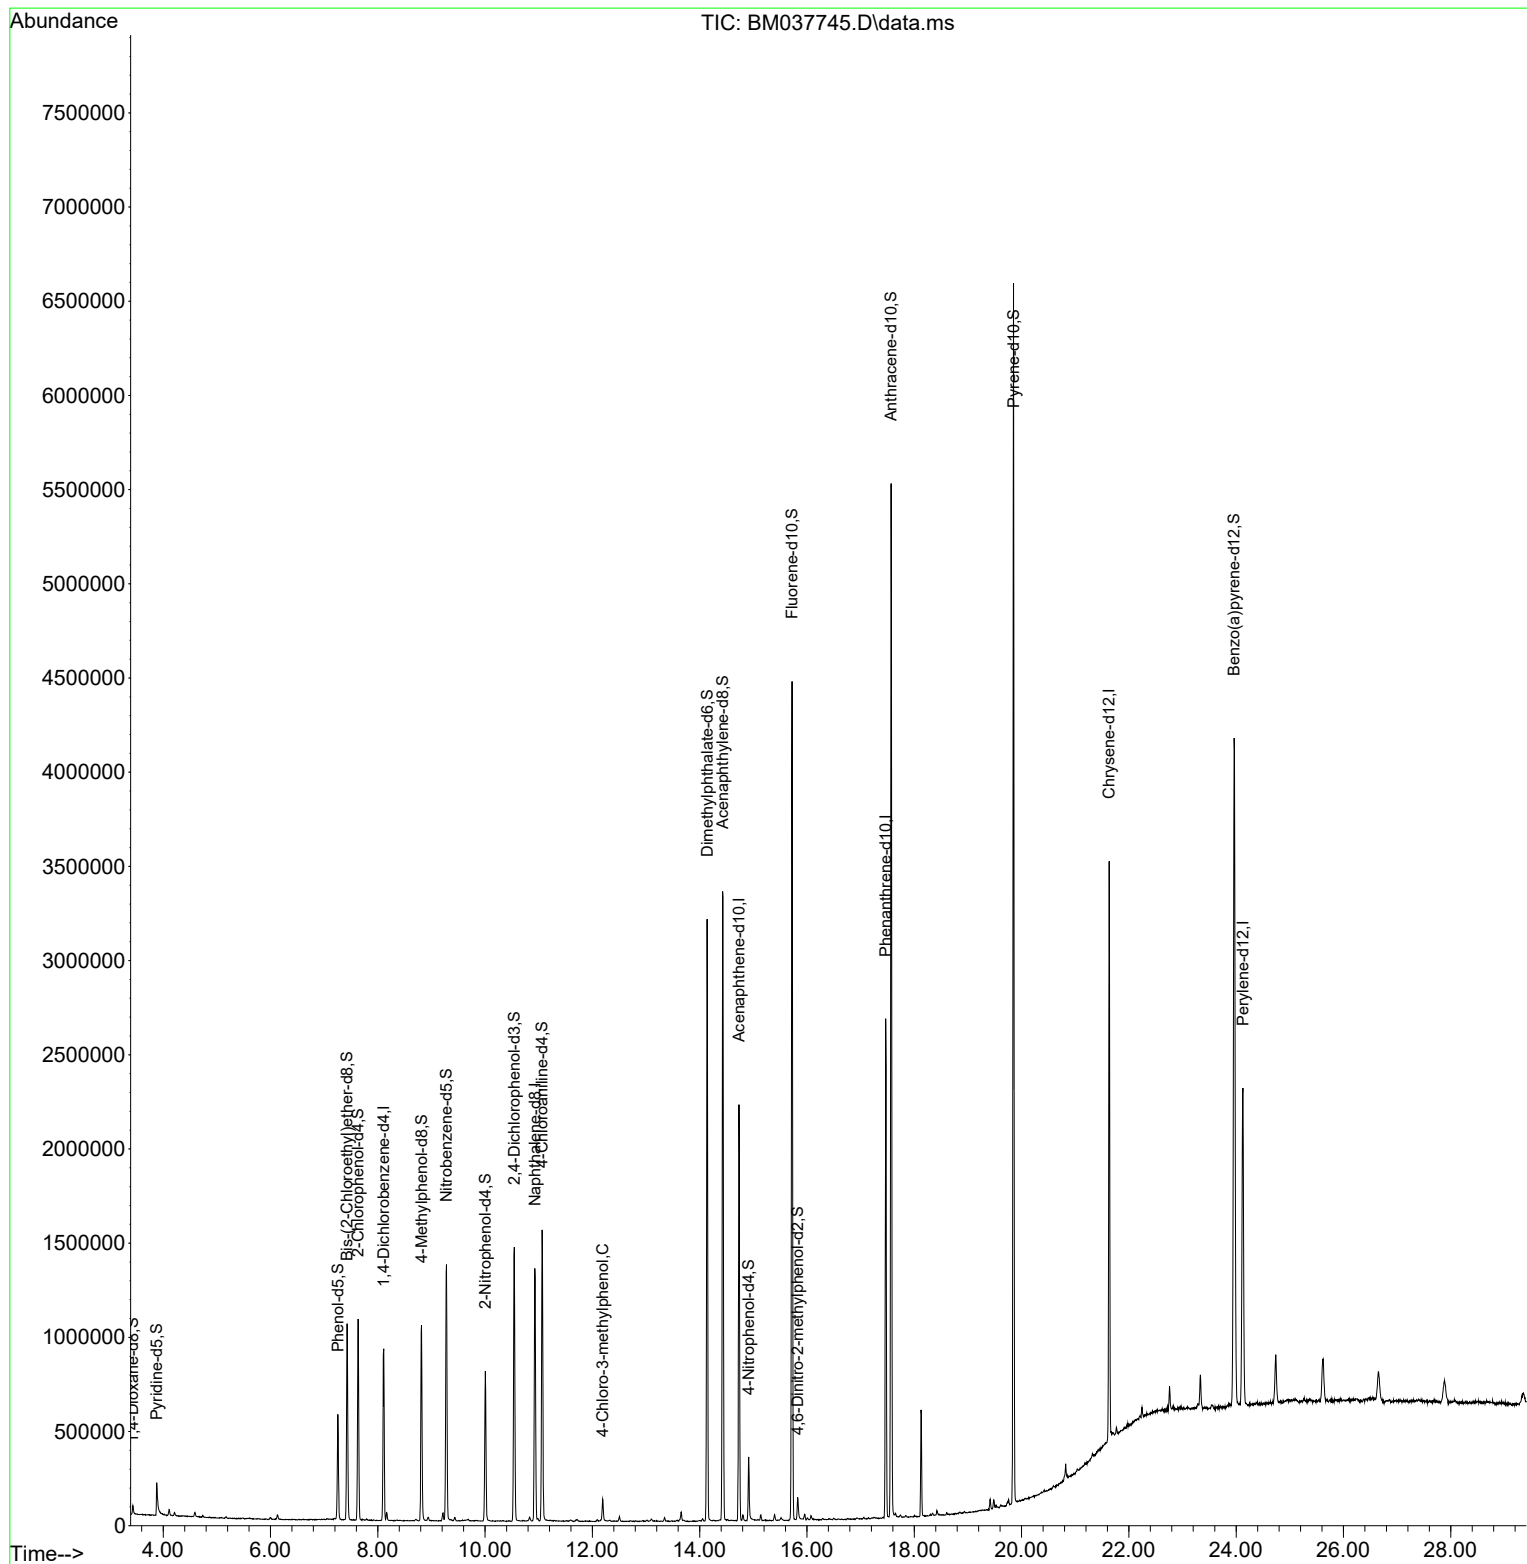

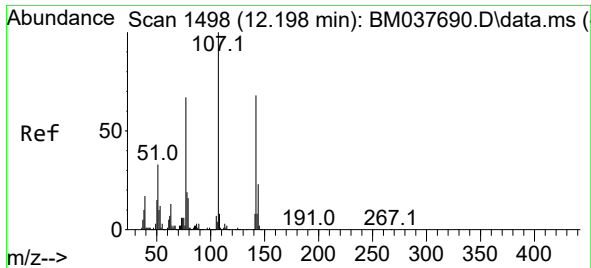

#35
 4-Chloro-3-methylphenol
 Concen: 1.754 ng/ul
 RT: 12.192 min Scan# 14
 Delta R.T. -0.012 min
 Lab File: BM037745.D
 Acq: 26 Nov 2022 22:23

Instrument :
 BNA_M
 ClientSampleId :
 BHB39

Tgt Ion:	107	Resp:	33190
Ion	Ratio	Lower	Upper
107	100		
144	27.8	20.2	30.4
142	81.3	62.6	93.8

