

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037748.D
 Acq On : 27 Nov 2022 00:13
 Operator : CG/JU
 Sample : N5694-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHB42

Quant Time: Nov 27 21:31:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	224217	20.000	ng/u1	0.00
20) Naphthalene-d8	10.927	136	1046759	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.733	164	684276	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.468	188	1555368	20.000	ng/u1	0.00
79) Chrysene-d12	21.633	240	1510690	20.000	ng/u1	# 0.00
88) Perylene-d12	24.127	264	1336952	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	25041	4.632	ng/uL	0.00
4) Pyridine-d5	3.875	84	192971	10.965	ng/u1	0.00
7) Phenol-d5	7.257	99	193193	8.637	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	456405	30.586	ng/u1	0.00
11) 2-Chlorophenol-d4	7.634	132	425089	27.348	ng/u1	0.00
15) 4-Methylphenol-d8	8.816	113	333472	18.734	ng/u1	0.00
21) Nitrobenzene-d5	9.281	128	285933	34.844	ng/u1	0.00
24) 2-Nitrophenol-d4	10.004	143	280959	34.747	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.545	165	488000	32.979	ng/u1	0.00
31) 4-Chloroaniline-d4	11.063	131	511482	20.831	ng/u1	-0.01
46) Dimethylphthalate-d6	14.139	166	1734489	35.786	ng/u1	0.00
49) Acenaphthylene-d8	14.427	160	1986747	34.727	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.921	143	89280	8.363	ng/u1	0.00
60) Fluorene-d10	15.721	176	1583973	37.315	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	243825	29.141	ng/u1	-0.01
73) Anthracene-d10	17.568	188	2778529	38.201	ng/u1	0.00
81) Pyrene-d10	19.850	212	3288042	42.830	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.962	264	2648512	38.487	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.469	88	45160	7.598	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037748.D
Acq On : 27 Nov 2022 00:13
Operator : CG/JU
Sample : N5694-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHB42

Quant Time: Nov 27 21:31:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration

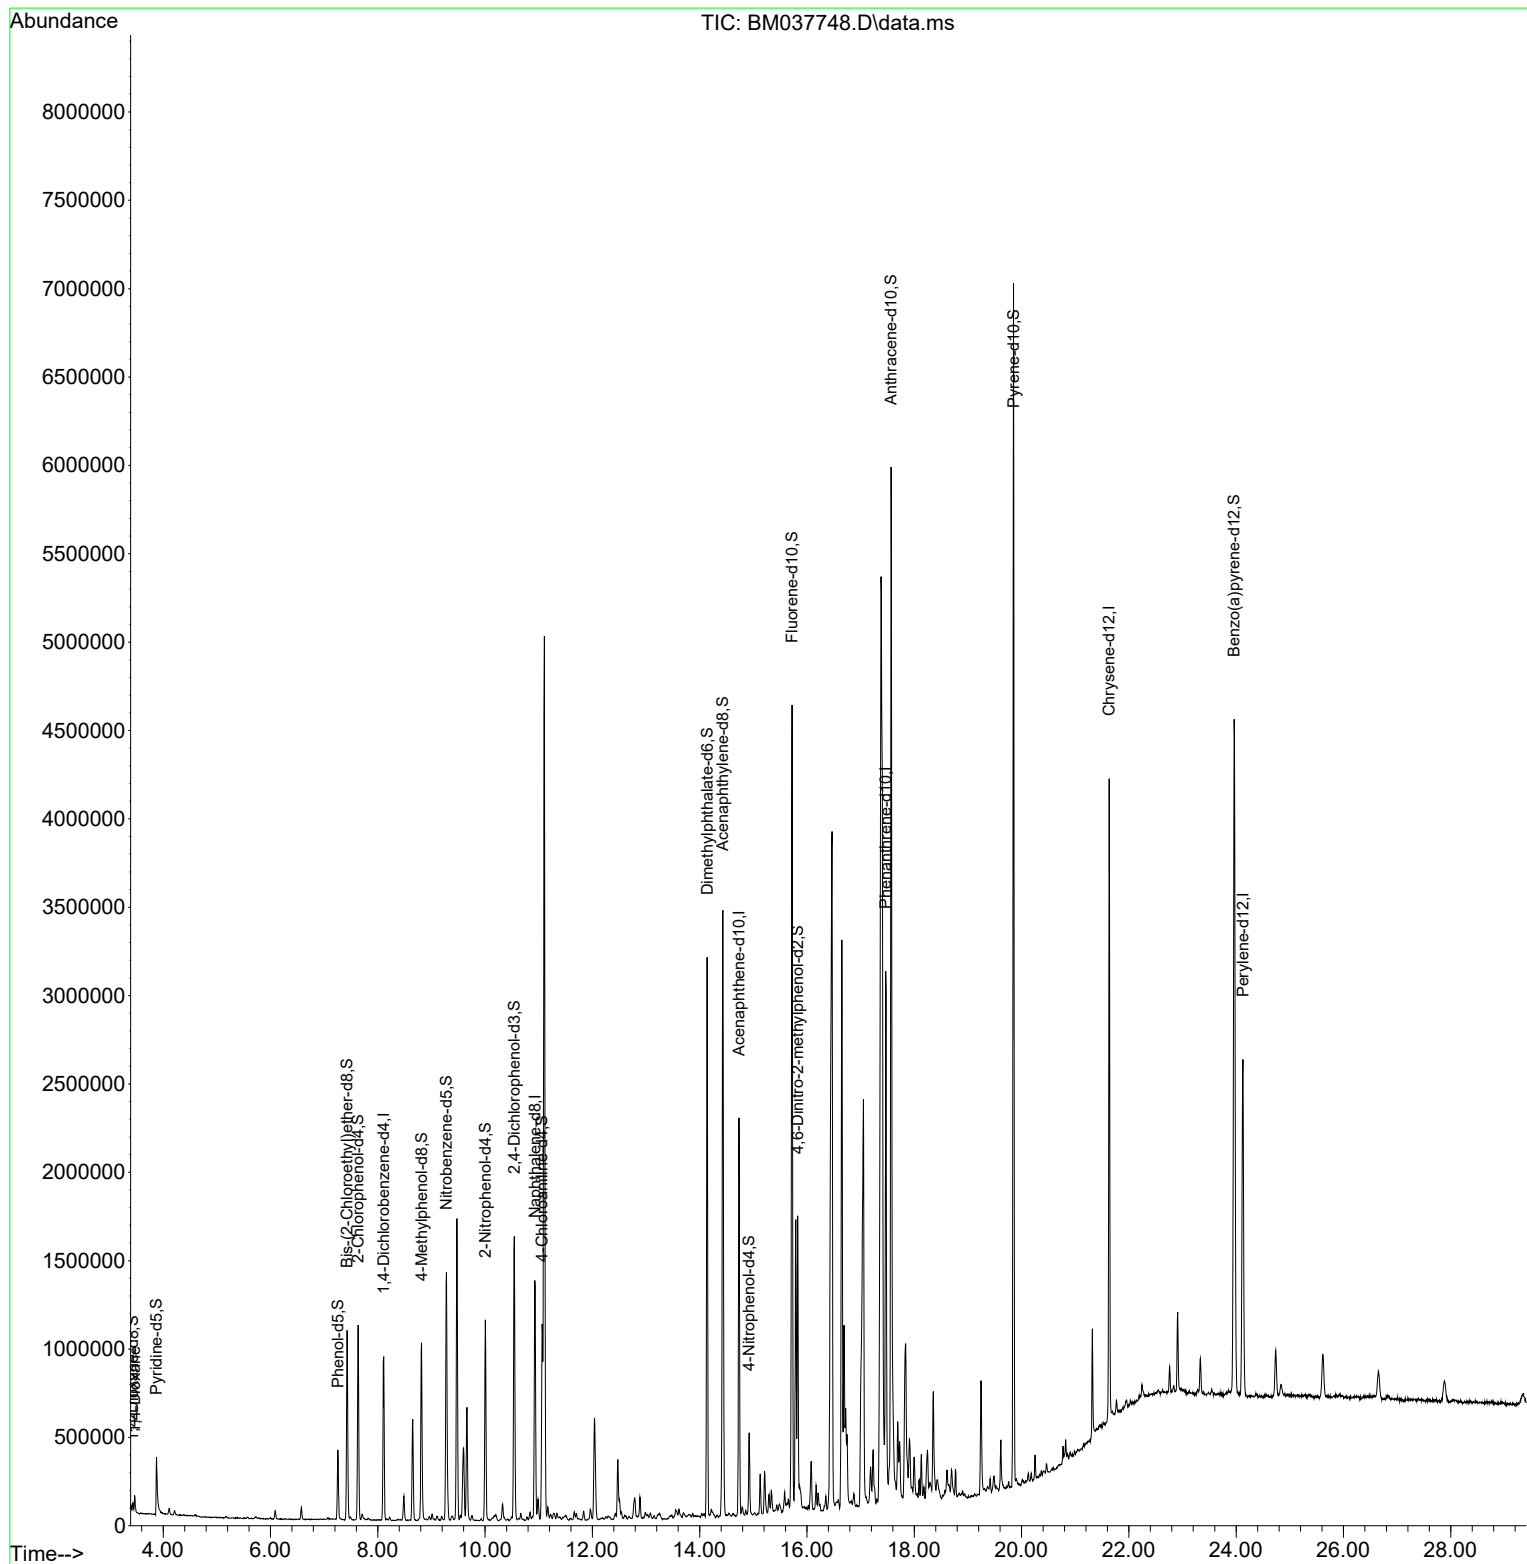

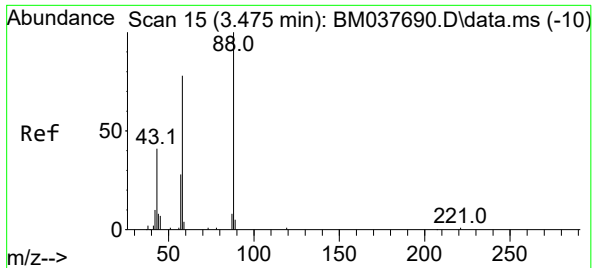

1,4-Dioxane
 Concen: 7.598 ng/uL
 RT: 3.469 min Scan# 14
 Delta R.T. -0.006 min
 Lab File: BM037748.D
 Acq: 27 Nov 2022 00:13

Instrument :
 BNA_M
 ClientSampleId :
 BHB42

Tgt Ion: 88	Resp: 45160
Ion Ratio	Lower Upper
88	100
43	44.0 42.8 64.2
58	85.6 62.6 94.0

