




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037715.D
 Acq On : 26 Nov 2022 03:14
 Operator : CG/JU
 Sample : N5591-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9826

Manual IntegrationsAPPROVED

Quant Time: Nov 26 04:28:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2022
 Supervised By :mohammad ahmed 11/28/2022

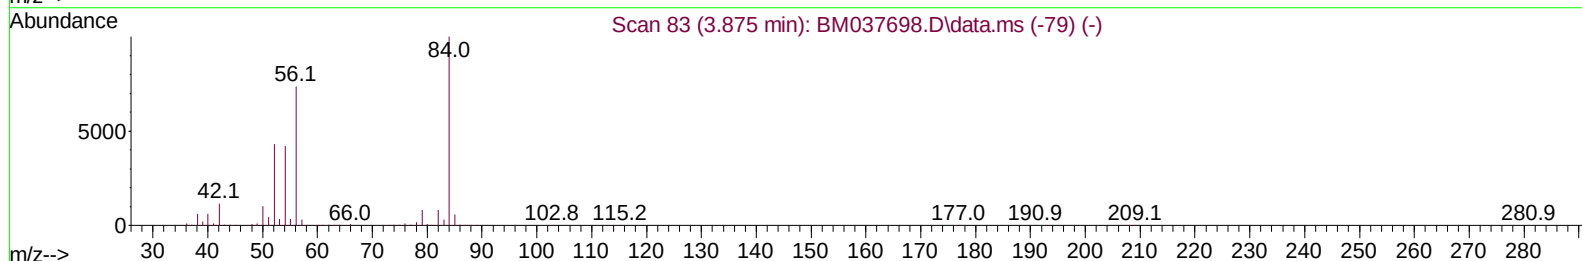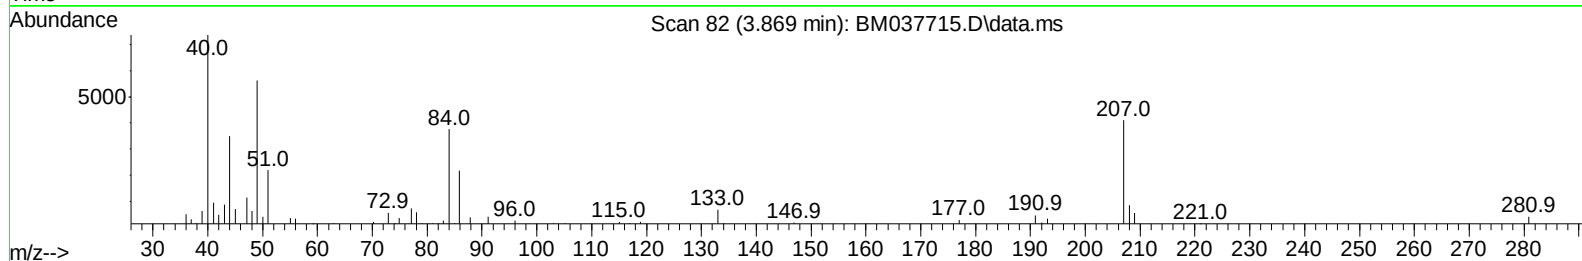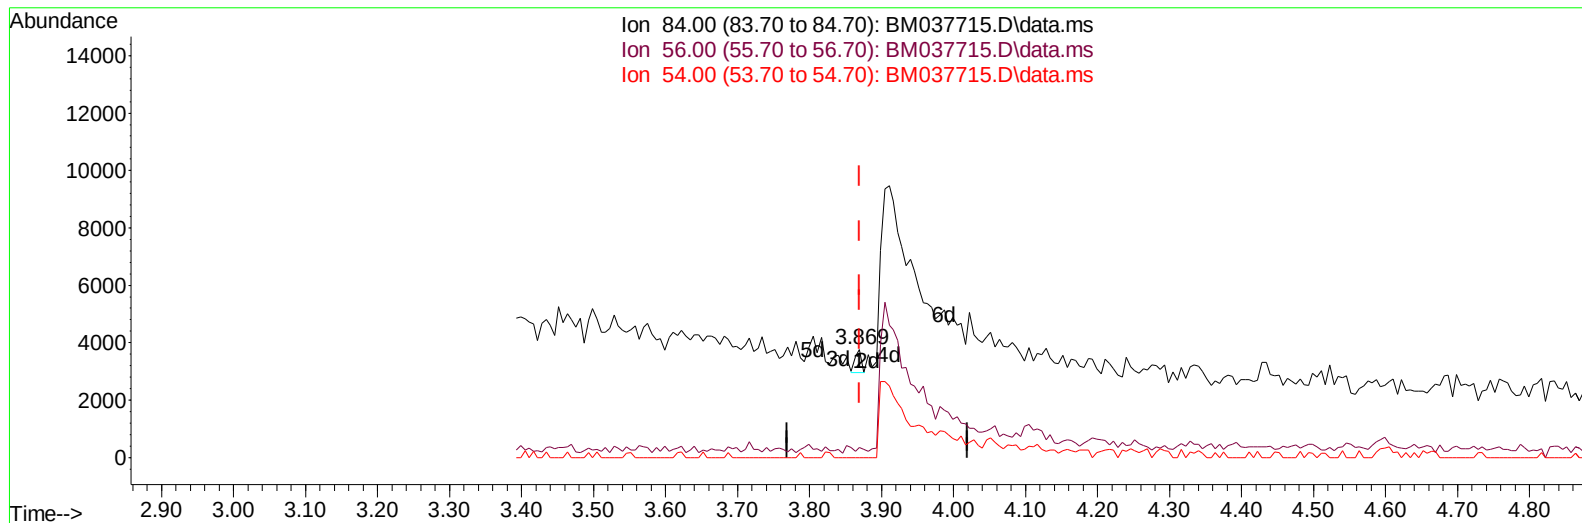

TIC: BM037715.D\data.ms

(4) Pyridine-d5 (S)

3.869min (0.000) 0.03 ng/u1

response 487

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	74.90	8.98#
54.00	37.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037715.D
 Acq On : 26 Nov 2022 03:14
 Operator : CG/JU
 Sample : N5591-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9826

Manual IntegrationsAPPROVED

Quant Time: Nov 26 04:28:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2022
 Supervised By :mohammad ahmed 11/28/2022

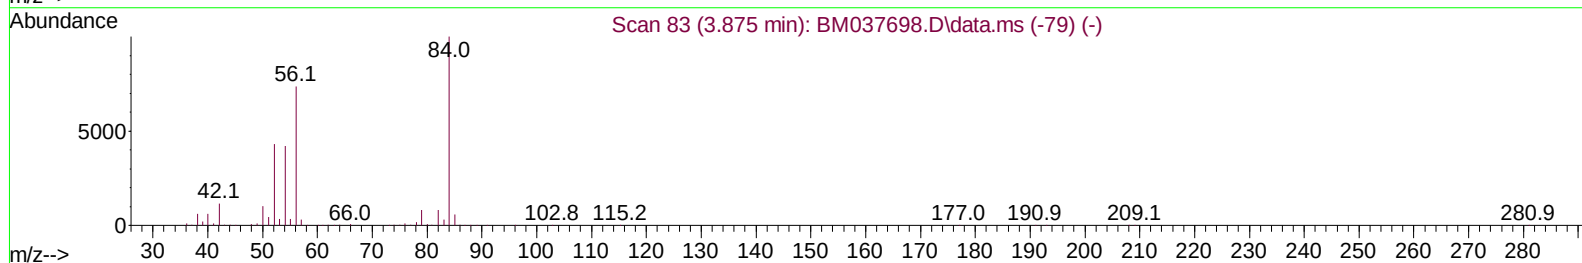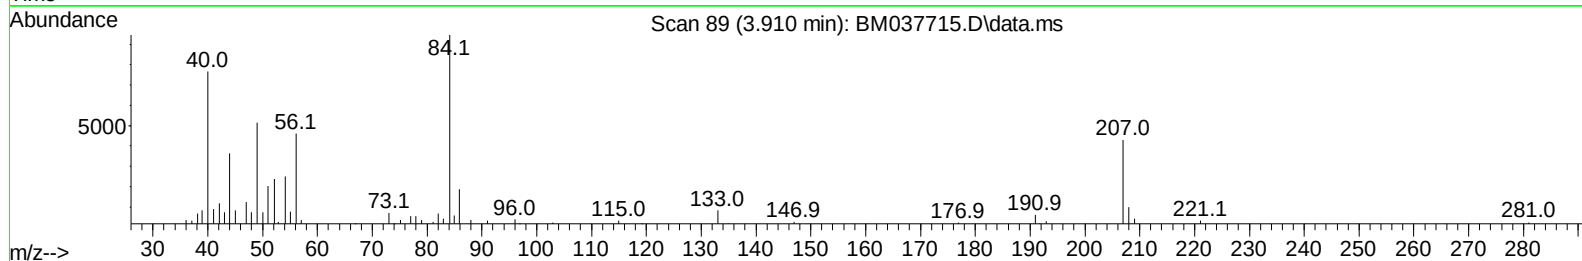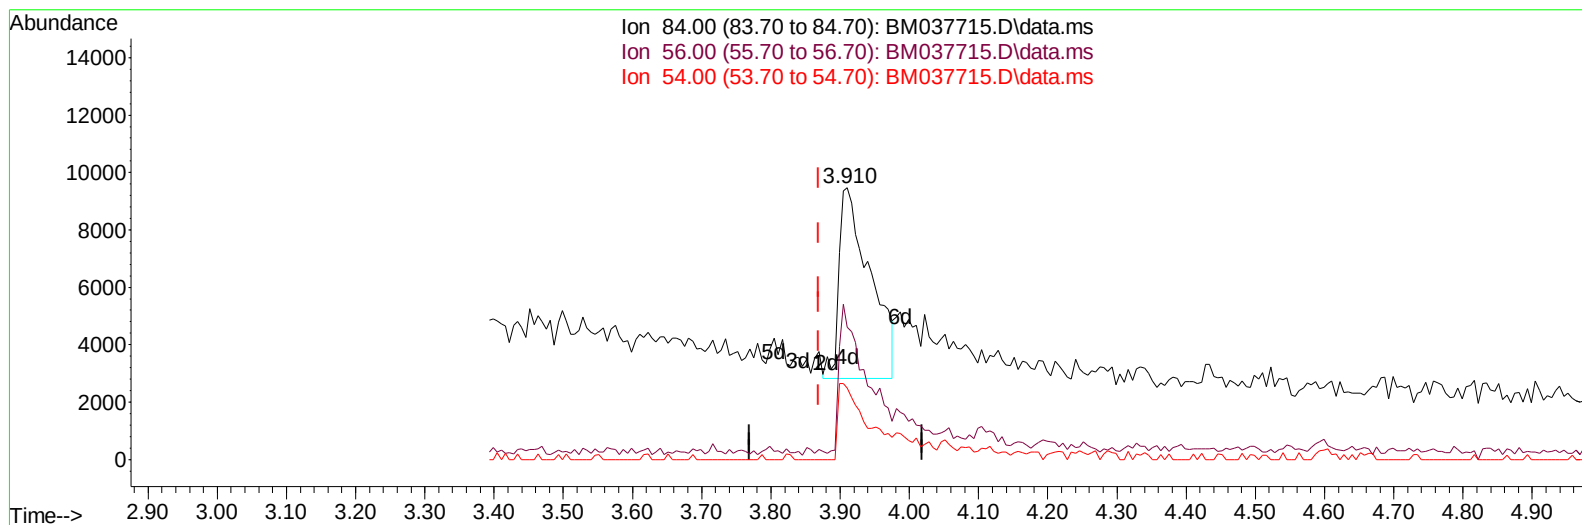

TIC: BM037715.D\data.ms

(4) Pyridine-d5 (S)

3.910min (+ 0.041) 1.42 ng/ul m

response 20835

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	74.90	48.60#
54.00	37.60	26.31#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037715.D
 Acq On : 26 Nov 2022 03:14
 Operator : CG/JU
 Sample : N5591-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9826

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2022
 Supervised By :mohammad ahmed 11/28/2022

Quant Time: Nov 26 04:28:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 24 01:27:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	187337	20.000	ng/ul	0.00
20) Naphthalene-d8	10.934	136	911912	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.739	164	569596	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.474	188	1160455	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	1124085	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	1079456	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	27650	6.121	ng/uL	0.00
4) Pyridine-d5	3.910	84	20835m	1.417	ng/ul	0.04
7) Phenol-d5	7.257	99	545002	29.161	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.434	67	397562	31.888	ng/ul	0.00
11) 2-Chlorophenol-d4	7.640	132	409386	31.523	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113	421046	28.310	ng/ul	0.00
21) Nitrobenzene-d5	9.281	128	216946	30.347	ng/ul	0.00
24) 2-Nitrophenol-d4	10.010	143	209849	29.790	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.545	165	365724	28.371	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131	560000	26.179	ng/ul	0.00
46) Dimethylphthalate-d6	14.145	166	1363193	33.788	ng/ul	0.00
49) Acenaphthylene-d8	14.433	160	1530085	32.130	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	259471	29.197	ng/ul	0.00
60) Fluorene-d10	15.721	176	1170777	33.134	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.833	200	153412	24.575	ng/ul	0.00
73) Anthracene-d10	17.574	188	1879496	34.634	ng/ul	0.00
81) Pyrene-d10	19.851	212	2214322	38.764	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	2045068	36.807	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037715.D
Acq On : 26 Nov 2022 03:14
Operator : CG/JU
Sample : N5591-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9826

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2022
Supervised By :mohammad ahmed 11/28/2022

Quant Time: Nov 26 04:28:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 24 01:27:15 2022
Response via : Initial Calibration

