

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM112522\  
 Data File : BM037746.D  
 Acq On : 26 Nov 2022 23:00  
 Operator : CG/JU  
 Sample : N5694-04  
 Misc :  
 ALS Vial : 58 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BHB40

Quant Time: Nov 27 21:30:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM112322.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Nov 24 01:27:15 2022  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	179920	20.000	ng/u1	0.00
20) Naphthalene-d8	10.927	136	841484	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.733	164	539563	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.468	188	1179214	20.000	ng/u1	0.00
79) Chrysene-d12	21.633	240	1210538	20.000	ng/u1	0.00
88) Perylene-d12	24.121	264	1101788	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	20643	4.758	ng/uL	0.00
4) Pyridine-d5	3.881	84	114589	8.115	ng/u1	0.01
7) Phenol-d5	7.257	99	134180	7.475	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	359207	29.999	ng/u1	0.00
11) 2-Chlorophenol-d4	7.634	132	323839	25.964	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	239205	16.747	ng/u1	-0.01
21) Nitrobenzene-d5	9.281	128	221760	33.616	ng/u1	0.00
24) 2-Nitrophenol-d4	10.004	143	216998	33.383	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.545	165	364805	30.668	ng/u1	0.00
31) 4-Chloroaniline-d4	11.063	131	458301	23.218	ng/u1	-0.01
46) Dimethylphthalate-d6	14.139	166	1339090	35.038	ng/u1	0.00
49) Acenaphthylene-d8	14.433	160	1514786	33.579	ng/u1	0.00
54) 4-Nitrophenol-d4	14.915	143	60403	7.175	ng/u1	0.00
60) Fluorene-d10	15.721	176	1180150	35.258	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.827	200	184917	29.151	ng/u1	-0.01
73) Anthracene-d10	17.568	188	2142776	38.858	ng/u1	0.00
81) Pyrene-d10	19.850	212	2528550	41.104	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.962	264	2251131	39.694	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.469	88	25610	5.369	ng/uL#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM112522\  
 Data File : BM037746.D  
 Acq On : 26 Nov 2022 23:00  
 Operator : CG/JU  
 Sample : N5694-04  
 Misc :  
 ALS Vial : 58 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BHB40

Quant Time: Nov 27 21:30:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM112322.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Nov 24 01:27:15 2022  
 Response via : Initial Calibration

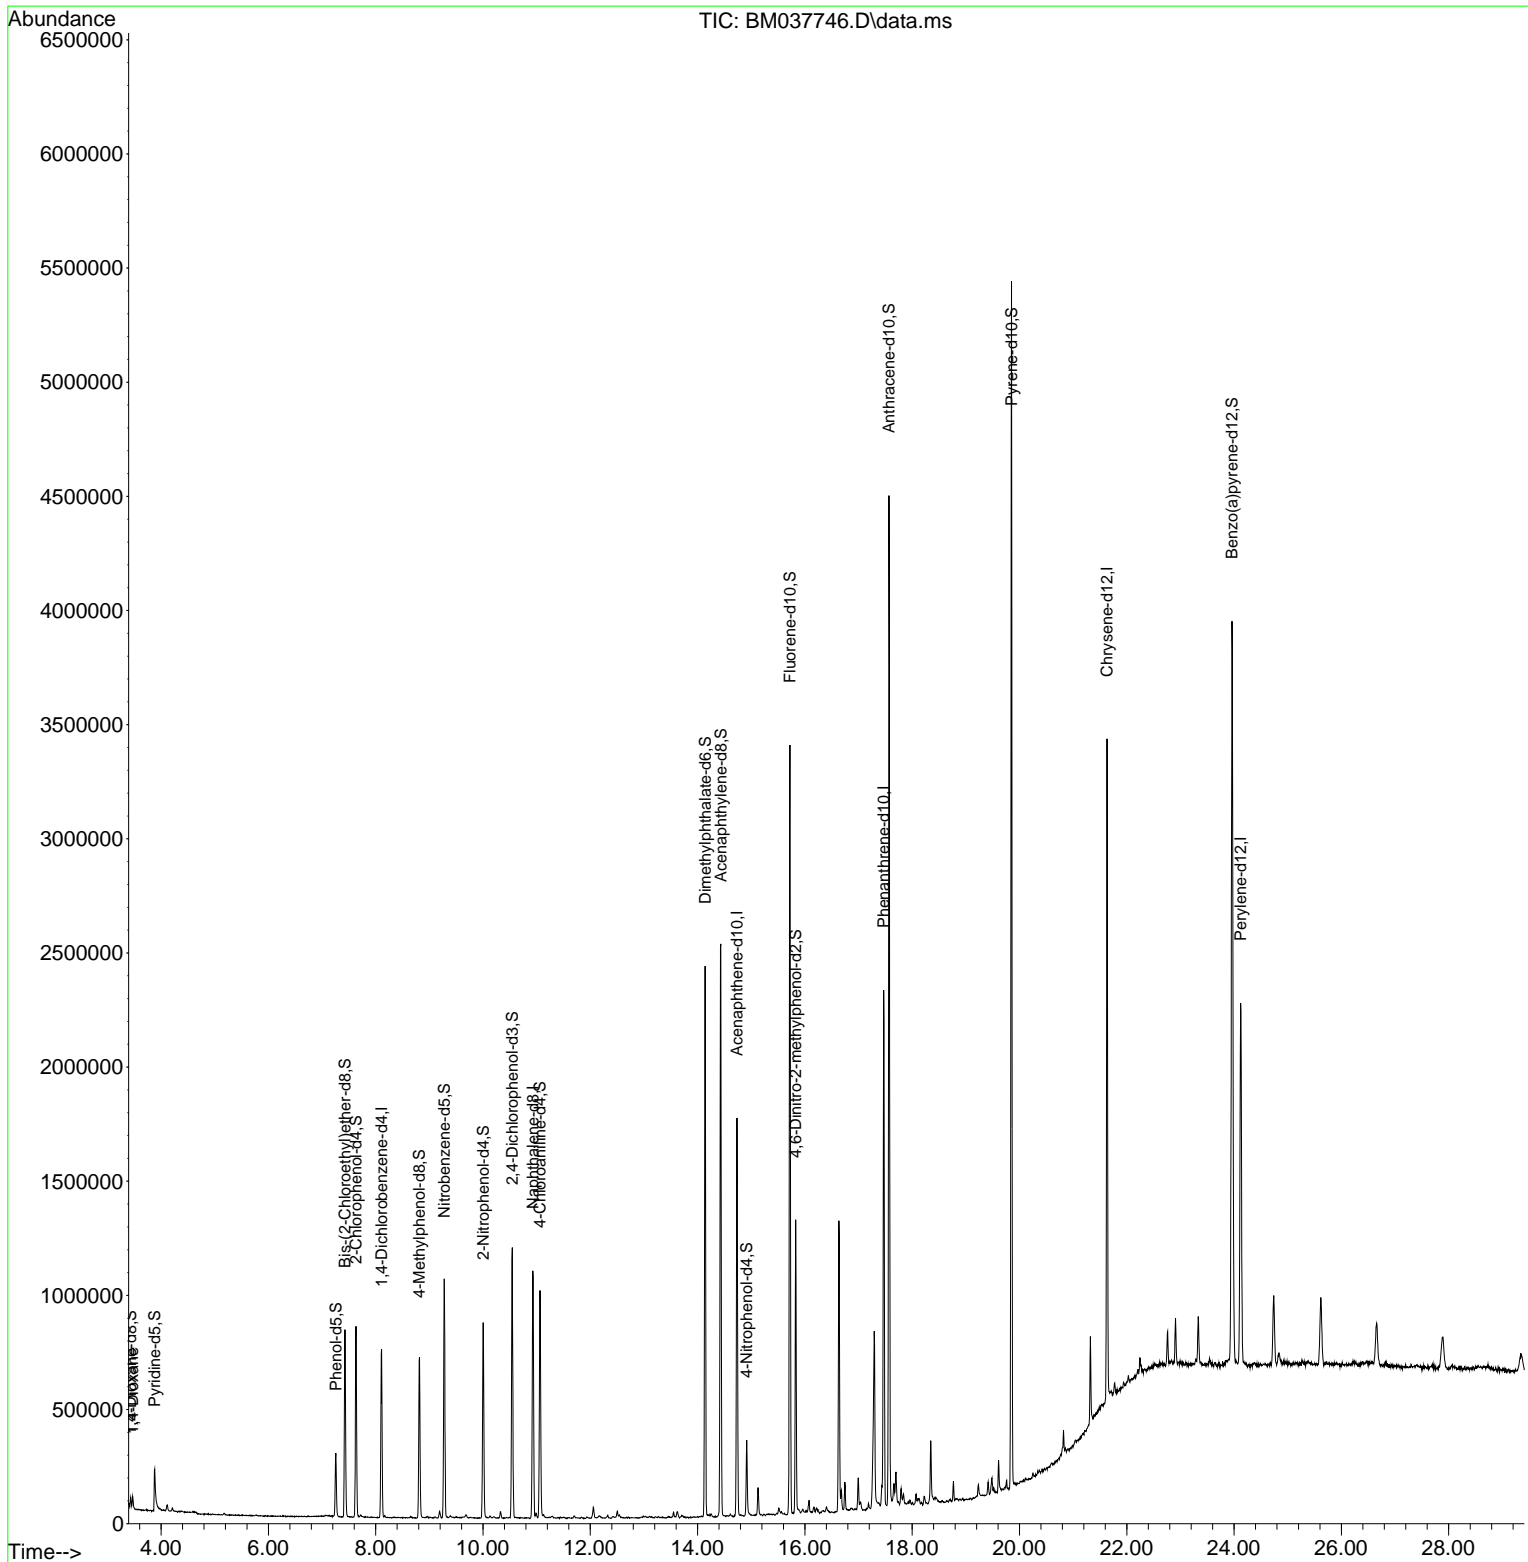

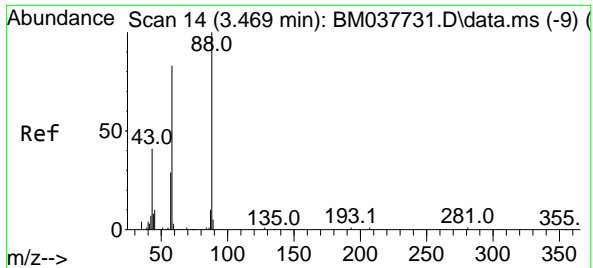

#2  
 1,4-Dioxane  
 Concen: 5.369 ng/uL  
 RT: 3.469 min Scan# 14  
 Delta R.T. -0.006 min  
 Lab File: BM037746.D  
 Acq: 26 Nov 2022 23:00

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BHB40

Tgt Ion	Resp	Lower	Upper
88	25610		
43	100	42.8	64.2#
58	79.2	62.6	94.0

