

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037691.D
 Acq On : 25 Nov 2022 10:48
 Operator : CG/JU
 Sample : PB149274BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	5	8	15	rBV	32054	44830	1.39%	0.128%
2	3.875	79	83	103	rBV	377273	681824	21.14%	1.948%
3	4.217	137	141	145	rBV4	9418	11970	0.37%	0.034%
4	4.699	218	223	225	rBV6	2993	4027	0.12%	0.012%
5	5.875	421	423	428	rBV6	1786	3695	0.11%	0.011%
6	7.081	625	628	630	rBV4	3856	4570	0.14%	0.013%
7	7.258	651	658	667	rBV	621154	953851	29.57%	2.725%
8	7.340	670	672	679	rVB6	3032	5014	0.16%	0.014%
9	7.434	679	688	697	rBV	452653	712903	22.10%	2.037%
10	7.640	716	723	730	rBV	571392	888298	27.54%	2.538%
11	8.116	797	804	812	rVB	457051	727871	22.57%	2.080%
12	8.816	916	923	934	rBV	697160	1092301	33.87%	3.121%
13	9.281	996	1002	1013	rVB	598142	966048	29.95%	2.760%
14	10.010	1117	1126	1137	rBV	476378	764208	23.69%	2.183%
15	10.546	1211	1217	1227	rBV	646944	1054557	32.70%	3.013%
16	10.846	1264	1268	1272	rBV7	2468	4342	0.13%	0.012%
17	10.934	1276	1283	1291	rVB	645915	1091059	33.83%	3.117%
18	11.069	1299	1306	1319	rBV	774899	1281895	39.75%	3.662%
19	12.510	1547	1551	1556	rVB2	11002	18055	0.56%	0.052%
20	13.092	1647	1650	1653	rBV5	2664	3885	0.12%	0.011%
21	14.004	1801	1805	1807	rBV5	4661	7169	0.22%	0.020%
22	14.145	1822	1829	1837	rBV	1294460	1770241	54.89%	5.058%
23	14.434	1871	1878	1886	rVV	1342724	1910809	59.24%	5.459%
24	14.657	1912	1916	1920	rVB4	2387	3760	0.12%	0.011%
25	14.739	1923	1930	1938	rBV	1025583	1476151	45.77%	4.217%
26	14.916	1953	1960	1976	rBV	808349	1170836	36.30%	3.345%
27	15.504	2055	2060	2065	rBV7	3743	9197	0.29%	0.026%
28	15.728	2091	2098	2106	rVB	1682048	2381025	73.82%	6.803%
29	15.833	2109	2116	2126	rBV	619541	857703	26.59%	2.451%
30	15.963	2135	2138	2142	rVB4	8869	12337	0.38%	0.035%
31	16.422	2212	2216	2219	rBV6	3036	3944	0.12%	0.011%
32	16.592	2240	2245	2247	rBV6	2603	4138	0.13%	0.012%
33	16.669	2254	2258	2261	rBV5	2405	3789	0.12%	0.011%
34	16.763	2269	2274	2275	rBV5	4010	6600	0.20%	0.019%
35	16.886	2293	2295	2300	rBV6	2565	3671	0.11%	0.010%
36	16.933	2300	2303	2307	rBV6	6428	9438	0.29%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037691.D
 Acq On : 25 Nov 2022 10:48
 Operator : CG/JU
 Sample : PB149274BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	17.004	2310	2315	2316	rBV5	2936	3442	0.11%	0.010%
38	17.210	2348	2350	2354	rBV5	4348	5989	0.19%	0.017%
39	17.475	2388	2395	2401	rBV	1328450	1784277	55.32%	5.098%
40	17.575	2405	2412	2422	rBV	2018137	2779400	86.18%	7.941%
41	17.910	2467	2469	2474	rBV6	2718	3534	0.11%	0.010%
42	18.010	2482	2486	2488	rBV5	4148	5516	0.17%	0.016%
43	18.345	2540	2543	2547	rBV5	9909	14321	0.44%	0.041%
44	19.416	2722	2725	2731	rVB2	23802	32047	0.99%	0.092%
45	19.486	2734	2737	2742	rVB	21502	24710	0.77%	0.071%
46	19.621	2756	2760	2762	rBV4	13233	17984	0.56%	0.051%
47	19.851	2793	2799	2810	rBV	2326065	3095045	95.96%	8.843%
48	20.827	2961	2965	2971	rBV	102934	123031	3.81%	0.352%
49	21.639	3098	3103	3109	rBV	1497526	1990582	61.72%	5.687%
50	23.968	3492	3499	3514	rVB2	1542964	3225284	100.00%	9.215%
51	24.127	3519	3526	3538	rVB2	918092	1949804	60.45%	5.571%




Sum of corrected areas: 35000977

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037691.D
Acq On : 25 Nov 2022 10:48
Operator : CG/JU
Sample : PB149274BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK274

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

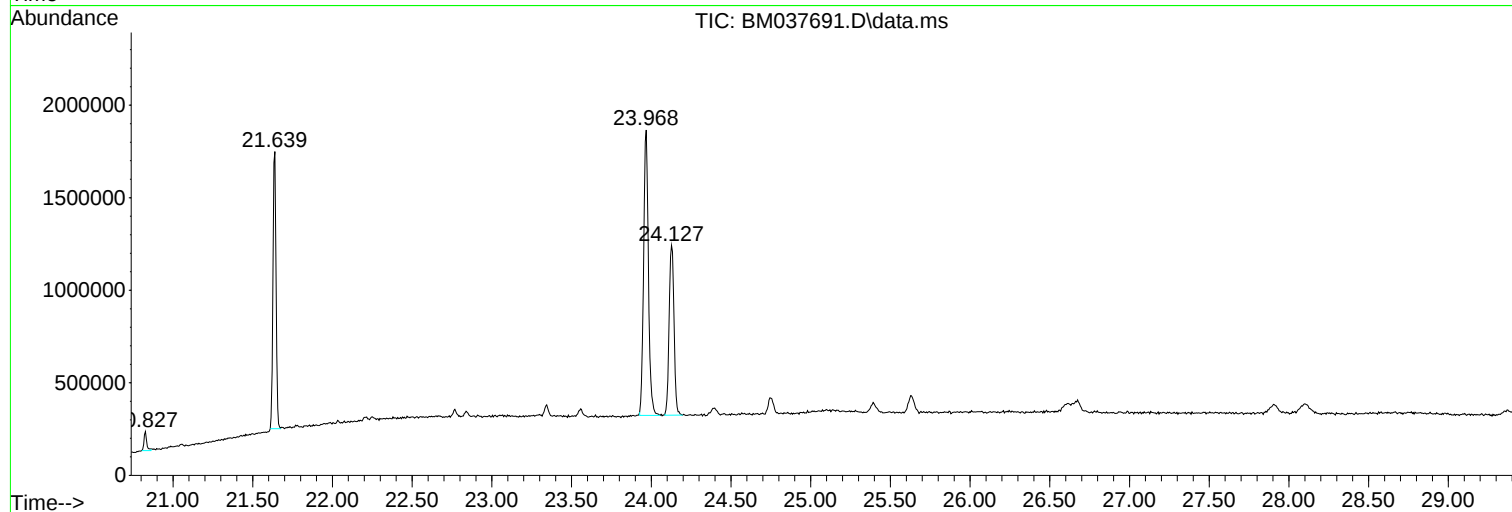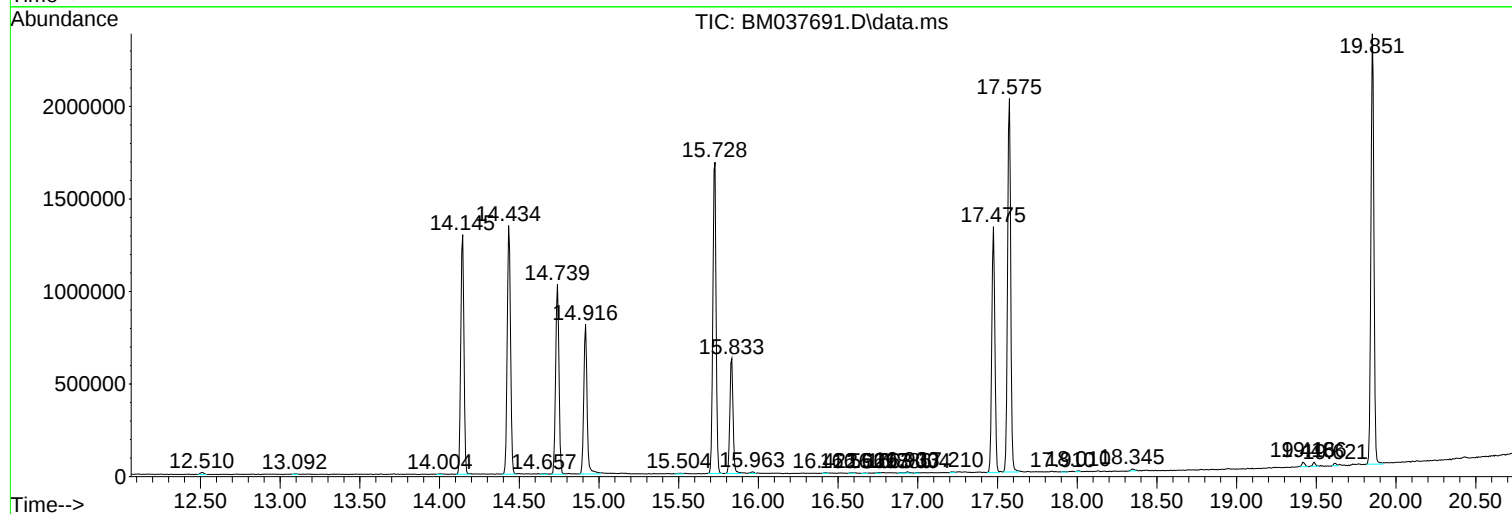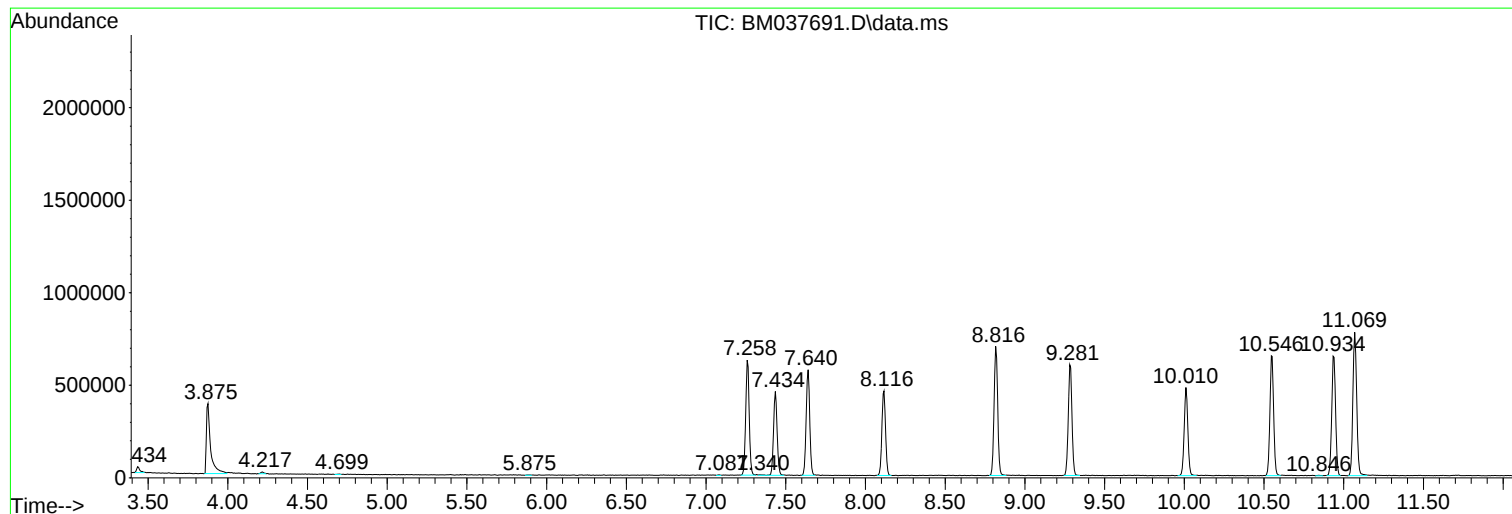

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037691.D
Acq On : 25 Nov 2022 10:48
Operator : CG/JU
Sample : PB149274BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK274

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037691.D
Acq On : 25 Nov 2022 10:48
Operator : CG/JU
Sample : PB149274BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK274

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc