

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037694.D
 Acq On : 25 Nov 2022 14:14
 Operator : CG/JU
 Sample : N5591-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9802

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	3	8	12	rBV	29288	42767	0.92%	0.115%
2	3.722	54	57	64	rBV	55854	84847	1.83%	0.229%
3	3.881	81	84	100	rBV	118928	232889	5.02%	0.628%
4	4.116	120	124	130	rVB3	15081	22494	0.49%	0.061%
5	4.216	137	141	145	rVB2	11469	15414	0.33%	0.042%
6	5.175	300	304	309	rBV	23653	32339	0.70%	0.087%
7	5.775	402	406	409	rVB6	3252	5374	0.12%	0.014%
8	7.257	651	658	668	rVB	197050	313070	6.75%	0.844%
9	7.434	681	688	697	rBV	531054	817802	17.64%	2.205%
10	7.639	716	723	729	rVB	194792	303557	6.55%	0.819%
11	8.116	796	804	811	rBV	508626	786335	16.96%	2.120%
12	8.816	917	923	933	rVB	429212	666386	14.37%	1.797%
13	9.286	995	1003	1010	rBV	707595	1141208	24.61%	3.077%
14	9.686	1069	1071	1075	rVB5	3955	5894	0.13%	0.016%
15	10.010	1118	1126	1133	rBV	98559	164745	3.55%	0.444%
16	10.551	1211	1218	1228	rVB	237562	394373	8.51%	1.063%
17	10.704	1240	1244	1250	rBV7	6882	14513	0.31%	0.039%
18	10.939	1276	1284	1291	rBV	743292	1213986	26.18%	3.274%
19	11.069	1295	1306	1316	rBV	755247	1268389	27.36%	3.420%
20	11.733	1412	1419	1423	rVB4	13376	23780	0.51%	0.064%
21	12.186	1487	1496	1502	rVB4	7484	21122	0.46%	0.057%
22	12.321	1513	1519	1526	rVB2	17800	26656	0.57%	0.072%
23	12.510	1546	1551	1557	rVB3	13384	19553	0.42%	0.053%
24	13.586	1729	1734	1738	rVB5	5077	9145	0.20%	0.025%
25	13.627	1738	1741	1745	rBV5	3414	4856	0.10%	0.013%
26	13.710	1750	1755	1756	rBV5	4317	6175	0.13%	0.017%
27	14.057	1809	1814	1819	rBV3	22804	31270	0.67%	0.084%
28	14.145	1822	1829	1838	rBV	1660581	2149079	46.35%	5.795%
29	14.368	1864	1867	1871	rBV5	7025	10264	0.22%	0.028%
30	14.433	1871	1878	1887	rBV	1606650	2373905	51.20%	6.401%
31	14.627	1904	1911	1913	rBV7	3144	5517	0.12%	0.015%
32	14.739	1924	1930	1937	rBV	1182935	1683258	36.31%	4.539%
33	14.915	1951	1960	1966	rBV	136913	225165	4.86%	0.607%
34	15.145	1996	1999	2002	rVB5	4384	5037	0.11%	0.014%
35	15.568	2068	2071	2075	rVB5	6246	8171	0.18%	0.022%
36	15.727	2090	2098	2111	rBV	2205671	3079428	66.42%	8.304%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037694.D
 Acq On : 25 Nov 2022 14:14
 Operator : CG/JU
 Sample : N5591-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9802

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	15.833	2111	2116	2120	rBV2	68462	98196	2.12%	0.265%
38	15.962	2132	2138	2144	rBV6	16357	25613	0.55%	0.069%
39	16.357	2201	2205	2209	rBV5	3160	6565	0.14%	0.018%
40	16.427	2212	2217	2220	rBV6	7901	10321	0.22%	0.028%
41	16.504	2226	2230	2234	rBV6	3794	6364	0.14%	0.017%
42	16.604	2242	2247	2252	rVB8	7179	13274	0.29%	0.036%
43	16.939	2299	2304	2309	rBV7	7902	13365	0.29%	0.036%
44	17.151	2337	2340	2343	rBV5	4960	6524	0.14%	0.018%
45	17.215	2348	2351	2355	rVV4	10275	10940	0.24%	0.030%
46	17.262	2356	2359	2364	rVV7	4120	8036	0.17%	0.022%
47	17.374	2376	2378	2387	rVB8	6811	11467	0.25%	0.031%
48	17.474	2389	2395	2402	rBV	1453220	1999462	43.13%	5.392%
49	17.574	2406	2412	2422	rVV2	2698331	3762981	81.16%	10.147%
50	18.127	2504	2506	2510	rVB5	9028	8727	0.19%	0.024%
51	18.350	2541	2544	2548	rBV6	12680	16222	0.35%	0.044%
52	19.421	2722	2726	2730	rBV4	25528	33444	0.72%	0.090%
53	19.486	2734	2737	2742	rVB2	23078	27750	0.60%	0.075%
54	19.615	2756	2759	2763	rBV5	14380	19458	0.42%	0.052%
55	19.850	2793	2799	2807	rBV	3165222	4280648	92.33%	11.543%
56	20.827	2962	2965	2968	rVB	55384	55114	1.19%	0.149%
57	21.321	3046	3049	3053	rBV	80165	91092	1.96%	0.246%
58	21.639	3098	3103	3109	rBV	1822968	2374665	51.22%	6.404%
59	23.968	3492	3499	3512	rVB2	2250874	4636337	100.00%	12.502%
60	24.127	3520	3526	3537	rVB2	1151956	2358348	50.87%	6.360%




Sum of corrected areas: 37083676

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037694.D
Acq On : 25 Nov 2022 14:14
Operator : CG/JU
Sample : N5591-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9802

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

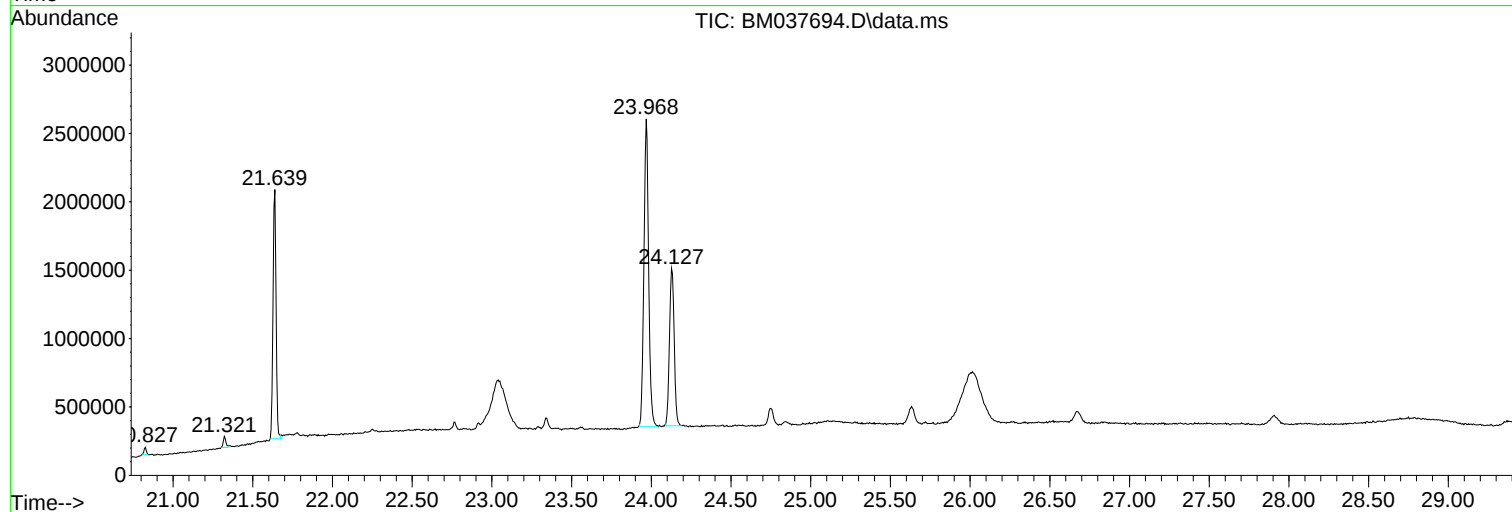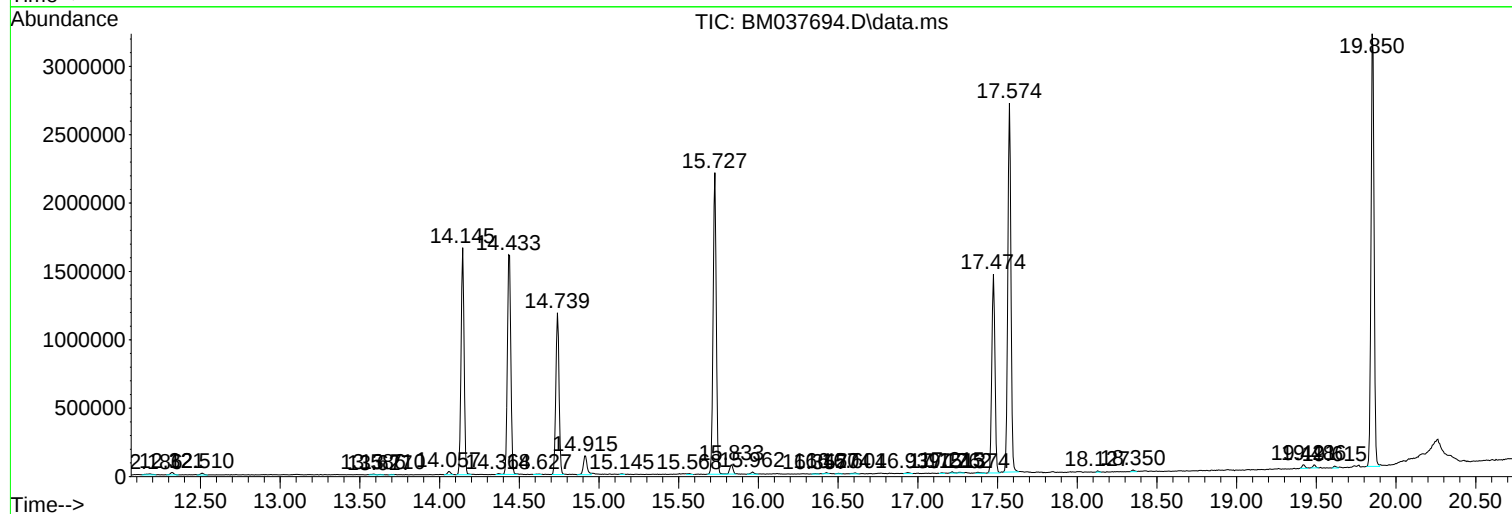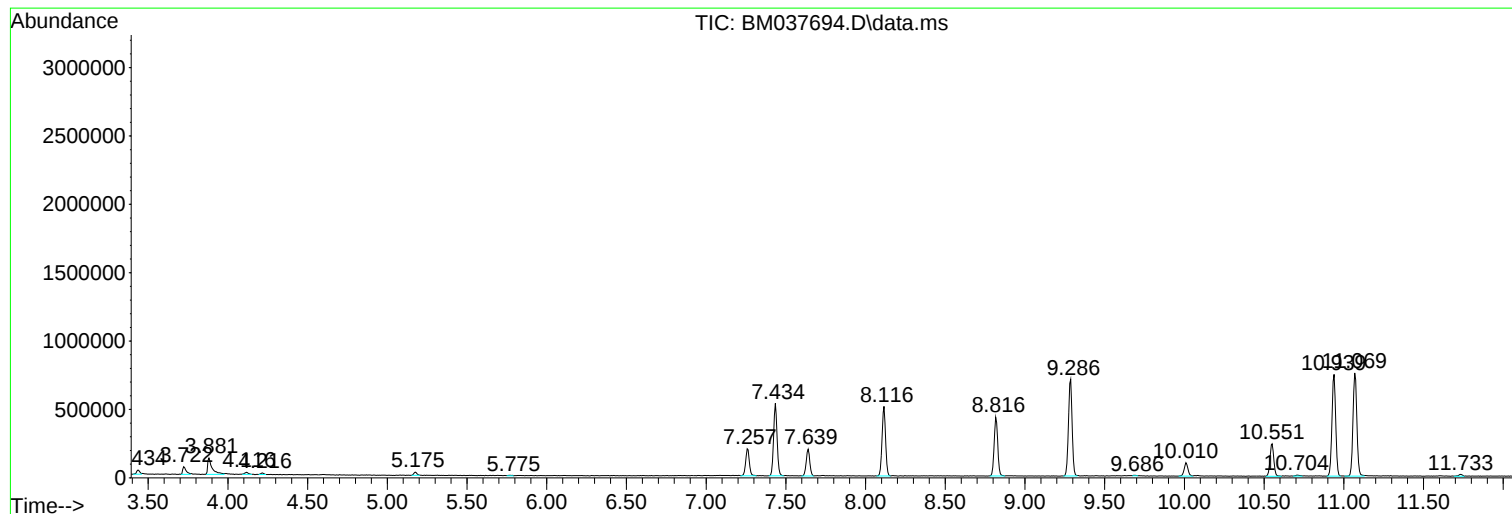

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037694.D
Acq On : 25 Nov 2022 14:14
Operator : CG/JU
Sample : N5591-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9802










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.722	2.16 ng/ul	84847	1,4-Dichlorobenzene-d4	8.116

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	(S)-(+)-1,2-Propanediol			76	C3H8O2	004254-15-3	40
2	4-Penten-2-ol			86	C5H10O	000625-31-0	9
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	9
4	Hydrazine, (2-methoxyethyl)-			90	C3H10N2O	003044-15-3	9
5	(2R,4R)-(-)-Pentanediol			104	C5H12O2	042075-32-1	9

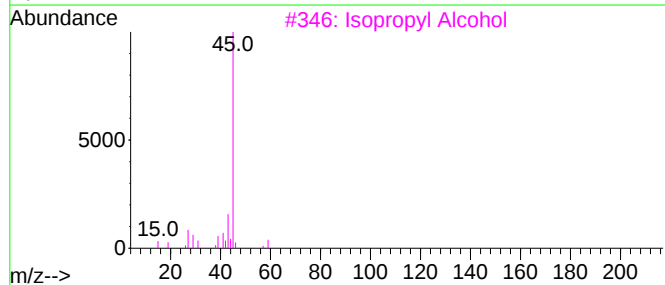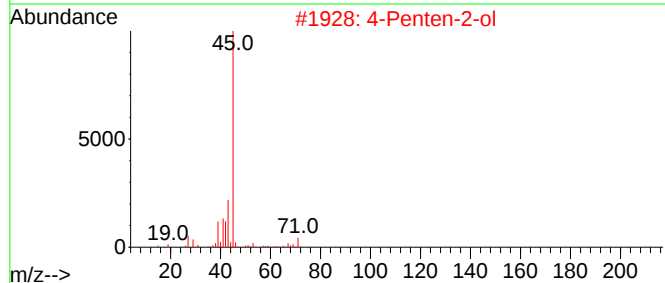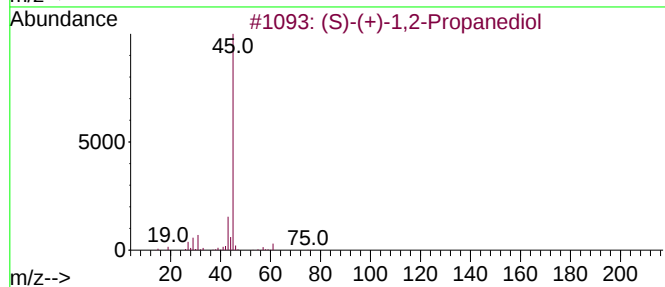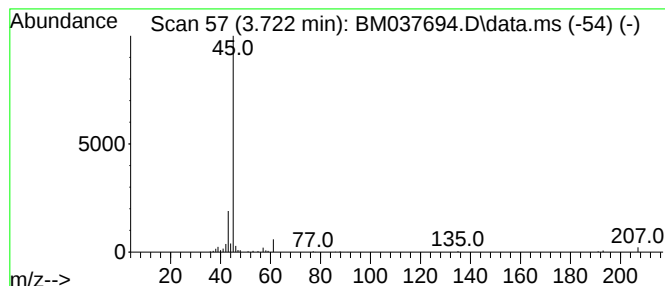

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037694.D
Acq On : 25 Nov 2022 14:14
Operator : CG/JU
Sample : N5591-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9802

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.722	2.2	ng/u1	84847	1	8.116	786335	20.0