

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037699.D
 Acq On : 25 Nov 2022 17:23
 Operator : CG/JU
 Sample : PB149070BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	16	rBV	55739	80063	1.66%	0.151%
2	3.869	79	82	98	rBV	692187	1162560	24.13%	2.187%
3	4.216	138	141	146	rVB	14304	19534	0.41%	0.037%
4	4.446	177	180	182	rBV3	4584	5955	0.12%	0.011%
5	7.257	651	658	668	rBV	966269	1487284	30.86%	2.798%
6	7.434	681	688	699	rVB	739750	1127894	23.41%	2.122%
7	7.640	714	723	732	rBV	894343	1393694	28.92%	2.622%
8	8.116	797	804	812	rVB	669488	1043014	21.64%	1.962%
9	8.816	916	923	933	rBV	1119157	1729220	35.88%	3.253%
10	9.287	995	1003	1009	rBV	916486	1513692	31.41%	2.847%
11	10.010	1117	1126	1140	rBV	719774	1182864	24.55%	2.225%
12	10.545	1209	1217	1227	rBV	1039573	1681149	34.89%	3.162%
13	10.934	1276	1283	1291	rBV	967715	1605454	33.32%	3.020%
14	11.069	1295	1306	1318	rBV	1173636	1918226	39.81%	3.608%
15	12.510	1544	1551	1557	rBV2	19834	31203	0.65%	0.059%
16	13.092	1644	1650	1654	rBV6	3730	6109	0.13%	0.011%
17	13.633	1736	1742	1743	rBV6	2438	4959	0.10%	0.009%
18	14.145	1822	1829	1835	rBV	2002260	2744819	56.96%	5.163%
19	14.433	1871	1878	1887	rBV2	2117424	3019625	62.66%	5.680%
20	14.739	1924	1930	1940	rBV	1512095	2148043	44.58%	4.041%
21	14.916	1953	1960	1971	rBV	1261746	1754385	36.41%	3.300%
22	15.145	1995	1999	2003	rVB7	7646	10374	0.22%	0.020%
23	15.498	2055	2059	2064	rBV8	3695	6442	0.13%	0.012%
24	15.727	2091	2098	2104	rVB	2677035	3756799	77.96%	7.067%
25	15.833	2109	2116	2128	rBV	958183	1306776	27.12%	2.458%
26	15.963	2131	2138	2144	rVB5	12442	21168	0.44%	0.040%
27	16.933	2300	2303	2309	rVB6	6334	12088	0.25%	0.023%
28	17.221	2346	2352	2355	rBV7	5978	11594	0.24%	0.022%
29	17.262	2355	2359	2361	rBV4	5837	8320	0.17%	0.016%
30	17.474	2388	2395	2403	rBV	1914171	2611953	54.20%	4.913%
31	17.574	2405	2412	2421	rVV	3151278	4273215	88.68%	8.038%
32	17.845	2455	2458	2464	rVB7	5069	8766	0.18%	0.016%
33	18.009	2483	2486	2488	rBV3	4406	5563	0.12%	0.010%
34	18.127	2503	2506	2507	rBV3	4676	5467	0.11%	0.010%
35	18.351	2540	2544	2548	rBV6	9441	15004	0.31%	0.028%
36	19.415	2722	2725	2729	rBV3	34045	48840	1.01%	0.092%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037699.D
Acq On : 25 Nov 2022 17:23
Operator : CG/JU
Sample : PB149070BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK070

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Title : SVOA CALIBRATION

37	19.486	2733	2737	2741	rVB3	36015	52011	1.08%	0.098%
38	19.856	2794	2800	2809	rBV	3593483	4818892	100.00%	9.065%
39	20.827	2962	2965	2970	rBV2	89560	100630	2.09%	0.189%
40	21.639	3098	3103	3108	rBV	2257144	2936977	60.95%	5.525%
41	23.974	3492	3500	3514	rVB2	2288827	4743094	98.43%	8.922%
42	24.133	3520	3527	3540	rVB	1353321	2745875	56.98%	5.165%




Sum of corrected areas: 53159594

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037699.D
Acq On : 25 Nov 2022 17:23
Operator : CG/JU
Sample : PB149070BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

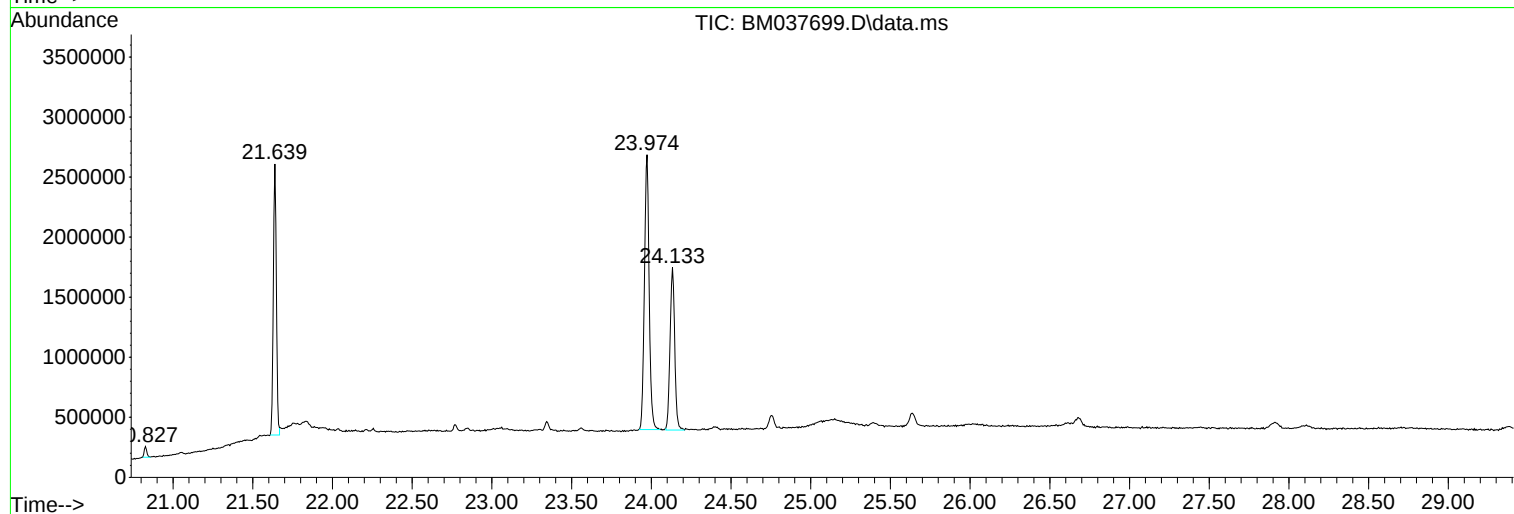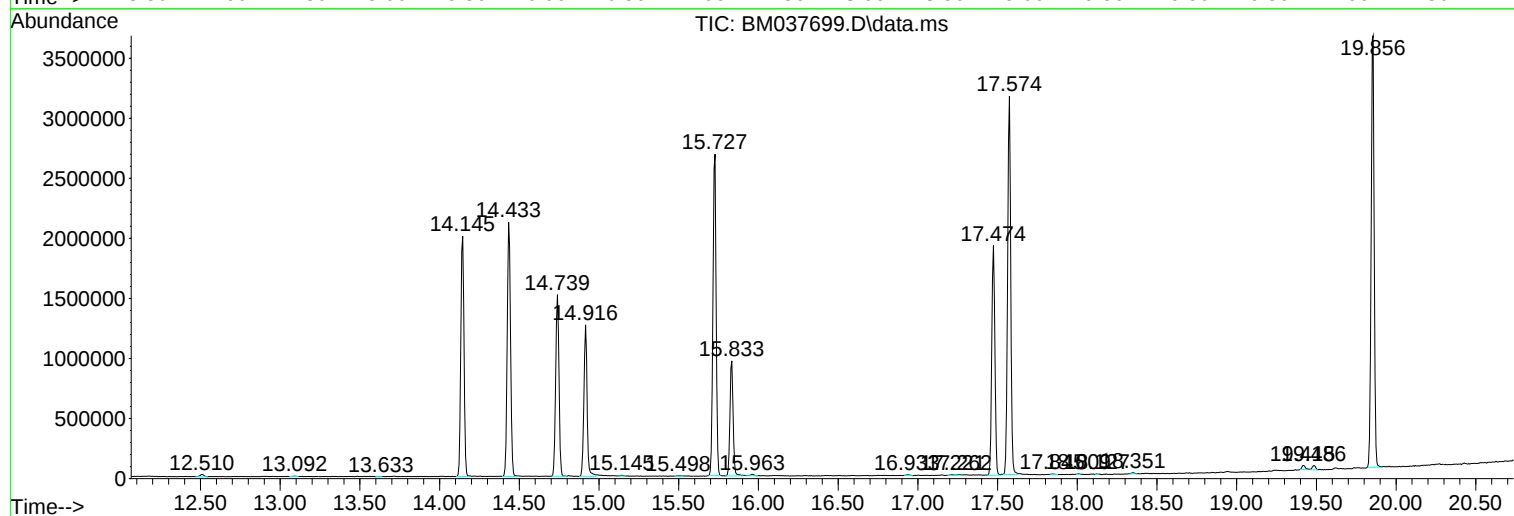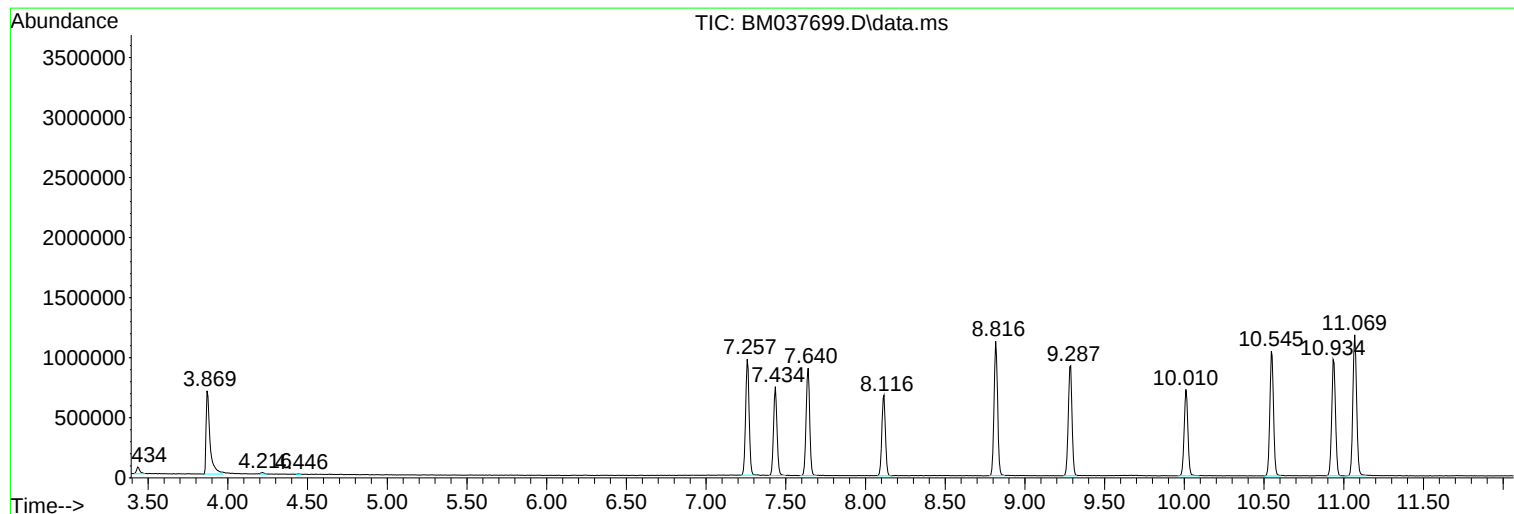

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037699.D
Acq On : 25 Nov 2022 17:23
Operator : CG/JU
Sample : PB149070BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037699.D
Acq On : 25 Nov 2022 17:23
Operator : CG/JU
Sample : PB149070BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc