

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037705.D
 Acq On : 25 Nov 2022 21:06
 Operator : CG/JU
 Sample : N5593-03DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	12	14	31	rVB	292456	460197	0.97%	0.514%
2	3.881	81	84	100	rBV	107984	214410	0.45%	0.239%
3	4.769	227	235	262	rBV	30767091	47231520	100.00%	52.711%
4	5.175	299	304	311	rVB	75944	108179	0.23%	0.121%
5	5.352	329	334	339	rBV	49514	74765	0.16%	0.083%
6	7.258	652	658	666	rVB	180428	269751	0.57%	0.301%
7	7.434	681	688	700	rBV	553157	864623	1.83%	0.965%
8	7.640	714	723	730	rBV	516196	830791	1.76%	0.927%
9	8.110	796	803	817	rVB	740137	1187591	2.51%	1.325%
10	8.469	859	864	869	rVB2	36475	59519	0.13%	0.066%
11	8.816	917	923	932	rBV	444288	690565	1.46%	0.771%
12	9.281	995	1002	1011	rBV	705114	1126608	2.39%	1.257%
13	10.010	1117	1126	1135	rBV	505400	822300	1.74%	0.918%
14	10.546	1210	1217	1227	rBV	730304	1162355	2.46%	1.297%
15	10.934	1274	1283	1294	rBV	1076310	1786632	3.78%	1.994%
16	11.069	1298	1306	1318	rVV	561556	948353	2.01%	1.058%
17	14.145	1821	1829	1838	rBV	1554492	2114705	4.48%	2.360%
18	14.434	1871	1878	1891	rBV	1662721	2324811	4.92%	2.595%
19	14.739	1923	1930	1936	rBV	1663411	2386417	5.05%	2.663%
20	14.910	1953	1959	1970	rBV	169853	275287	0.58%	0.307%
21	15.722	2089	2097	2104	rBV	2095598	2965610	6.28%	3.310%
22	15.828	2108	2115	2129	rBV	678475	963584	2.04%	1.075%
23	17.475	2388	2395	2402	rBV	2052639	2828742	5.99%	3.157%
24	17.575	2405	2412	2427	rVV	2369197	3281600	6.95%	3.662%
25	18.345	2539	2543	2553	rBV2	120609	192385	0.41%	0.215%
26	18.439	2554	2559	2568	rVB2	121288	177542	0.38%	0.198%
27	19.480	2732	2736	2741	rBV3	32611	64793	0.14%	0.072%
28	19.616	2755	2759	2765	rBV	107220	148942	0.32%	0.166%
29	19.851	2794	2799	2809	rBV	2978383	3795920	8.04%	4.236%
30	20.827	2961	2965	2969	rBV	190644	212639	0.45%	0.237%
31	21.639	3098	3103	3110	rBV	2472515	3203649	6.78%	3.575%
32	23.968	3492	3499	3511	rVB2	1820410	3831707	8.11%	4.276%
33	24.133	3520	3527	3538	rVB2	1469154	2998804	6.35%	3.347%




Sum of corrected areas: 89605296

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037705.D
Acq On : 25 Nov 2022 21:06
Operator : CG/JU
Sample : N5593-03DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

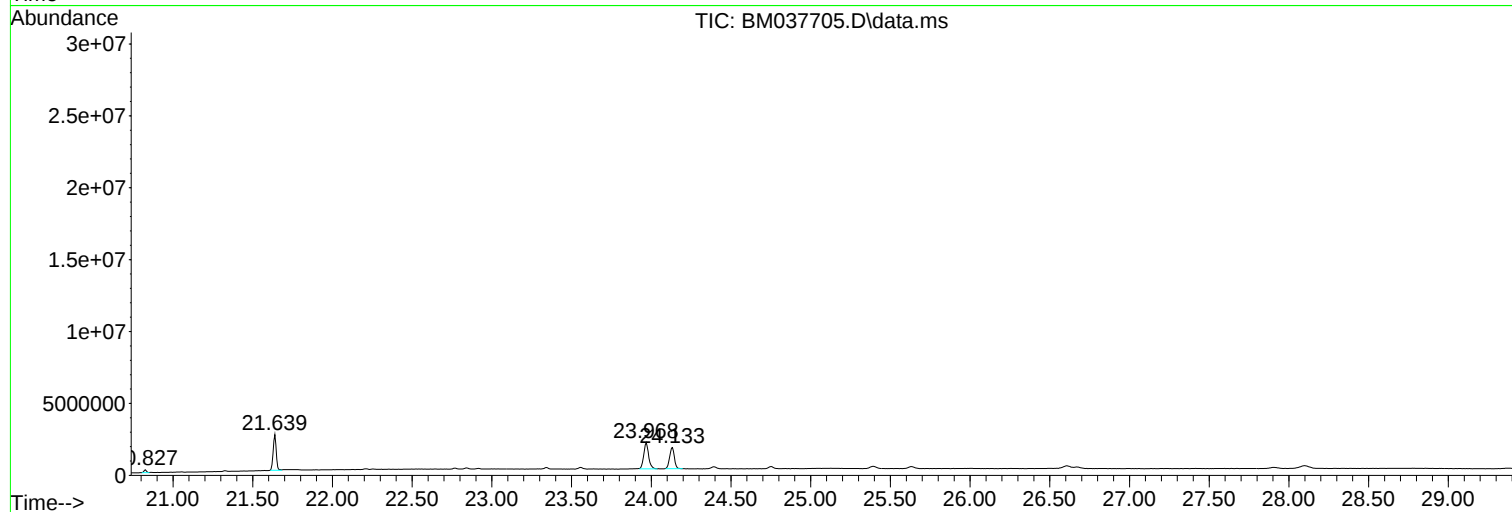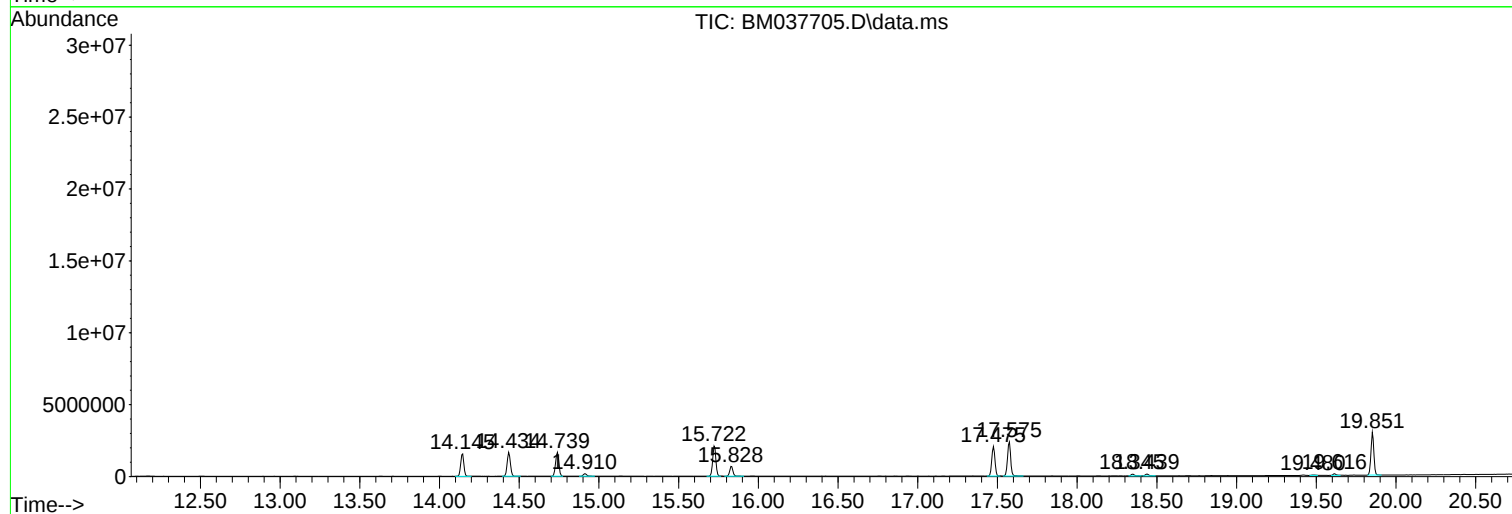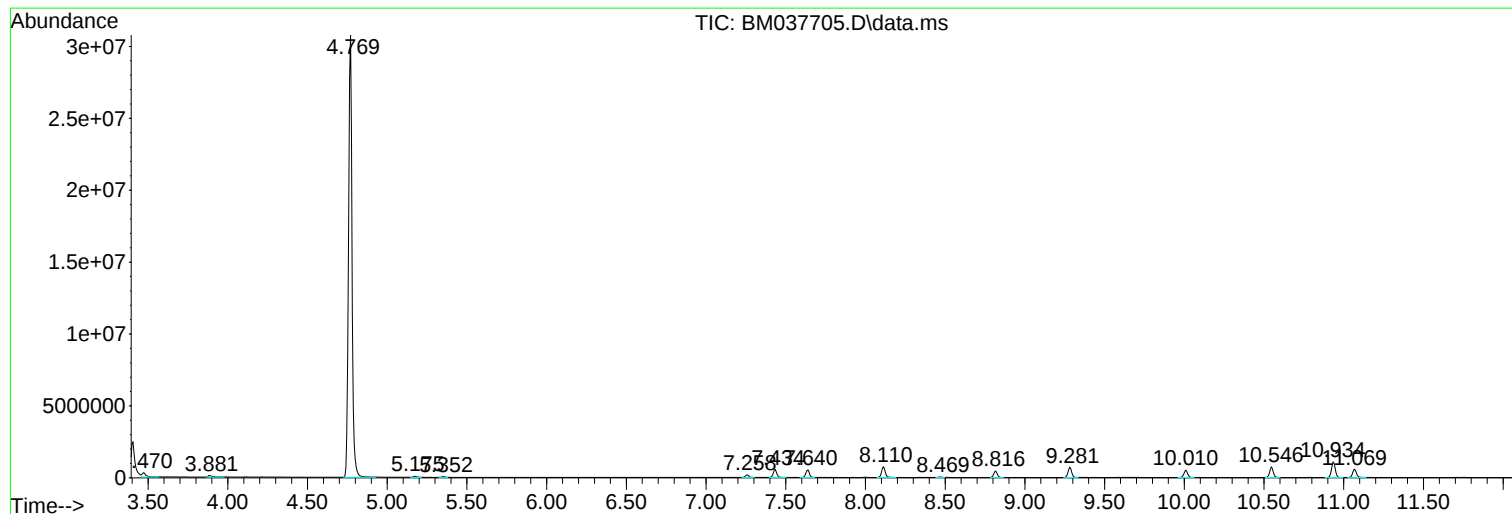

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037705.D
Acq On : 25 Nov 2022 21:06
Operator : CG/JU
Sample : N5593-03DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD1DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.769	795.42 ng/ul	47231500	1,4-Dichlorobenzene-d4	8.110

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

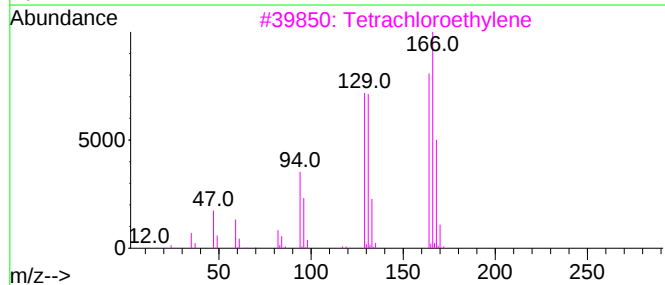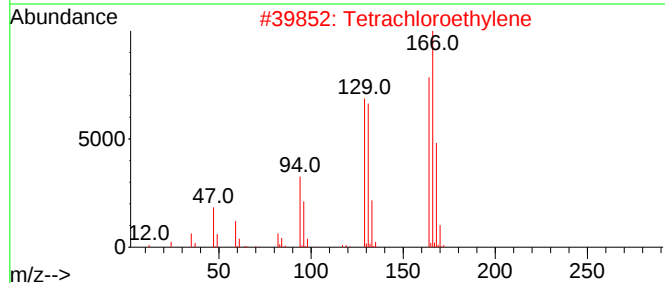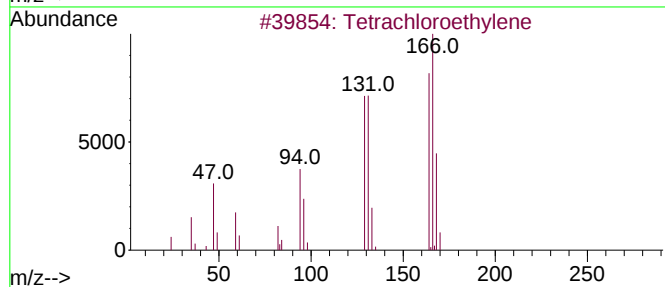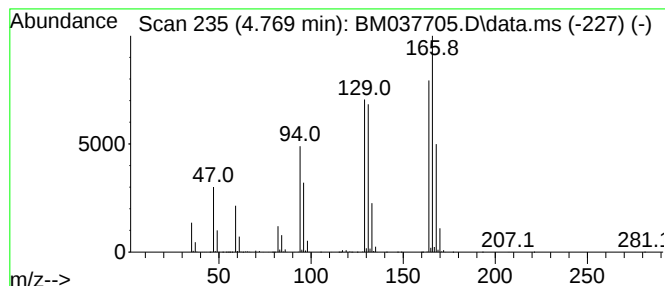

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037705.D
Acq On : 25 Nov 2022 21:06
Operator : CG/JU
Sample : N5593-03DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.769	795.4	ng/ul	47231500	1	8.110	1187590	20.0