

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037718.D
 Acq On : 26 Nov 2022 05:42
 Operator : CG/JU
 Sample : PB149074BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	16	rBV	64058	94968	1.69%	0.146%
2	3.869	78	82	106	rBV	825683	1410893	25.15%	2.176%
3	4.210	137	140	144	rVB3	15602	17795	0.32%	0.027%
4	5.716	393	396	399	rBV4	3665	6000	0.11%	0.009%
5	7.257	649	658	669	rBV	1175245	1796897	32.03%	2.771%
6	7.434	681	688	697	rVB	876153	1368543	24.40%	2.110%
7	7.634	715	722	735	rBV	1061409	1664782	29.68%	2.567%
8	8.110	796	803	811	rVB	893914	1389134	24.76%	2.142%
9	8.816	915	923	932	rVV	1355313	2104613	37.52%	3.245%
10	9.281	994	1002	1010	rBV	1131399	1822341	32.48%	2.810%
11	10.010	1116	1126	1136	rBV	847609	1424636	25.40%	2.197%
12	10.545	1209	1217	1228	rBV	1274295	2022211	36.05%	3.118%
13	10.934	1276	1283	1292	rVB	1333066	2186459	38.98%	3.372%
14	11.069	1298	1306	1317	rBV	1341349	2266374	40.40%	3.495%
15	12.175	1486	1494	1499	rVB3	12032	26067	0.46%	0.040%
16	12.504	1545	1550	1555	rBV2	22477	34471	0.61%	0.053%
17	13.092	1646	1650	1654	rBV6	4650	8632	0.15%	0.013%
18	13.627	1736	1741	1746	rVB6	9201	14263	0.25%	0.022%
19	13.710	1750	1755	1758	rVV7	5644	10085	0.18%	0.016%
20	14.139	1822	1828	1835	rBV	2356909	3208935	57.20%	4.948%
21	14.433	1871	1878	1890	rBV	2602934	3691091	65.80%	5.692%
22	14.739	1922	1930	1939	rBV	1988258	2937915	52.37%	4.531%
23	14.810	1939	1942	1947	rVB7	7262	9992	0.18%	0.015%
24	14.916	1952	1960	1975	rBV	1504572	2135185	38.06%	3.293%
25	15.092	1986	1990	1995	rVB8	6823	11654	0.21%	0.018%
26	15.139	1995	1998	2001	rBV5	7844	10181	0.18%	0.016%
27	15.721	2087	2097	2104	rBV	3257825	4551305	81.13%	7.019%
28	15.827	2108	2115	2123	rBV	1128817	1521884	27.13%	2.347%
29	15.963	2134	2138	2141	rVB4	17266	21512	0.38%	0.033%
30	16.586	2242	2244	2246	rBV3	5171	5682	0.10%	0.009%
31	16.874	2287	2293	2294	rBV4	3623	5797	0.10%	0.009%
32	16.933	2299	2303	2311	rVB4	10683	17823	0.32%	0.027%
33	17.145	2336	2339	2342	rBV5	5837	7635	0.14%	0.012%
34	17.215	2348	2351	2353	rBV4	5760	7656	0.14%	0.012%
35	17.474	2388	2395	2404	rBV	2491420	3418818	60.94%	5.272%
36	17.568	2405	2411	2425	rVV2	3462849	5079080	90.54%	7.832%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037718.D
 Acq On : 26 Nov 2022 05:42
 Operator : CG/JU
 Sample : PB149074BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK074

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	17.839	2455	2457	2461	rVB4	6945	8810	0.16%	0.014%
38	18.127	2503	2506	2510	rBV5	8562	12533	0.22%	0.019%
39	18.351	2540	2544	2548	rBV5	13497	16663	0.30%	0.026%
40	19.415	2722	2725	2729	rVB3	38061	46391	0.83%	0.072%
41	19.486	2733	2737	2742	rVV3	38931	52423	0.93%	0.081%
42	19.609	2756	2758	2763	rBV6	15235	18070	0.32%	0.028%
43	19.851	2793	2799	2808	rBV	4234657	5470387	97.51%	8.436%
44	20.821	2961	2964	2968	rBV	151196	157306	2.80%	0.243%
45	21.633	3097	3102	3109	rBV	2808629	3664535	65.32%	5.651%
46	23.962	3491	3498	3509	rVB2	2628453	5609846	100.00%	8.651%
47	24.127	3519	3526	3537	rVB2	1709722	3478948	62.02%	5.365%


Sum of corrected areas: 64847221

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037718.D
Acq On : 26 Nov 2022 05:42
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK074

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

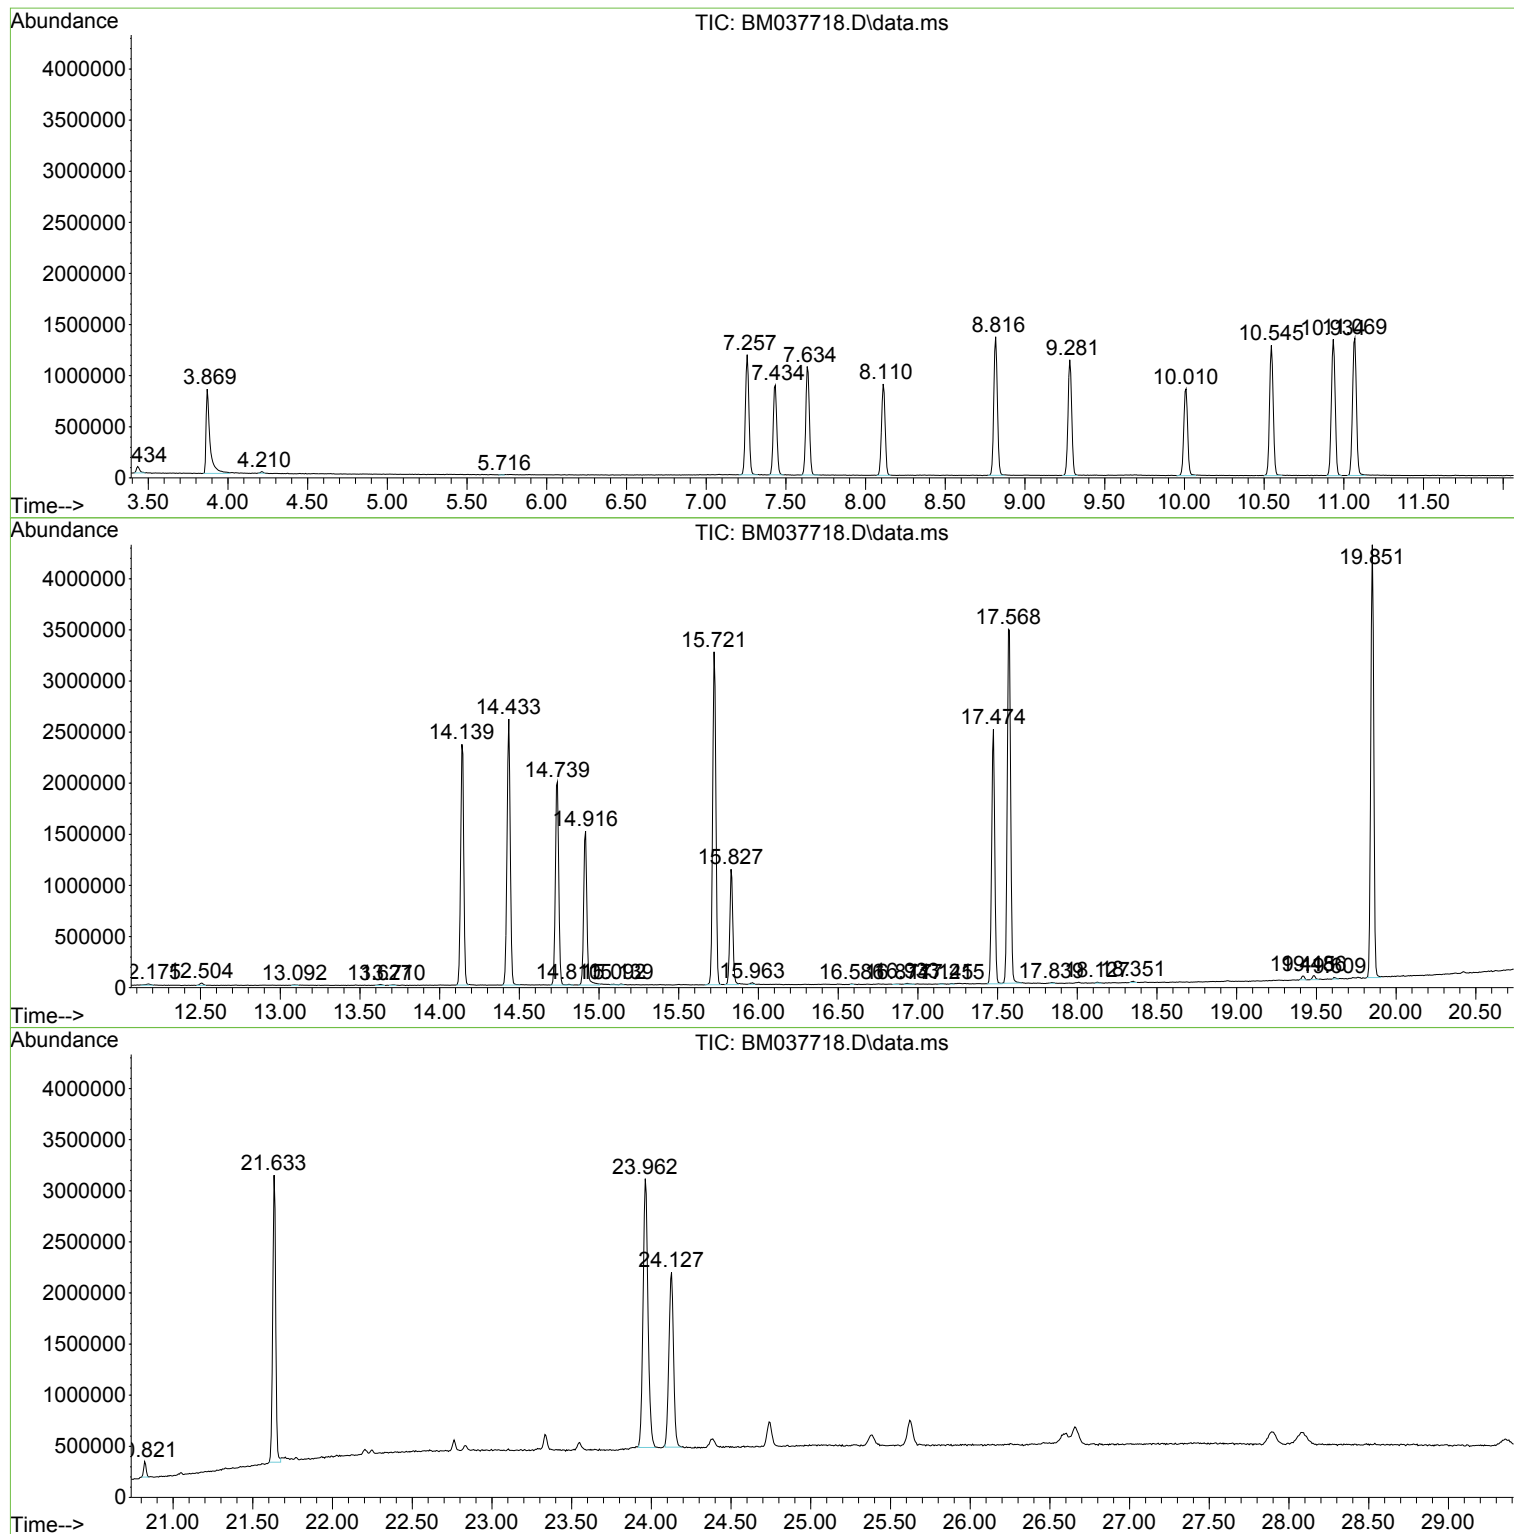

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037718.D
Acq On : 26 Nov 2022 05:42
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK074

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037718.D
Acq On : 26 Nov 2022 05:42
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK074

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc