

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037720.D
 Acq On : 26 Nov 2022 06:55
 Operator : CG/JU
 Sample : PB149030BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK030

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rBV	75157	105065	1.56%	0.142%
2	3.869	78	82	106	rBV	1001831	1686790	25.02%	2.283%
3	4.211	137	140	147	rVB3	16016	24447	0.36%	0.033%
4	7.257	651	658	667	rVB	1427104	2176756	32.29%	2.946%
5	7.428	681	687	699	rVB	1063569	1694671	25.14%	2.294%
6	7.634	714	722	730	rBV	1287558	2043737	30.32%	2.766%
7	8.110	796	803	811	rBV	893438	1337816	19.85%	1.811%
8	8.816	914	923	933	rBV	1650825	2594397	38.49%	3.512%
9	9.281	994	1002	1009	rBV	1416560	2251123	33.40%	3.047%
10	10.010	1117	1126	1139	rBV	1073796	1789011	26.54%	2.422%
11	10.222	1160	1162	1169	rVB6	4831	7461	0.11%	0.010%
12	10.546	1209	1217	1226	rBV	1597647	2522345	37.42%	3.414%
13	10.934	1275	1283	1292	rBV	1260034	2085684	30.94%	2.823%
14	11.069	1297	1306	1317	rBV	1648549	2797762	41.51%	3.787%
15	11.698	1409	1413	1417	rBV6	6229	9365	0.14%	0.013%
16	12.169	1482	1493	1499	rBV5	13714	34230	0.51%	0.046%
17	12.504	1546	1550	1555	rBV	29140	45394	0.67%	0.061%
18	13.628	1737	1741	1746	rBV	29612	38017	0.56%	0.051%
19	13.716	1752	1756	1759	rBV3	7630	11055	0.16%	0.015%
20	14.139	1822	1828	1835	rBV	2939560	3965772	58.83%	5.368%
21	14.433	1870	1878	1886	rBV	3254246	4618288	68.52%	6.251%
22	14.739	1923	1930	1938	rBV	1875253	2806582	41.64%	3.799%
23	14.816	1938	1943	1946	rVB7	7212	10042	0.15%	0.014%
24	14.916	1953	1960	1974	rBV	1724976	2539439	37.67%	3.437%
25	15.133	1995	1997	2004	rVB7	7264	9159	0.14%	0.012%
26	15.498	2055	2059	2065	rBV7	3996	8207	0.12%	0.011%
27	15.722	2088	2097	2107	rVB	4025747	5641401	83.69%	7.636%
28	15.828	2107	2115	2126	rBV	1399617	1957450	29.04%	2.650%
29	15.957	2133	2137	2142	rVB5	19150	29805	0.44%	0.040%
30	16.927	2300	2302	2304	rBV3	6655	7439	0.11%	0.010%
31	16.992	2310	2313	2316	rBV4	4989	7131	0.11%	0.010%
32	17.257	2355	2358	2362	rBV5	5712	8859	0.13%	0.012%
33	17.474	2388	2395	2403	rBV	2260641	3253808	48.27%	4.404%
34	17.569	2405	2411	2428	rVB2	4422312	6317054	93.72%	8.550%
35	17.757	2441	2443	2449	rVB6	8737	11729	0.17%	0.016%
36	17.845	2454	2458	2461	rVB5	10702	12614	0.19%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037720.D
Acq On : 26 Nov 2022 06:55
Operator : CG/JU
Sample : PB149030BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK030

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Title : SVOA CALIBRATION

37	19.416	2721	2725	2731	rVB3	54006	76665	1.14%	0.104%
38	19.480	2733	2736	2741	rVB2	44001	60485	0.90%	0.082%
39	19.851	2793	2799	2807	rBV	5184367	6740526	100.00%	9.124%
40	20.821	2962	2964	2970	rVB3	69881	69439	1.03%	0.094%
41	21.633	3097	3102	3110	rBV2	2549739	3318638	49.23%	4.492%
42	23.962	3491	3498	3514	rVB2	2869976	6156934	91.34%	8.334%
43	24.127	3519	3526	3539	rVB2	1433654	2997049	44.46%	4.057%




Sum of corrected areas: 73879641

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037720.D
Acq On : 26 Nov 2022 06:55
Operator : CG/JU
Sample : PB149030BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

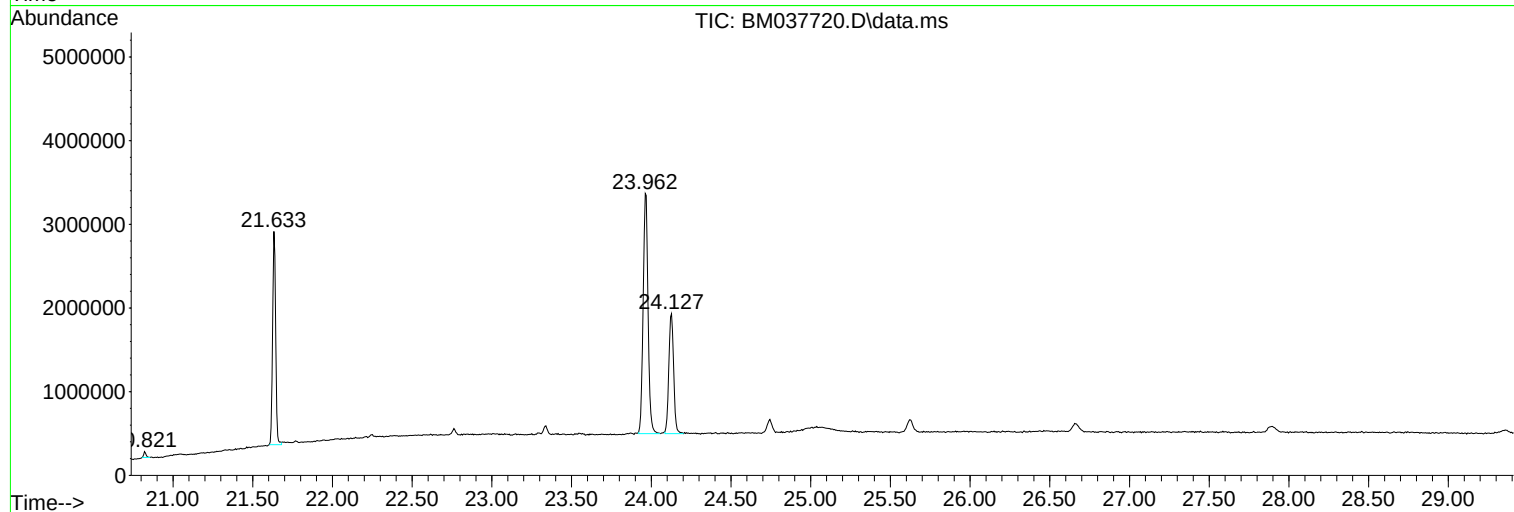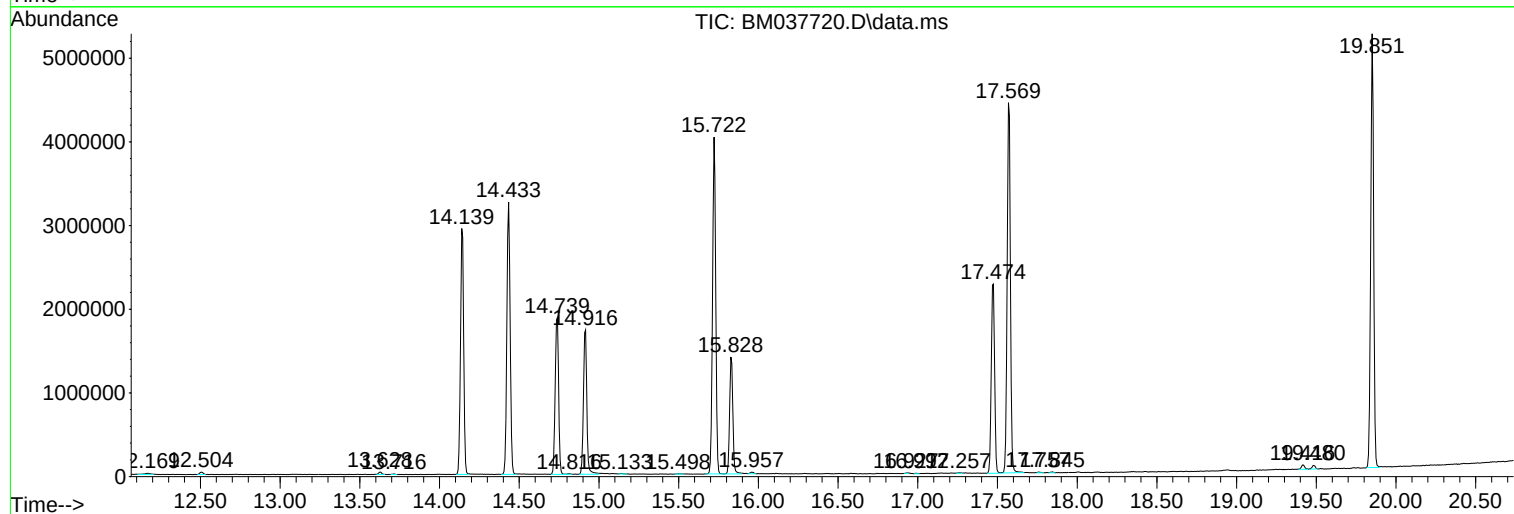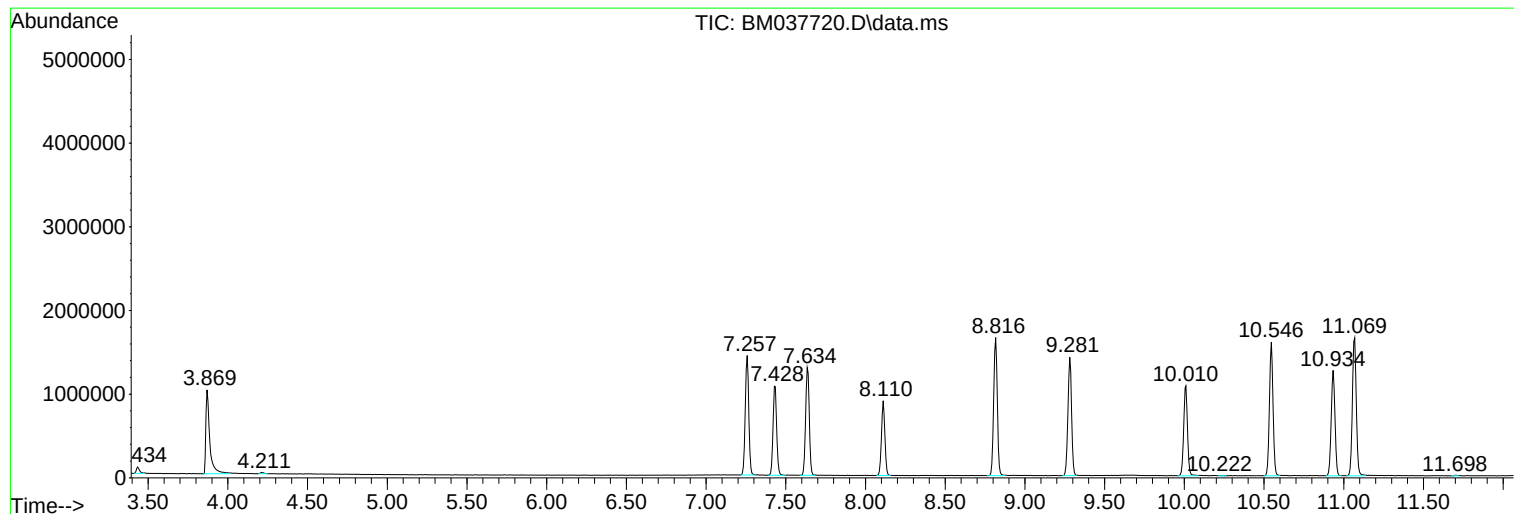

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037720.D
Acq On : 26 Nov 2022 06:55
Operator : CG/JU
Sample : PB149030BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037720.D
Acq On : 26 Nov 2022 06:55
Operator : CG/JU
Sample : PB149030BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc