

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037727.D
 Acq On : 26 Nov 2022 11:12
 Operator : CG/JU
 Sample : N5592-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	19	rBV	58613	86214	1.13%	0.121%
2	3.875	80	83	98	rBV	278313	497433	6.52%	0.699%
3	4.116	120	124	134	rVB2	27753	44875	0.59%	0.063%
4	4.216	136	141	146	rVB3	18664	28380	0.37%	0.040%
5	4.763	230	234	242	rVB5	16912	27657	0.36%	0.039%
6	7.063	621	625	630	rBV7	5917	7814	0.10%	0.011%
7	7.257	651	658	668	rVB	321481	505978	6.63%	0.711%
8	7.428	680	687	699	rBV	1074658	1670876	21.90%	2.347%
9	7.634	715	722	729	rBV	1005769	1555542	20.39%	2.185%
10	7.722	733	737	740	rBV5	6574	10168	0.13%	0.014%
11	8.110	796	803	811	rBV	842495	1280577	16.79%	1.799%
12	8.816	915	923	931	rBV	837255	1344943	17.63%	1.889%
13	9.281	994	1002	1014	rBV	1442620	2297850	30.12%	3.228%
14	9.375	1014	1018	1026	rVV8	4838	13825	0.18%	0.019%
15	9.440	1026	1029	1033	rVB5	6209	8800	0.12%	0.012%
16	10.004	1117	1125	1137	rBV	1029376	1716541	22.50%	2.411%
17	10.222	1158	1162	1166	rVB6	5430	9090	0.12%	0.013%
18	10.545	1210	1217	1230	rBV	1419093	2320692	30.42%	3.260%
19	10.934	1274	1283	1292	rBV	1221057	2051696	26.89%	2.882%
20	11.063	1298	1305	1317	rBV	1143656	1963826	25.74%	2.759%
21	11.698	1407	1413	1418	rBV5	11250	20209	0.26%	0.028%
22	12.316	1513	1518	1521	rBV6	4718	8599	0.11%	0.012%
23	12.510	1546	1551	1557	rVB2	30794	52489	0.69%	0.074%
24	12.581	1557	1563	1567	rBV5	3329	8593	0.11%	0.012%
25	13.104	1648	1652	1655	rVB6	8152	12170	0.16%	0.017%
26	13.351	1688	1694	1699	rBV9	10938	20381	0.27%	0.029%
27	13.627	1735	1741	1746	rBV2	15947	23892	0.31%	0.034%
28	14.139	1822	1828	1841	rBV	3101835	4216304	55.27%	5.923%
29	14.433	1871	1878	1885	rVV	3416820	4835671	63.38%	6.793%
30	14.733	1923	1929	1938	rVB	1921337	2778998	36.43%	3.904%
31	14.816	1938	1943	1946	rBV6	6371	8279	0.11%	0.012%
32	14.910	1953	1959	1973	rBV	374153	560689	7.35%	0.788%
33	15.139	1992	1998	2001	rBV6	20498	35569	0.47%	0.050%
34	15.498	2055	2059	2062	rBV4	5765	10540	0.14%	0.015%
35	15.721	2088	2097	2104	rBV	4392751	6106004	80.04%	8.577%
36	15.827	2109	2115	2128	rVV	1568456	2141095	28.06%	3.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037727.D
 Acq On : 26 Nov 2022 11:12
 Operator : CG/JU
 Sample : N5592-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	15.957	2133	2137	2143	rVB4	23068	38010	0.50%	0.053%
38	16.110	2161	2163	2170	rVB9	4615	8007	0.10%	0.011%
39	16.410	2210	2214	2221	rBV6	14274	23187	0.30%	0.033%
40	16.933	2297	2303	2307	rBV7	10803	16887	0.22%	0.024%
41	17.151	2336	2340	2344	rBV7	9157	12189	0.16%	0.017%
42	17.257	2354	2358	2362	rBV6	4902	9100	0.12%	0.013%
43	17.380	2372	2379	2380	rBV7	6186	10279	0.13%	0.014%
44	17.468	2388	2394	2401	rBV	2266423	3221257	42.22%	4.525%
45	17.568	2404	2411	2424	rBV2	4931163	7052350	92.44%	9.906%
46	17.845	2455	2458	2461	rVB4	7228	8471	0.11%	0.012%
47	18.127	2503	2506	2510	rVB5	11212	14332	0.19%	0.020%
48	18.345	2538	2543	2551	rBV	180551	259299	3.40%	0.364%
49	18.427	2554	2557	2562	rVB3	29450	39043	0.51%	0.055%
50	19.415	2721	2725	2730	rBV2	63115	80052	1.05%	0.112%
51	19.486	2732	2737	2742	rBV	68830	119028	1.56%	0.167%
52	19.609	2754	2758	2763	rBV	178193	222154	2.91%	0.312%
53	19.851	2793	2799	2807	rBV	6112197	7629140	100.00%	10.717%
54	20.821	2961	2964	2968	rVB	71816	78033	1.02%	0.110%
55	21.321	3047	3049	3054	rVB2	78714	78697	1.03%	0.111%
56	21.633	3097	3102	3108	rBV	2664607	3412794	44.73%	4.794%
57	23.968	3491	3499	3511	rVB2	3529107	7448079	97.63%	10.462%
58	24.121	3519	3525	3534	rVB2	1485791	3126738	40.98%	4.392%




Sum of corrected areas: 71189385

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037727.D
Acq On : 26 Nov 2022 11:12
Operator : CG/JU
Sample : N5592-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

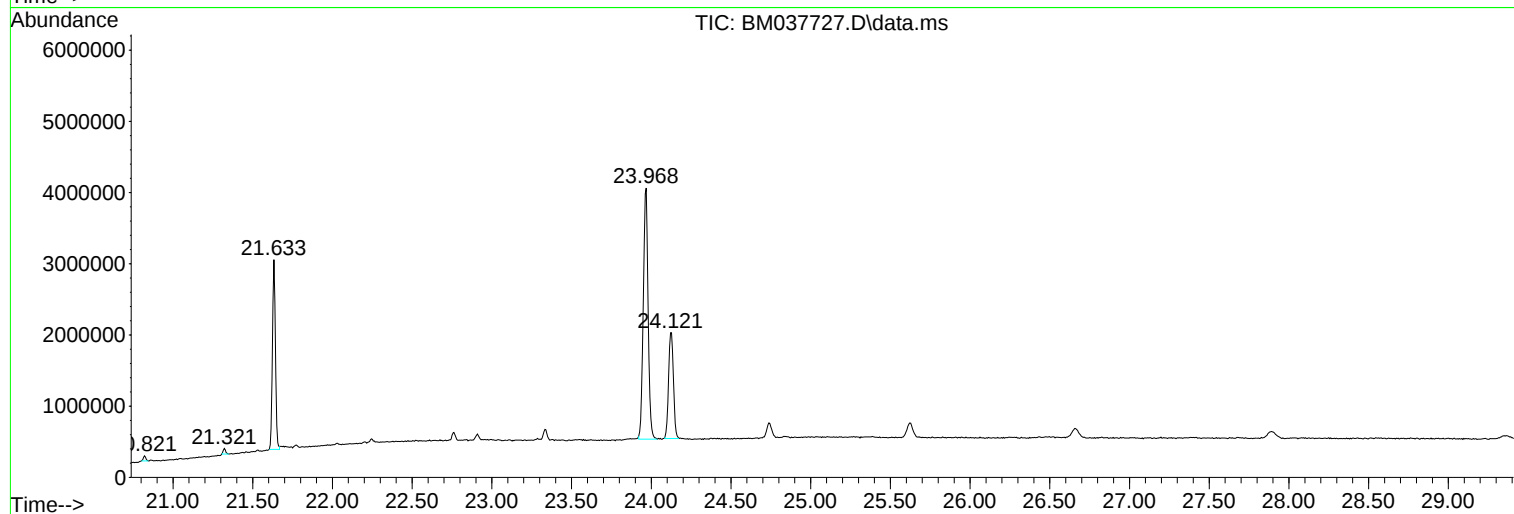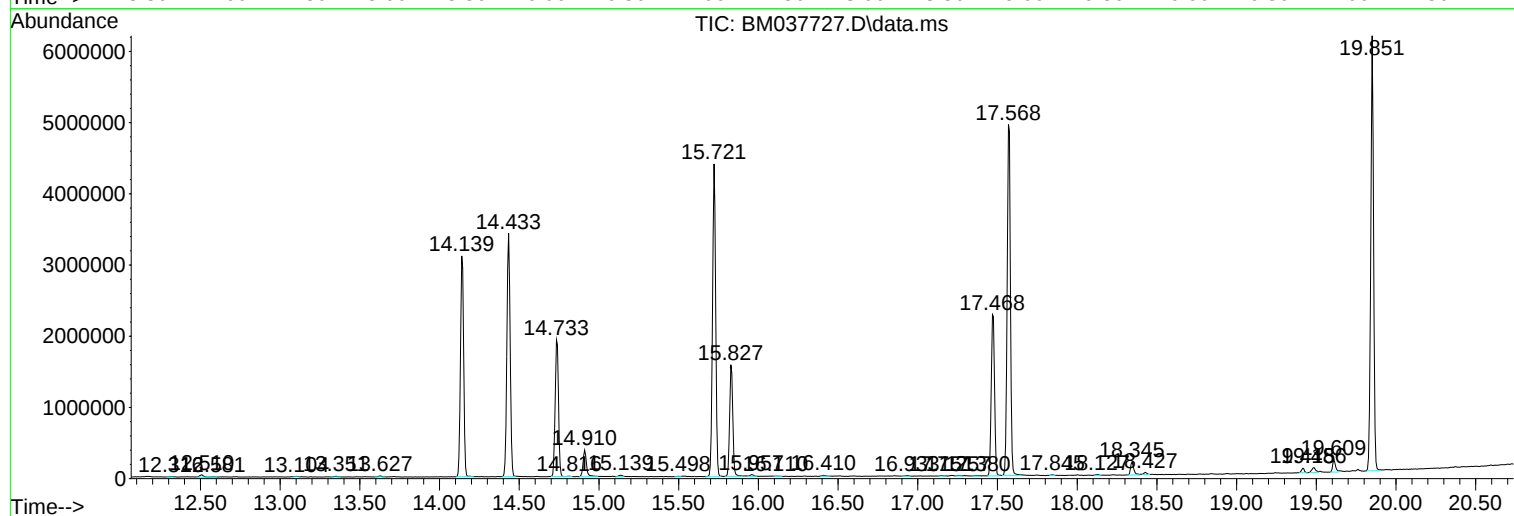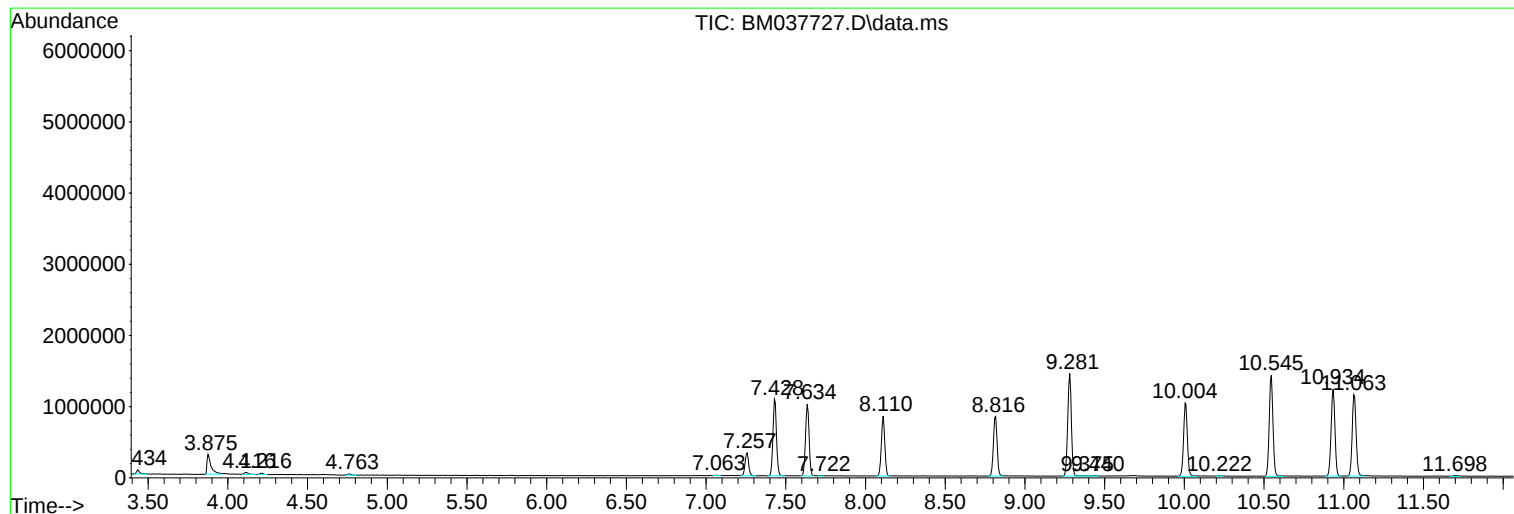

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037727.D
Acq On : 26 Nov 2022 11:12
Operator : CG/JU
Sample : N5592-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037727.D
Acq On : 26 Nov 2022 11:12
Operator : CG/JU
Sample : N5592-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc