

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037728.D
 Acq On : 26 Nov 2022 11:49
 Operator : CG/JU
 Sample : N5592-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	5	8	17	rVB	56892	81589	0.86%	0.099%
2	3.875	80	83	99	rBV	266835	486108	5.13%	0.591%
3	4.110	120	123	130	rVB	29300	49165	0.52%	0.060%
4	4.210	137	140	146	rVB3	16878	25830	0.27%	0.031%
5	5.351	330	334	340	rVB3	13262	20089	0.21%	0.024%
6	7.069	622	626	630	rBV6	6722	10529	0.11%	0.013%
7	7.257	652	658	667	rVB	369469	578188	6.10%	0.703%
8	7.428	681	687	696	rBV	1099328	1750604	18.47%	2.128%
9	7.634	714	722	731	rBV	1120362	1747496	18.43%	2.124%
10	7.722	733	737	745	rVB9	9178	17478	0.18%	0.021%
11	8.110	796	803	810	rBV	920098	1429294	15.08%	1.737%
12	8.169	810	813	817	rVB4	9733	16174	0.17%	0.020%
13	8.816	914	923	935	rBV	982163	1550035	16.35%	1.884%
14	9.280	994	1002	1011	rBV	1513798	2417362	25.50%	2.938%
15	9.375	1014	1018	1023	rVV5	13115	24697	0.26%	0.030%
16	9.445	1025	1030	1034	rVB7	6483	10842	0.11%	0.013%
17	9.686	1068	1071	1077	rVB3	9471	15938	0.17%	0.019%
18	10.010	1117	1126	1136	rBV	1115857	1854710	19.56%	2.254%
19	10.545	1209	1217	1225	rBV	1630044	2623772	27.68%	3.189%
20	10.933	1275	1283	1290	rBV	1381940	2265153	23.89%	2.753%
21	11.004	1290	1295	1299	rVV3	11826	21361	0.23%	0.026%
22	11.063	1299	1305	1317	rVB	1086464	1838874	19.40%	2.235%
23	11.698	1408	1413	1416	rBV7	12263	19643	0.21%	0.024%
24	11.739	1416	1420	1426	rVB7	8682	16791	0.18%	0.020%
25	12.174	1486	1494	1502	rVB4	8250	20451	0.22%	0.025%
26	12.316	1512	1518	1524	rBV5	22814	45283	0.48%	0.055%
27	12.504	1545	1550	1555	rVB3	30243	47338	0.50%	0.058%
28	13.104	1647	1652	1656	rBV6	9074	15012	0.16%	0.018%
29	13.345	1689	1693	1698	rBV5	19445	28366	0.30%	0.034%
30	13.480	1710	1716	1721	rBV8	7080	14588	0.15%	0.018%
31	13.627	1736	1741	1747	rBV2	25799	39191	0.41%	0.048%
32	13.715	1747	1756	1762	rBV10	6961	14141	0.15%	0.017%
33	14.139	1821	1828	1834	rBV	3329475	4692322	49.50%	5.704%
34	14.374	1862	1868	1871	rBV8	10751	20646	0.22%	0.025%
35	14.433	1871	1878	1885	rBV	3652007	5168352	54.52%	6.282%
36	14.621	1903	1910	1916	rVB9	10619	21699	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037728.D
 Acq On : 26 Nov 2022 11:49
 Operator : CG/JU
 Sample : N5592-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	14.733	1922	1929	1939	rBV	2064297	3046279	32.13%	3.703%
38	14.862	1944	1951	1953	rVV7	7621	18336	0.19%	0.022%
39	14.910	1953	1959	1972	rVV	464593	707166	7.46%	0.860%
40	15.010	1972	1976	1981	rVB2	29595	46964	0.50%	0.057%
41	15.086	1986	1989	1993	rVV6	8854	14997	0.16%	0.018%
42	15.139	1993	1998	2004	rVB8	27960	47352	0.50%	0.058%
43	15.521	2060	2063	2068	rBV4	7403	15604	0.16%	0.019%
44	15.562	2068	2070	2074	rVB3	13743	16017	0.17%	0.019%
45	15.721	2088	2097	2108	rBV	4805071	6767958	71.39%	8.227%
46	15.827	2109	2115	2129	rVV	1631985	2245463	23.69%	2.729%
47	15.957	2132	2137	2142	rVB4	24997	47871	0.50%	0.058%
48	16.080	2154	2158	2161	rBV5	5728	9517	0.10%	0.012%
49	16.415	2209	2215	2223	rBV8	23670	50791	0.54%	0.062%
50	16.856	2286	2290	2296	rVB7	13244	15396	0.16%	0.019%
51	16.933	2300	2303	2307	rVB5	10200	12798	0.13%	0.016%
52	17.145	2336	2339	2343	rBV6	9673	11786	0.12%	0.014%
53	17.215	2347	2351	2355	rVV3	19472	27937	0.29%	0.034%
54	17.262	2355	2359	2366	rVB8	12626	23603	0.25%	0.029%
55	17.468	2388	2394	2401	rBV	2447778	3525885	37.19%	4.286%
56	17.574	2405	2412	2424	rVV	5814079	8154309	86.01%	9.912%
57	17.845	2454	2458	2464	rBV3	11124	19846	0.21%	0.024%
58	18.127	2502	2506	2512	rVB	92557	118662	1.25%	0.144%
59	18.345	2538	2543	2550	rBV	232565	329147	3.47%	0.400%
60	18.421	2554	2556	2563	rVB2	23524	35464	0.37%	0.043%
61	18.839	2625	2627	2632	rVB5	16722	20803	0.22%	0.025%
62	19.415	2721	2725	2730	rVB3	78155	104621	1.10%	0.127%
63	19.486	2732	2737	2741	rBV	88534	143085	1.51%	0.174%
64	19.609	2754	2758	2766	rBV2	143630	203317	2.14%	0.247%
65	19.850	2793	2799	2809	rBV	7075682	9278365	97.87%	11.278%
66	20.821	2962	2964	2968	rVB	82797	76002	0.80%	0.092%
67	21.321	3046	3049	3058	rBV	264686	339547	3.58%	0.413%
68	21.633	3097	3102	3109	rBV2	3029411	3928527	41.44%	4.775%
69	22.762	3291	3294	3299	rVB	157782	212569	2.24%	0.258%
70	22.909	3316	3319	3327	rVB	320759	461659	4.87%	0.561%
71	23.968	3491	3499	3514	rVB2	4560087	9480267	100.00%	11.523%
72	24.127	3519	3526	3536	rVB2	1816522	3712869	39.16%	4.513%




Sum of corrected areas: 82269890

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037728.D
Acq On : 26 Nov 2022 11:49
Operator : CG/JU
Sample : N5592-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

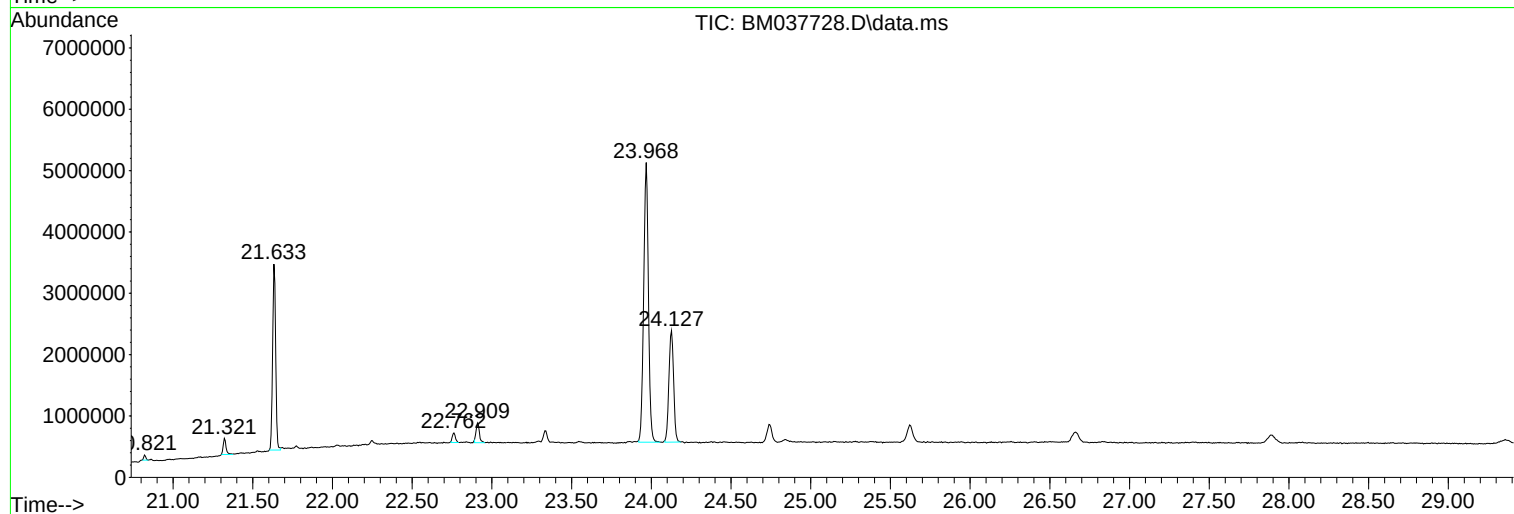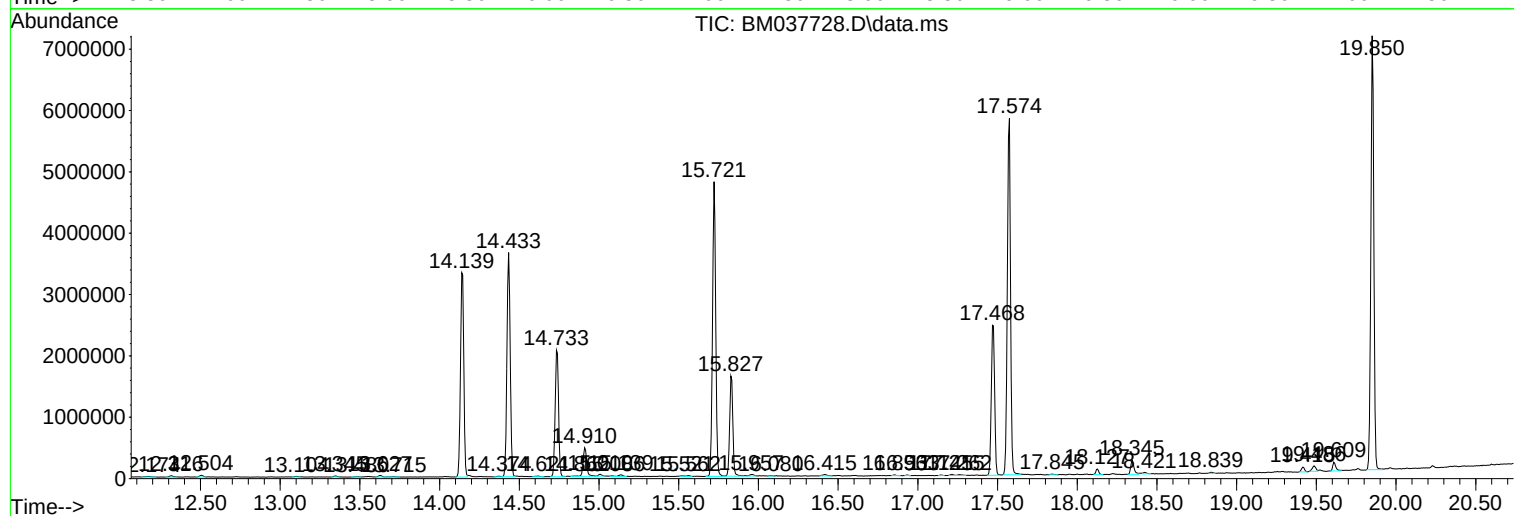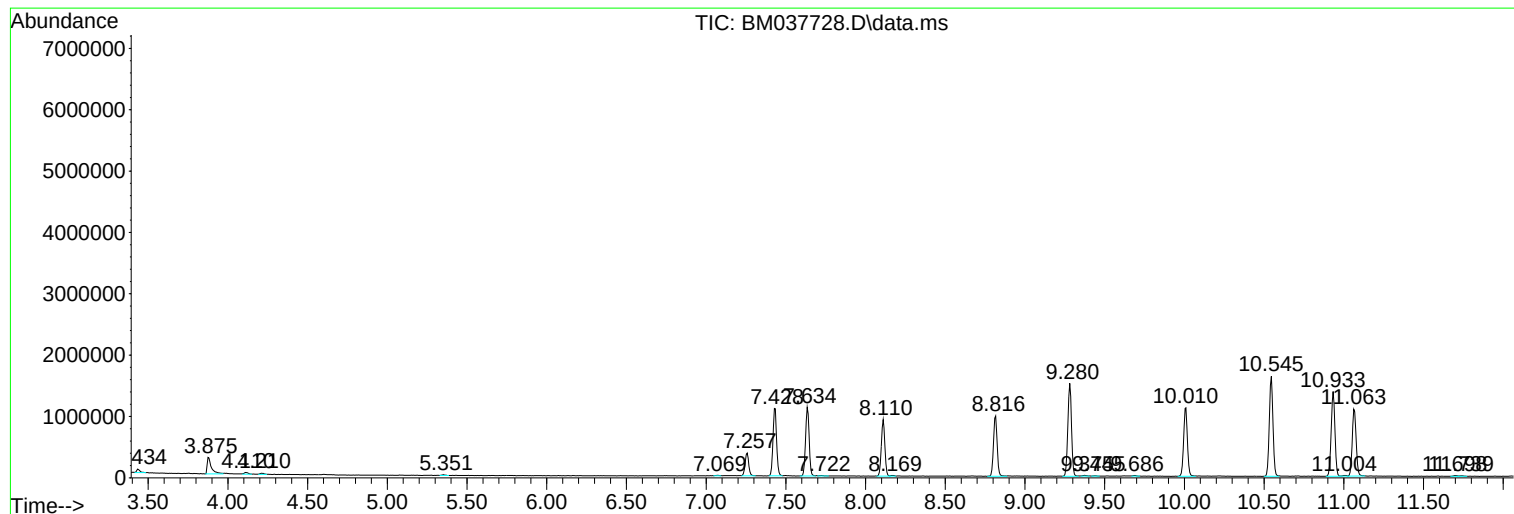

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037728.D
Acq On : 26 Nov 2022 11:49
Operator : CG/JU
Sample : N5592-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,3,5-Trimethyl-2,3,5-hexan... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.909	2.49 ng/ul	461659	Perylene-d12	24.127

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,3,5-Trimethyl-2,3,5-hexanetric...	203	C12H17N3	003974-79-6	64		
2	1,5-Heptadiene, 3,3,6-trimethyl-	138	C10H18	035387-63-4	58		
3	Propanoic acid, 2,2-dimethyl-, [...	306	C20H34O2	1000164-38-8	56		
4	4-Methyl-1,5-Heptadiene	110	C8H14	000998-94-7	53		
5	1,5-Heptadiene, 3,3,6-trimethyl-	138	C10H18	035387-63-4	53		

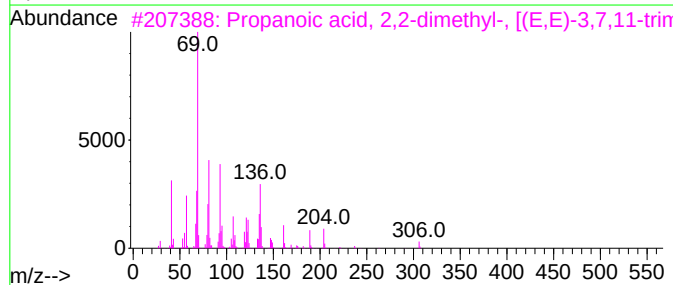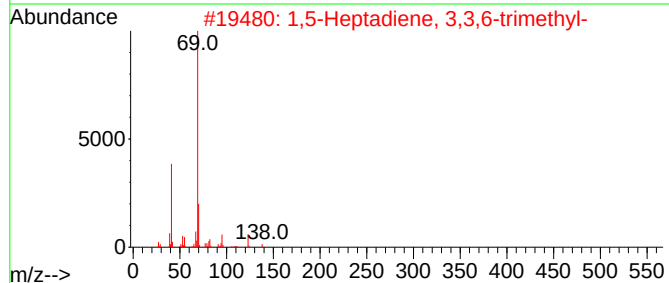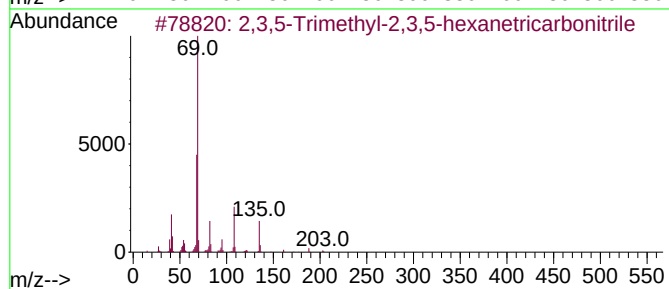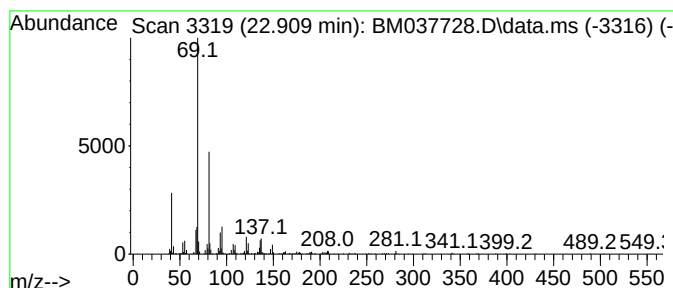

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037728.D
Acq On : 26 Nov 2022 11:49
Operator : CG/JU
Sample : N5592-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,3,5-Trimethyl...	22.909	2.5	ng/u1	461659	6	24.127	3712870	20.0