

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037732.D
 Acq On : 26 Nov 2022 14:17
 Operator : CG/JU
 Sample : PB149109BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK109

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	14	rBV	90830	123068	2.04%	0.178%
2	3.869	78	82	98	rBV	892680	1461354	24.19%	2.113%
3	4.210	137	140	145	rBV2	19554	25401	0.42%	0.037%
4	7.257	649	658	666	rBV	1239617	1926243	31.89%	2.785%
5	7.428	680	687	697	rVB	937726	1478144	24.47%	2.137%
6	7.634	715	722	730	rBV	1168138	1789946	29.63%	2.588%
7	8.110	796	803	811	rVB	913433	1408520	23.32%	2.037%
8	8.816	915	923	932	rBV	1470493	2289143	37.90%	3.310%
9	9.280	993	1002	1011	rBV	1247123	2000635	33.12%	2.893%
10	10.004	1118	1125	1133	rBV	948763	1578737	26.14%	2.283%
11	10.545	1210	1217	1230	rBV	1404616	2241940	37.11%	3.242%
12	10.933	1275	1283	1290	rBV	1354780	2261997	37.45%	3.271%
13	11.069	1297	1306	1319	rBV	1474688	2521204	41.74%	3.646%
14	11.704	1409	1414	1418	rBV7	5434	9376	0.16%	0.014%
15	12.174	1488	1494	1498	rVV4	12132	23155	0.38%	0.033%
16	12.504	1546	1550	1557	rVB2	25820	41588	0.69%	0.060%
17	13.086	1644	1649	1655	rBV7	4758	10828	0.18%	0.016%
18	14.139	1822	1828	1838	rBV	2598005	3528878	58.42%	5.103%
19	14.433	1869	1878	1886	rBV	2876006	4131447	68.40%	5.974%
20	14.739	1921	1930	1939	rBV	2047341	3092574	51.20%	4.472%
21	14.804	1939	1941	1945	rVB5	4186	6094	0.10%	0.009%
22	14.915	1952	1960	1975	rBV	1548143	2233521	36.98%	3.230%
23	15.133	1994	1997	2004	rVB8	10523	17910	0.30%	0.026%
24	15.721	2085	2097	2105	rBV	3612702	5042051	83.47%	7.291%
25	15.833	2109	2116	2133	rVV	1172521	1651508	27.34%	2.388%
26	15.962	2133	2138	2141	rVB6	17262	26470	0.44%	0.038%
27	16.427	2215	2217	2221	rBV5	4338	6509	0.11%	0.009%
28	16.509	2226	2231	2234	rVB7	5964	9161	0.15%	0.013%
29	16.933	2300	2303	2308	rVV4	8221	11628	0.19%	0.017%
30	17.474	2388	2395	2401	rBV	2526656	3550682	58.78%	5.134%
31	17.574	2405	2412	2424	rVV	3895195	5543397	91.77%	8.016%
32	18.003	2483	2485	2492	rVB7	9626	12355	0.20%	0.018%
33	18.345	2540	2543	2549	rVB7	11852	20723	0.34%	0.030%
34	19.415	2721	2725	2731	rBV4	42495	65721	1.09%	0.095%
35	19.486	2733	2737	2741	rBV	42546	62847	1.04%	0.091%
36	19.762	2781	2784	2788	rVB5	21426	24254	0.40%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037732.D
Acq On : 26 Nov 2022 14:17
Operator : CG/JU
Sample : PB149109BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK109

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Title : SVOA CALIBRATION

37	19.850	2793	2799	2807	rBV	4800220	6040534	100.00%	8.734%
38	20.821	2962	2964	2969	rVB2	71024	72602	1.20%	0.105%
39	21.633	3097	3102	3110	rBV	2832199	3790807	62.76%	5.481%
40	23.968	3491	3499	3509	rVB2	2714110	5693815	94.26%	8.233%
41	24.127	3519	3526	3537	rVB2	1620244	3331384	55.15%	4.817%




Sum of corrected areas: 69158151

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037732.D
Acq On : 26 Nov 2022 14:17
Operator : CG/JU
Sample : PB149109BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK109

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

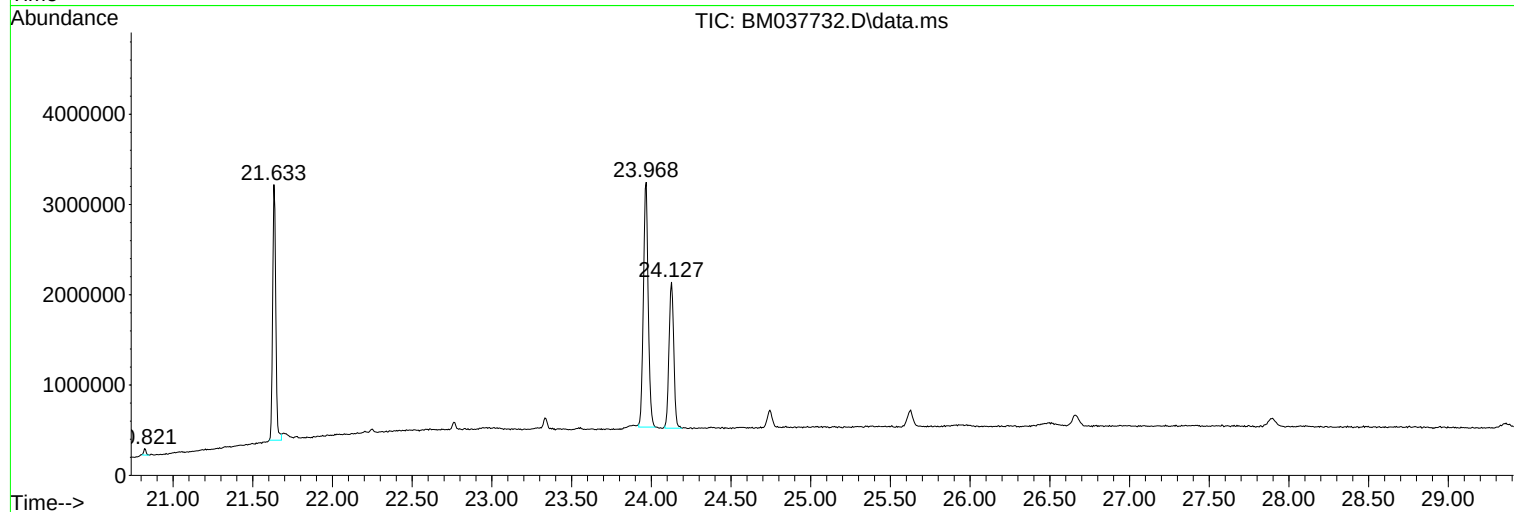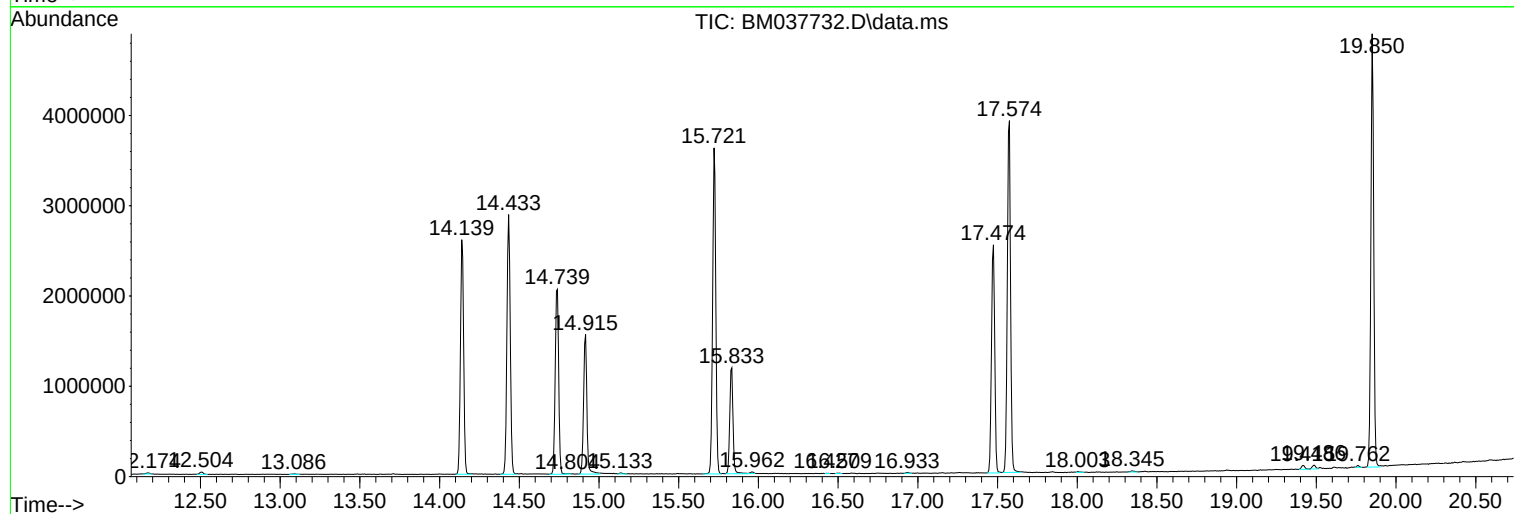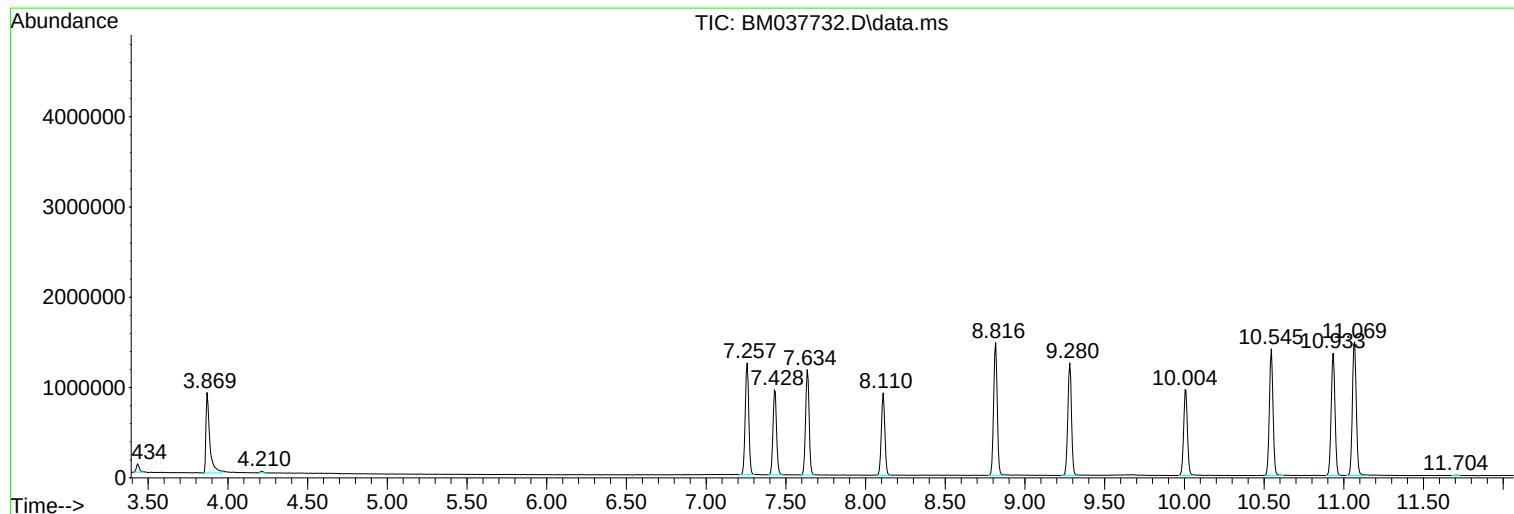

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037732.D
Acq On : 26 Nov 2022 14:17
Operator : CG/JU
Sample : PB149109BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK109

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037732.D
Acq On : 26 Nov 2022 14:17
Operator : CG/JU
Sample : PB149109BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK109

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc