

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037736.D
 Acq On : 26 Nov 2022 16:52
 Operator : CG/JU
 Sample : N5602-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	12	rBV	49580	63830	0.78%	0.088%
2	3.875	80	83	102	rBV	219448	411246	5.01%	0.568%
3	4.111	120	123	128	rVB	28166	42907	0.52%	0.059%
4	4.211	137	140	150	rVB2	17117	27088	0.33%	0.037%
5	5.169	299	303	313	rVB	28211	48928	0.60%	0.068%
6	7.258	651	658	666	rVB	390338	605869	7.39%	0.837%
7	7.428	681	687	697	rBV	1048364	1632065	19.90%	2.255%
8	7.634	715	722	730	rBV	1082001	1660125	20.24%	2.294%
9	8.110	796	803	810	rBV	740414	1147438	13.99%	1.586%
10	8.816	915	923	932	rBV	994456	1565016	19.08%	2.163%
11	9.281	994	1002	1011	rBV	1450902	2292178	27.95%	3.168%
12	10.004	1116	1125	1135	rBV	1103857	1840303	22.44%	2.543%
13	10.546	1208	1217	1228	rBV	1553623	2545236	31.04%	3.517%
14	10.699	1241	1243	1246	rBV4	7443	9142	0.11%	0.013%
15	10.934	1272	1283	1290	rBV	1097025	1828470	22.30%	2.527%
16	11.063	1296	1305	1316	rBV	1088659	1831699	22.34%	2.531%
17	11.698	1410	1413	1419	rVB5	8582	13246	0.16%	0.018%
18	12.175	1488	1494	1500	rVB4	9782	20995	0.26%	0.029%
19	12.504	1544	1550	1556	rBV	30887	46072	0.56%	0.064%
20	12.998	1631	1634	1639	rBV6	5422	9010	0.11%	0.012%
21	13.710	1751	1755	1759	rVB5	6768	9410	0.11%	0.013%
22	14.139	1821	1828	1834	rBV	3135924	4286285	52.27%	5.923%
23	14.434	1871	1878	1887	rBV	3486963	5025067	61.27%	6.944%
24	14.734	1923	1929	1937	rBV	1729106	2539300	30.96%	3.509%
25	14.810	1938	1942	1948	rVB9	10333	17046	0.21%	0.024%
26	14.910	1953	1959	1970	rBV	462968	690805	8.42%	0.955%
27	15.081	1983	1988	1992	rBV8	9960	20434	0.25%	0.028%
28	15.134	1992	1997	2005	rVB5	32047	57561	0.70%	0.080%
29	15.722	2087	2097	2108	rBV	4587230	6286783	76.66%	8.688%
30	15.828	2109	2115	2126	rBV	1643176	2209285	26.94%	3.053%
31	15.957	2132	2137	2143	rVB4	22145	36790	0.45%	0.051%
32	16.386	2204	2210	2211	rBV	140799	207771	2.53%	0.287%
33	16.398	2211	2212	2222	rVB	164518	191304	2.33%	0.264%
34	16.716	2261	2266	2269	rBV7	6463	13860	0.17%	0.019%
35	16.933	2300	2303	2307	rVB2	9590	12001	0.15%	0.017%
36	17.475	2388	2395	2401	rBV	2106281	3018875	36.81%	4.172%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037736.D
 Acq On : 26 Nov 2022 16:52
 Operator : CG/JU
 Sample : N5602-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	17.575	2405	2412	2426	rVV	4847171	7055719	86.04%	9.750%
38	18.345	2539	2543	2552	rBV2	68230	98885	1.21%	0.137%
39	19.416	2722	2725	2731	rVB2	68775	84318	1.03%	0.117%
40	19.480	2732	2736	2741	rBV2	64876	101762	1.24%	0.141%
41	19.610	2755	2758	2763	rBV2	77034	99368	1.21%	0.137%
42	19.851	2793	2799	2810	rBV	6482371	8200982	100.00%	11.333%
43	20.821	2962	2964	2969	rVB	81880	86758	1.06%	0.120%
44	21.633	3097	3102	3108	rBV	2563219	3382767	41.25%	4.675%
45	23.968	3492	3499	3509	rVB2	3810279	7860334	95.85%	10.862%
46	24.127	3519	3526	3538	rVB2	1507929	3129824	38.16%	4.325%




Sum of corrected areas: 72364157

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037736.D
Acq On : 26 Nov 2022 16:52
Operator : CG/JU
Sample : N5602-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

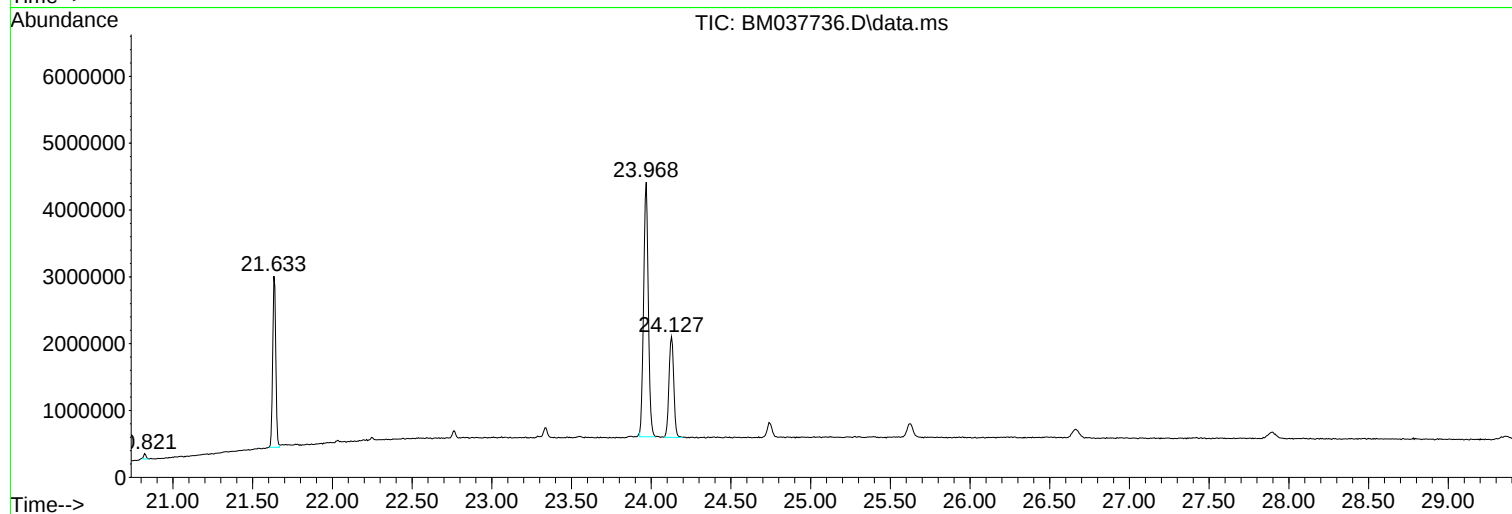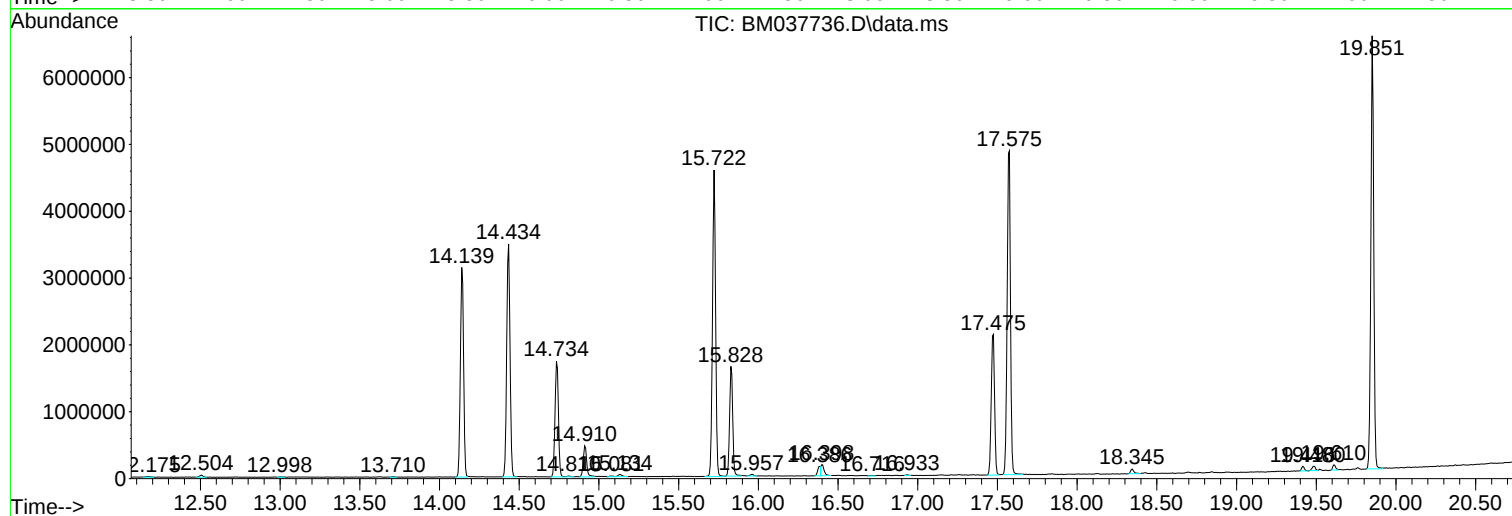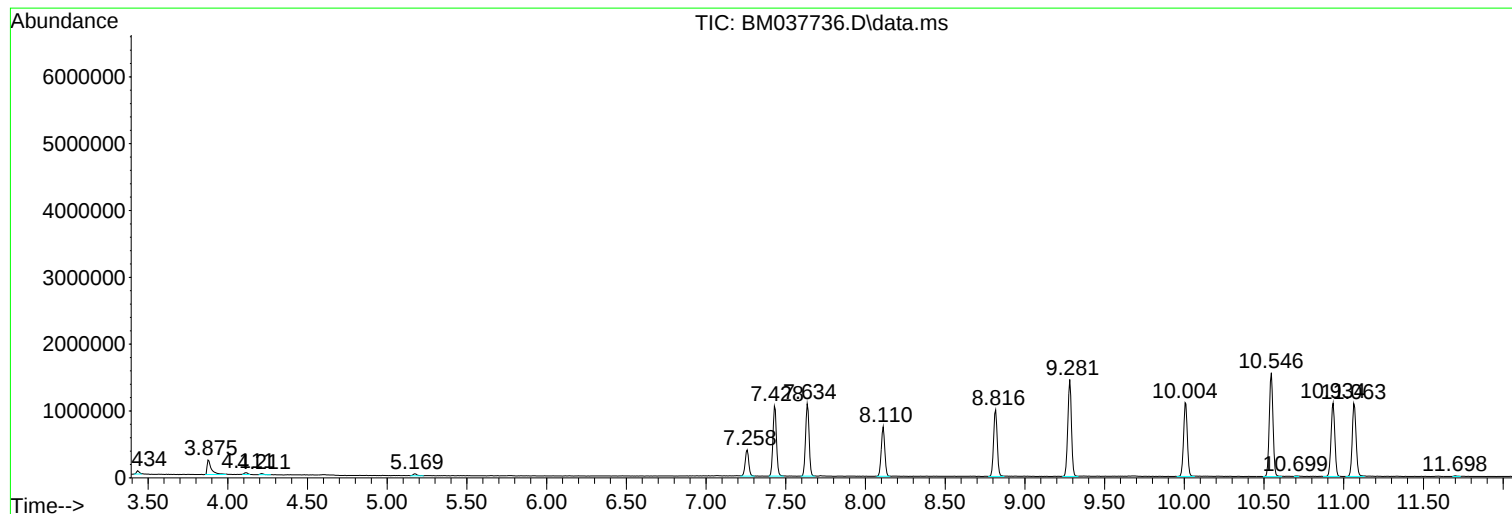

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037736.D
Acq On : 26 Nov 2022 16:52
Operator : CG/JU
Sample : N5602-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037736.D
Acq On : 26 Nov 2022 16:52
Operator : CG/JU
Sample : N5602-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc