

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037737.D
 Acq On : 26 Nov 2022 17:29
 Operator : CG/JU
 Sample : N5602-14
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rBV	51436	74869	1.02%	0.110%
2	3.881	81	84	97	rBV	138771	259898	3.54%	0.380%
3	4.116	118	124	129	rBV2	31992	52503	0.72%	0.077%
4	4.216	137	141	145	rBV2	19358	29706	0.40%	0.043%
5	4.599	203	206	210	rVB6	7476	10436	0.14%	0.015%
6	5.175	299	304	310	rVB	30783	47115	0.64%	0.069%
7	5.351	330	334	339	rVB2	17575	25304	0.34%	0.037%
8	7.257	651	658	666	rVB	407180	625621	8.52%	0.916%
9	7.428	681	687	696	rBV	981452	1520806	20.72%	2.226%
10	7.634	714	722	729	rBV	1034598	1600929	21.81%	2.343%
11	8.110	794	803	810	rBV	877740	1353919	18.45%	1.982%
12	8.169	810	813	817	rVB6	6827	7847	0.11%	0.011%
13	8.816	916	923	932	rBV	979437	1546244	21.07%	2.263%
14	9.186	981	986	990	rBV	10015	14539	0.20%	0.021%
15	9.281	995	1002	1013	rVV	1322432	2154204	29.35%	3.153%
16	10.004	1118	1125	1138	rBV	1036659	1700603	23.17%	2.489%
17	10.545	1209	1217	1227	rBV	1515953	2449145	33.37%	3.585%
18	10.710	1240	1245	1248	rBV6	5625	9203	0.13%	0.013%
19	10.792	1253	1259	1261	rBV7	5108	11353	0.15%	0.017%
20	10.933	1275	1283	1291	rBV	1281180	2151129	29.31%	3.149%
21	11.063	1298	1305	1318	rBV	743198	1251728	17.05%	1.832%
22	11.704	1407	1414	1417	rBV5	13261	22603	0.31%	0.033%
23	11.739	1417	1420	1425	rVV7	6760	12167	0.17%	0.018%
24	11.804	1428	1431	1437	rVB8	5818	9325	0.13%	0.014%
25	12.169	1485	1493	1499	rBV6	10934	26869	0.37%	0.039%
26	12.504	1545	1550	1556	rBV2	27009	41196	0.56%	0.060%
27	13.092	1644	1650	1653	rBV8	4685	8494	0.12%	0.012%
28	13.274	1677	1681	1685	rVB7	5905	7877	0.11%	0.012%
29	14.139	1820	1828	1834	rBV	2861729	3928019	53.52%	5.750%
30	14.433	1870	1878	1885	rBV	3260484	4644258	63.27%	6.798%
31	14.733	1922	1929	1937	rBV	1991298	2885965	39.32%	4.224%
32	14.804	1939	1941	1949	rVB9	13454	21098	0.29%	0.031%
33	14.916	1954	1960	1969	rBV	420097	636690	8.67%	0.932%
34	15.074	1983	1987	1992	rBV4	19180	33482	0.46%	0.049%
35	15.133	1994	1997	2002	rVV6	18747	26862	0.37%	0.039%
36	15.721	2090	2097	2108	rVB	4092735	5728079	78.04%	8.385%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037737.D
Acq On : 26 Nov 2022 17:29
Operator : CG/JU
Sample : N5602-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Title : SVOA CALIBRATION

37	15.827	2109	2115	2127	rBV	1431335	1977574	26.94%	2.895%
38	17.474	2389	2395	2401	rBV	2400181	3382809	46.09%	4.952%
39	17.568	2405	2411	2421	rBV	4333507	6231719	84.90%	9.122%
40	18.345	2539	2543	2550	rBV	131623	205225	2.80%	0.300%
41	19.615	2755	2759	2768	rBV	175849	260226	3.55%	0.381%
42	19.851	2794	2799	2806	rVB	5732074	7339861	100.00%	10.744%
43	21.639	3098	3103	3110	rBV	3062764	3823074	52.09%	5.596%
44	23.968	3492	3499	3517	rVB2	3120583	6850323	93.33%	10.027%
45	24.133	3520	3527	3541	rVB2	1612045	3315541	45.17%	4.853%




Sum of corrected areas: 68316437

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037737.D
Acq On : 26 Nov 2022 17:29
Operator : CG/JU
Sample : N5602-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

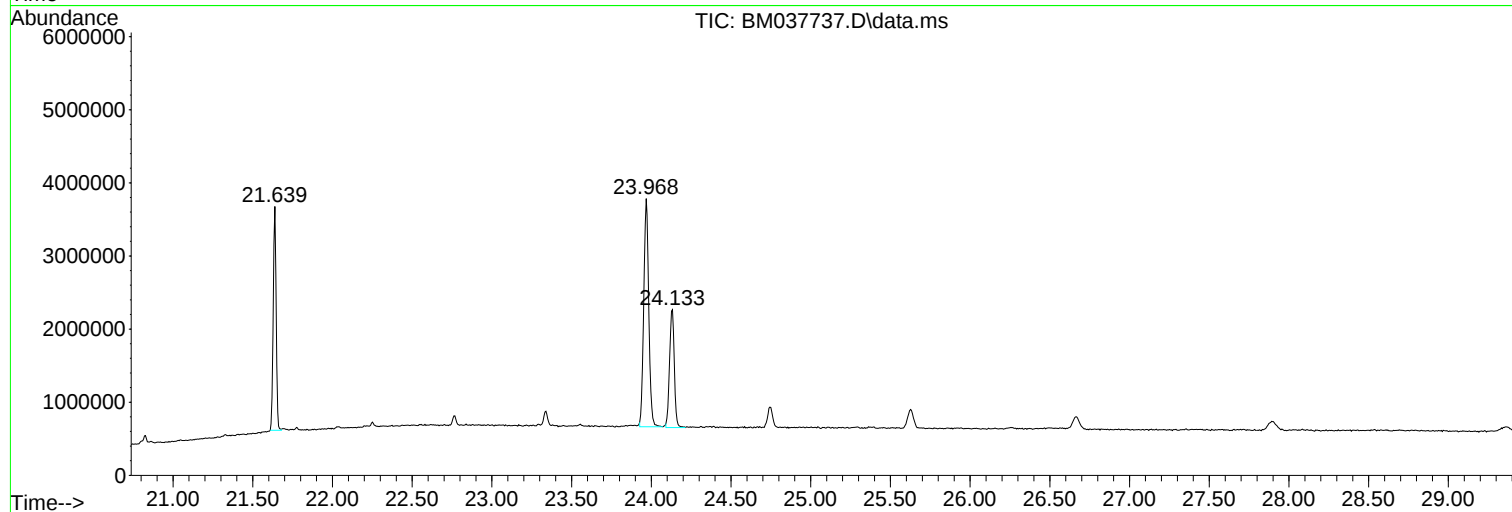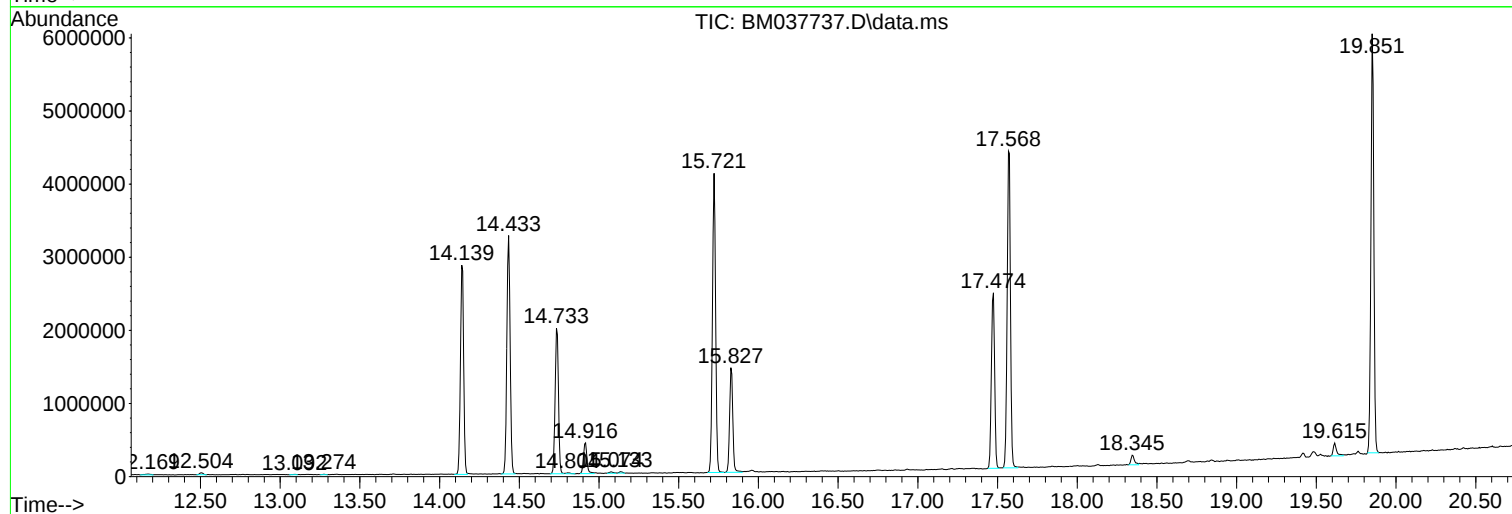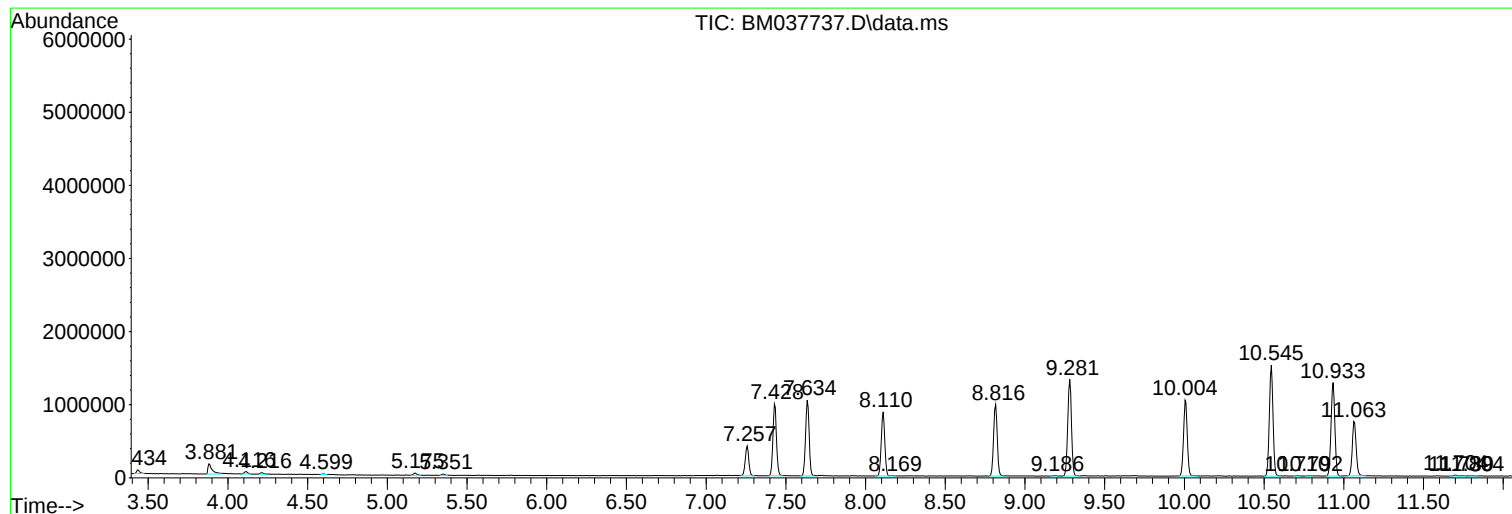

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037737.D
Acq On : 26 Nov 2022 17:29
Operator : CG/JU
Sample : N5602-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037737.D
Acq On : 26 Nov 2022 17:29
Operator : CG/JU
Sample : N5602-14
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc