

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037738.D
 Acq On : 26 Nov 2022 18:06
 Operator : CG/JU
 Sample : N5602-15
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	13	rBV	54853	75023	0.83%	0.092%
2	3.881	80	84	103	rBV	225207	429530	4.75%	0.528%
3	4.111	119	123	131	rVB	38227	61708	0.68%	0.076%
4	4.211	136	140	145	rBV2	20496	30225	0.33%	0.037%
5	4.599	204	206	211	rVB5	8413	9919	0.11%	0.012%
6	4.963	263	268	271	rBV6	4222	9317	0.10%	0.011%
7	5.169	298	303	310	rVB	160951	224221	2.48%	0.276%
8	5.352	330	334	339	rVB7	6080	10633	0.12%	0.013%
9	5.958	434	437	443	rVB7	12264	22652	0.25%	0.028%
10	6.181	470	475	479	rBV7	5023	11102	0.12%	0.014%
11	6.393	507	511	514	rVB6	7094	9686	0.11%	0.012%
12	7.257	650	658	667	rVB	461386	718582	7.95%	0.884%
13	7.428	679	687	698	rBV	1234062	1895729	20.98%	2.332%
14	7.634	715	722	729	rBV	1307762	2009794	22.24%	2.472%
15	7.705	731	734	740	rVB4	14449	24177	0.27%	0.030%
16	8.110	796	803	809	rBV	983466	1537778	17.02%	1.892%
17	8.816	916	923	931	rBV	1182406	1846698	20.44%	2.272%
18	8.999	949	954	960	rBV10	8959	23300	0.26%	0.029%
19	9.122	968	975	980	rBV10	5130	12451	0.14%	0.015%
20	9.181	980	985	993	rBV	15506	29504	0.33%	0.036%
21	9.281	993	1002	1012	rBV	1660101	2658408	29.42%	3.270%
22	9.934	1109	1113	1114	rBV4	8245	11089	0.12%	0.014%
23	10.004	1119	1125	1137	rVV	1313659	2133496	23.61%	2.625%
24	10.128	1140	1146	1148	rVV5	6234	12370	0.14%	0.015%
25	10.210	1155	1160	1167	rVB6	12558	25138	0.28%	0.031%
26	10.546	1209	1217	1233	rVB	1893079	3019332	33.41%	3.714%
27	10.710	1240	1245	1250	rBB7	5526	9731	0.11%	0.012%
28	10.787	1253	1258	1266	rBV7	11952	27982	0.31%	0.034%
29	10.934	1276	1283	1290	rBV	1446204	2401380	26.57%	2.954%
30	11.063	1299	1305	1323	rVB	794833	1389717	15.38%	1.710%
31	11.510	1377	1381	1388	rVB9	12570	22064	0.24%	0.027%
32	11.698	1406	1413	1418	rBV8	18770	42365	0.47%	0.052%
33	11.792	1425	1429	1431	rBV5	13159	18780	0.21%	0.023%
34	12.175	1490	1494	1499	rVB3	19514	34031	0.38%	0.042%
35	12.475	1541	1545	1546	rBV3	12924	14001	0.15%	0.017%
36	12.504	1546	1550	1555	rVB2	34640	54782	0.61%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
 Data File : BM037738.D
 Acq On : 26 Nov 2022 18:06
 Operator : CG/JU
 Sample : N5602-15
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
 Title : SVOA CALIBRATION

37	12.687	1577	1581	1586	rBV8	10154	16374	0.18%	0.020%
38	12.781	1590	1597	1598	rBV7	8554	17416	0.19%	0.021%
39	12.839	1604	1607	1610	rBV5	5895	9397	0.10%	0.012%
40	12.916	1616	1620	1623	rVB6	13708	21734	0.24%	0.027%
41	12.963	1624	1628	1629	rBV4	7974	9646	0.11%	0.012%
42	13.275	1676	1681	1687	rVB6	17951	34464	0.38%	0.042%
43	13.463	1709	1713	1719	rBV9	11981	27982	0.31%	0.034%
44	13.586	1729	1734	1736	rBV6	9928	15291	0.17%	0.019%
45	14.139	1822	1828	1835	rBV	3393142	4648128	51.44%	5.718%
46	14.433	1871	1878	1885	rBV	3812616	5516245	61.04%	6.786%
47	14.733	1923	1929	1936	rBV	2230078	3185418	35.25%	3.919%
48	14.804	1937	1941	1948	rVB7	38049	68246	0.76%	0.084%
49	14.916	1954	1960	1968	rBV	513156	748605	8.28%	0.921%
50	15.075	1984	1987	1993	rVB5	35910	56766	0.63%	0.070%
51	15.133	1994	1997	2002	rVB7	23903	33005	0.37%	0.041%
52	15.722	2091	2097	2104	rBV	5022432	6828231	75.56%	8.400%
53	15.828	2110	2115	2122	rBV	1800533	2490163	27.56%	3.063%
54	15.933	2130	2133	2135	rBV	33908	40798	0.45%	0.050%
55	17.469	2389	2394	2400	rBV	2676213	3857933	42.69%	4.746%
56	17.569	2405	2411	2418	rBV	5302973	7698507	85.19%	9.471%
57	18.351	2540	2544	2551	rBV	215217	319966	3.54%	0.394%
58	19.616	2756	2759	2765	rBV	272464	330007	3.65%	0.406%
59	19.851	2794	2799	2807	rVB	6972663	9036740	100.00%	11.117%
60	21.639	3098	3103	3109	rBV	3325278	4182964	46.29%	5.146%
61	23.968	3492	3499	3511	rVB2	3717790	7731956	85.56%	9.512%
62	24.127	3520	3526	3536	rVB2	1760538	3495551	38.68%	4.300%




Sum of corrected areas: 81288228

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037738.D
Acq On : 26 Nov 2022 18:06
Operator : CG/JU
Sample : N5602-15
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

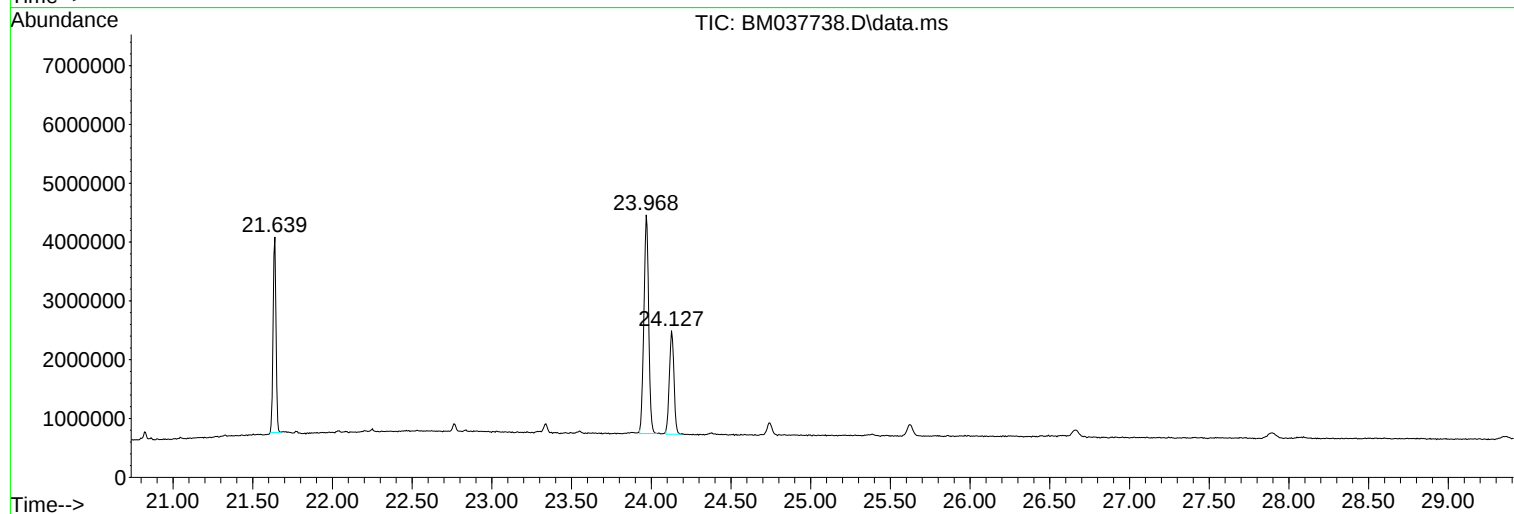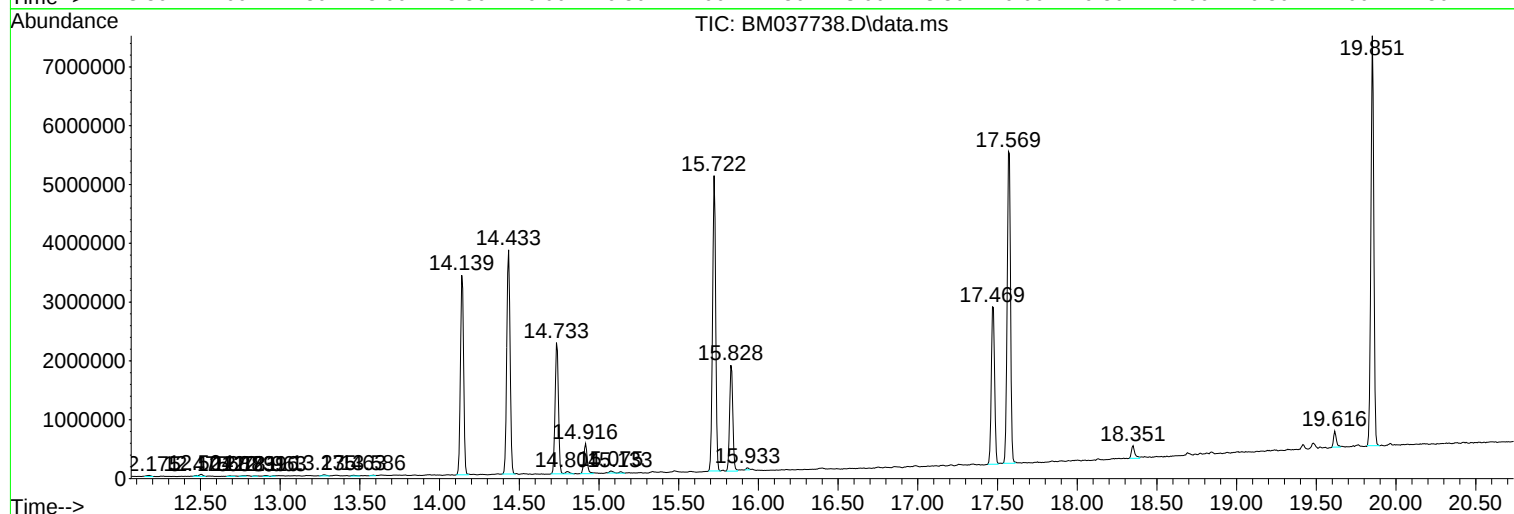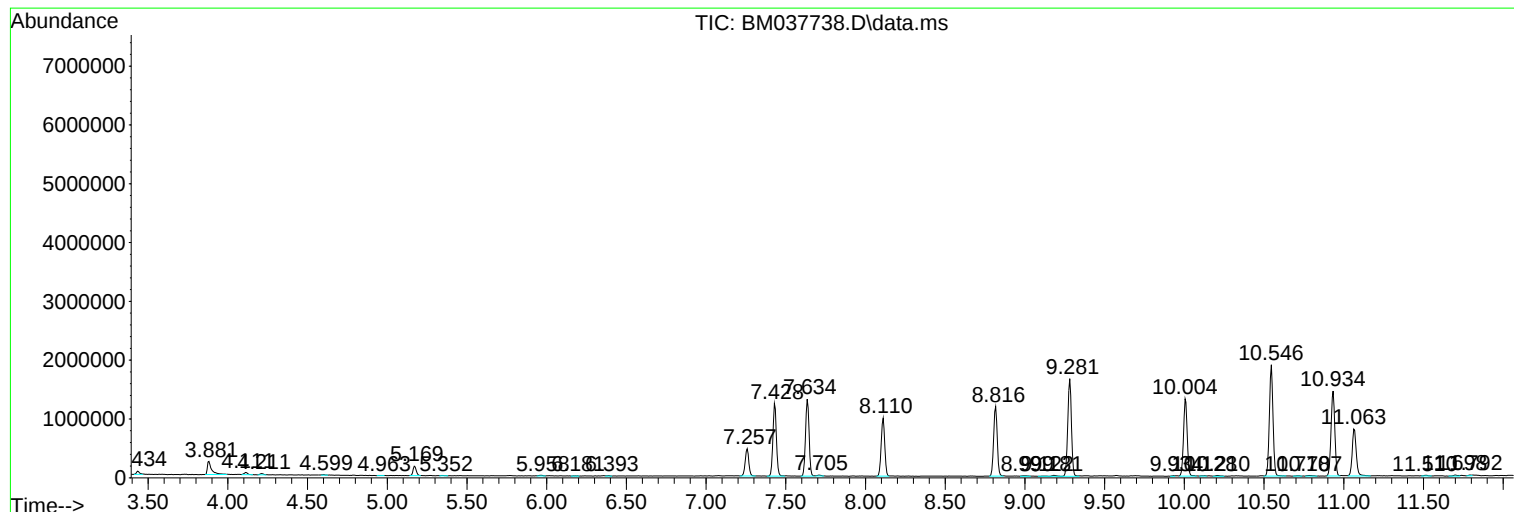

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037738.D
Acq On : 26 Nov 2022 18:06
Operator : CG/JU
Sample : N5602-15
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.169	2.92 ng/ul	224221	1,4-Dichlorobenzene-d4	8.110

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
3	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38		
4	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	28		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16		

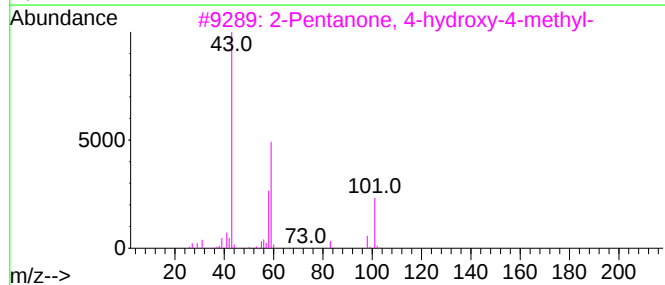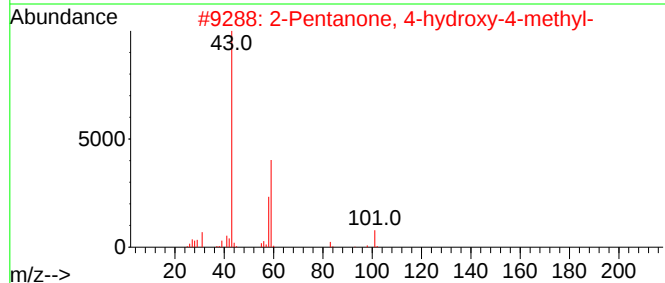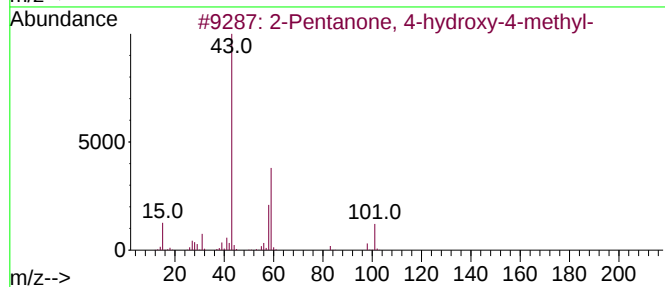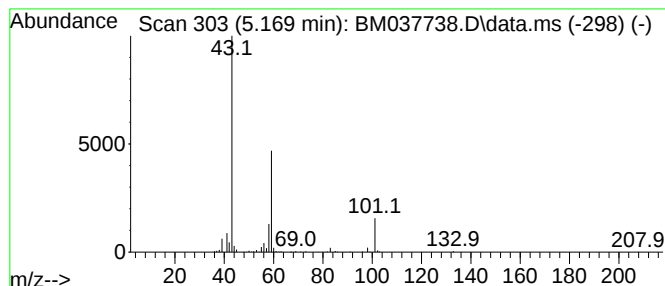

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112522\
Data File : BM037738.D
Acq On : 26 Nov 2022 18:06
Operator : CG/JU
Sample : N5602-15
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM112322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.169	2.9	ng/u1	224221	1	8.110	1537780	20.0