

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112715\
 Data File : BM003314.D
 Acq On : 27 Nov 2015 20:57
 Operator : UM/IZ
 Sample : G4510-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-14A-111815

Quant Time: Nov 28 02:19:34 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM112715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 27 16:36:40 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	52184	5.00	ng	0.00
7) Naphthalene-d8	10.52	136	207608	5.00	ng	0.00
13) Acenaphthene-d10	14.38	164	108443	5.00	ng	0.00
19) Phenanthrene-d10	17.12	188	252794	5.00	ng	0.00
26) Chrysene-d12	21.32	240	218403	5.00	ng	0.00
35) Perylene-d12	23.58	264	172640	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.31	112	37600	3.65	ng	0.00
5) Phenol-d6	6.90	99	30156	2.55	ng	0.00
8) Nitrobenzene-d5	8.90	82	32446	3.51	ng	0.00
14) 2,4,6-Tribromophenol	15.87	330	23413	9.26	ng	0.00
15) 2-Fluorobiphenyl	13.00	172	123297	3.52	ng	0.00
29) Terphenyl-d14	19.76	244	125816	4.13	ng	0.00
Target Compounds						
10) Naphthalene	10.58	128	34043	0.76	ng	# 96
12) 2-Methylnaphthalene	12.19	142	20904	0.74	ng	# 96
18) Fluorene	15.42	166	2175	0.07	ng	# 94
22) Pentachlorophenol	16.79	266	797	0.37	ng	# 82
34) Indeno(1,2,3-cd)pyrene	25.85	276	2781	0.05	ng	# 76
39) Dibenzo(a,h)anthracene	25.88	278	3072	0.09	ng	# 78
40) Benzo(g,h,i)perylene	26.55	276	1542	0.04	ng	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112715\
Data File : BM003314.D
Acq On : 27 Nov 2015 20:57
Operator : UM/IZ
Sample : G4510-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-14A-111815

Quant Time: Nov 28 02:19:34 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM112715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 27 16:36:40 2015
Response via : Initial Calibration

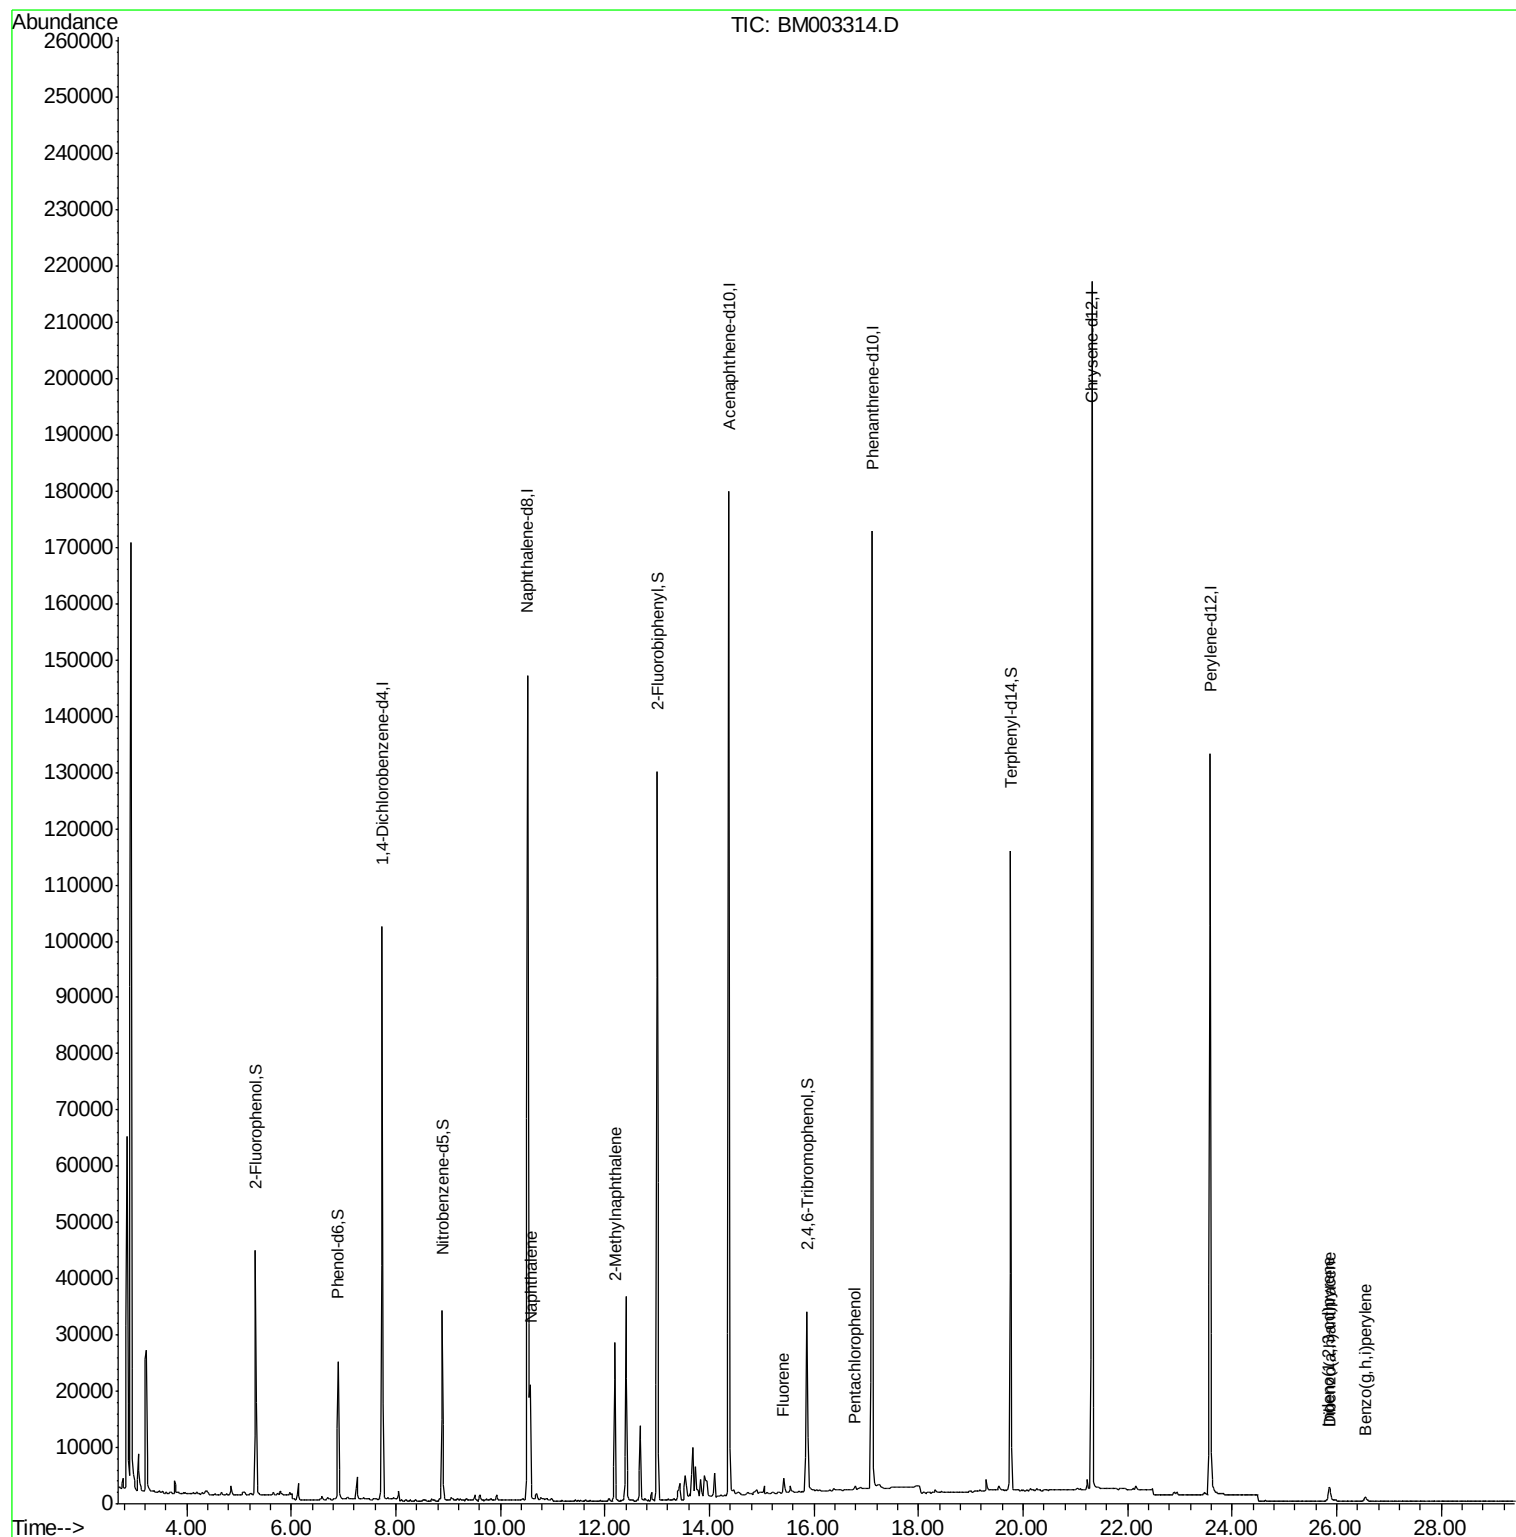

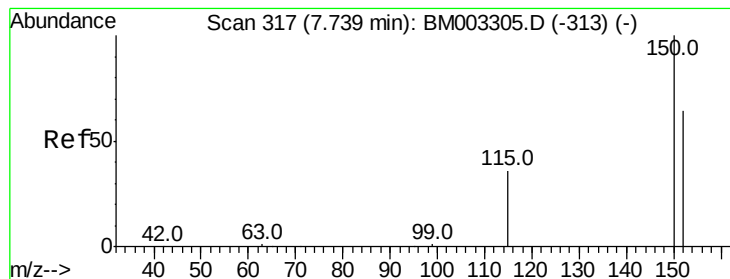

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.74 min Scan# 317

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57

Instrument :

BNA_M

ClientSampleId :

MW-14A-111815


Tot Ion:152 Resp: 52184

Ion Ratio Lower Upper

152 100

150 150.8 143.6 215.4




115 52.3 58.5 87.7#

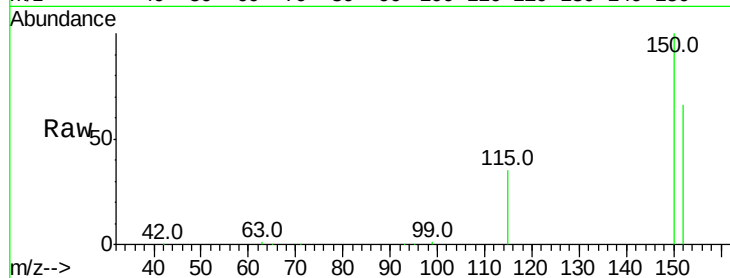

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

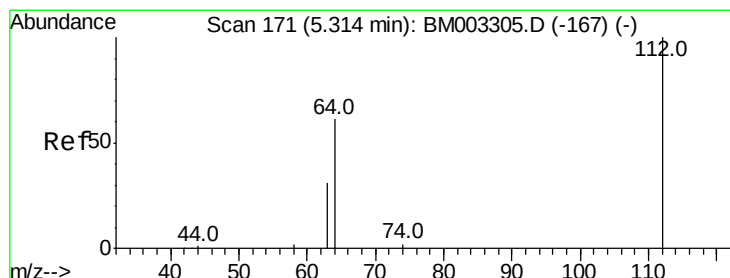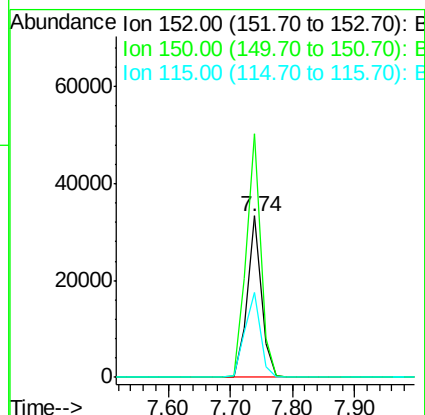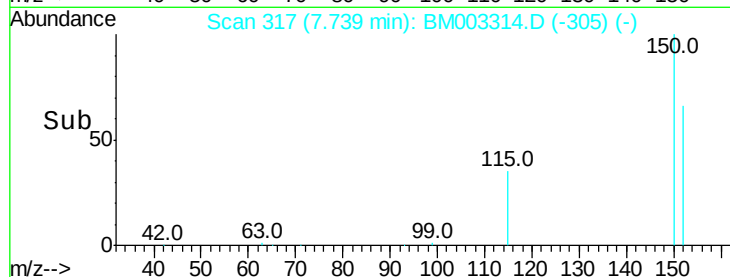

#4

2-Fluorophenol

Concen: 3.65 ng

RT: 5.31 min Scan# 171

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57


Tgt Ion:112 Resp: 37600

Ion Ratio Lower Upper

112 100

64 51.2 41.2 61.8



63 26.6 21.2 31.8

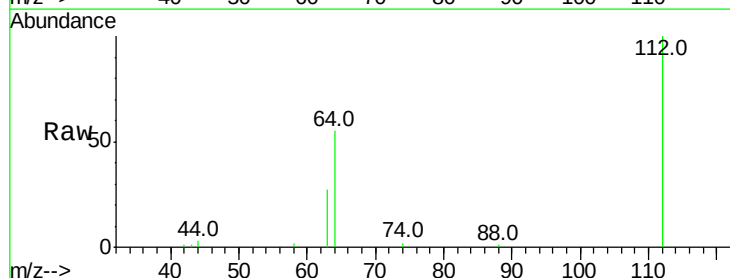


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

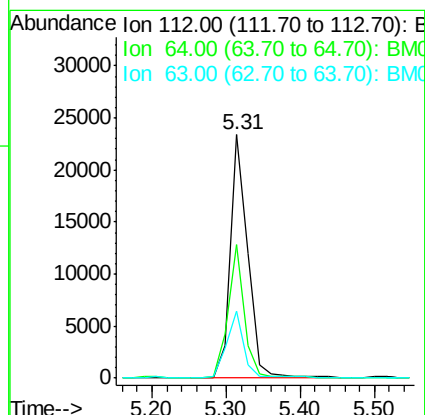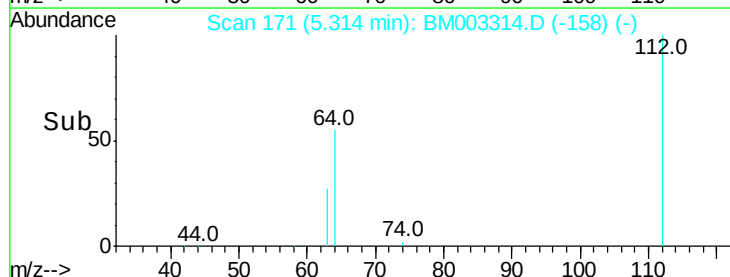



#5

Phenol-d6

Concen: 2.55 ng

RT: 6.90 min Scan# 268

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57

Instrument :

BNA_M

ClientSampleId :

MW-14A-111815


Tot Ion: 99 Resp: 30156

Ion Ratio Lower Upper

99 100

42 17.8 14.6 22.0




71 29.8 23.3 34.9

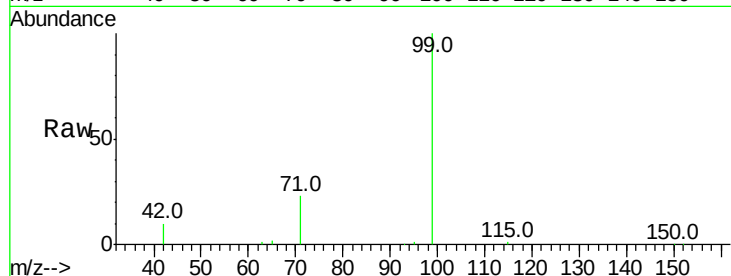

Abundance Ion 99.00 (98.70 to 99.70): BM003314.D (-256) (-)

Ion 42.00 (41.70 to 42.70): BM003314.D (-256) (-)

Ion 71.00 (70.70 to 71.70): BM003314.D (-256) (-)

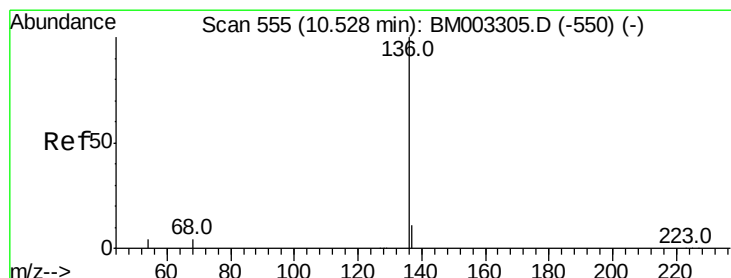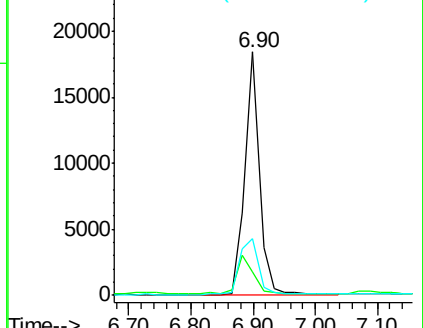

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.52 min Scan# 554

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57

Tgt Ion: 136 Resp: 207608


Ion Ratio Lower Upper

136 100

137 11.1 8.0 12.0

54 4.7 7.4 11.0#

68 4.1 5.8 8.6#


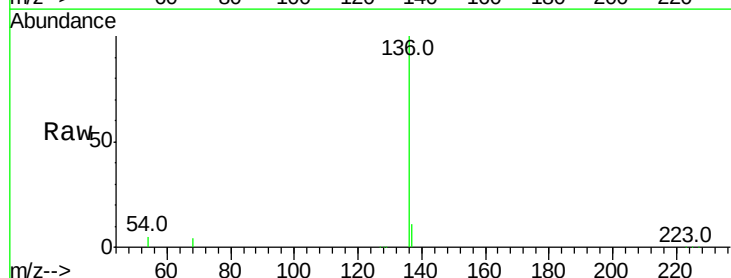



Abundance Ion 136.00 (135.70 to 136.70): BM003314.D (-543) (-)

Ion 137.00 (136.70 to 137.70): BM003314.D (-543) (-)

Ion 54.00 (53.70 to 54.70): BM003314.D (-543) (-)

Ion 68.00 (67.70 to 68.70): BM003314.D (-543) (-)




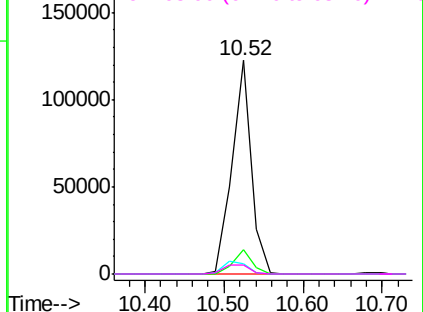




#8
 Nitrobenzene-d5
 Concen: 3.51 ng
 RT: 8.90 min Scan# 417
 Delta R.T. 0.01 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57




Instrument :
 BNA_M
 ClientSampleId :
 MW-14A-111815


Tot Ion	82	Resp	32446
Ion Ratio	Lower	Upper	
82	100		
128	51.1	35.2	52.8
54	36.8	36.4	54.6

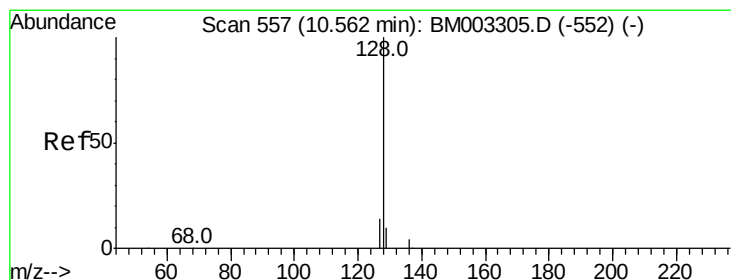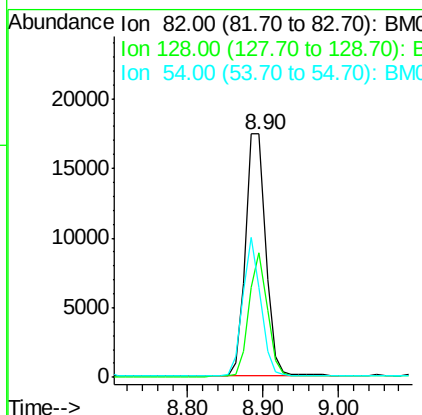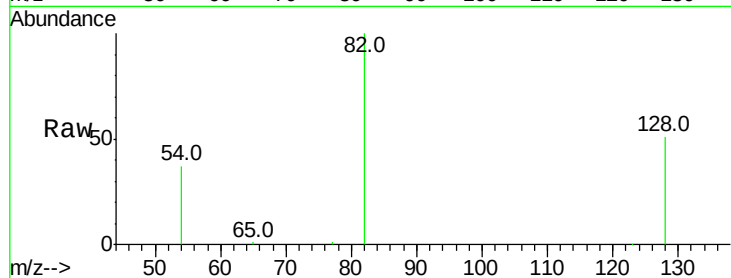

#10
 Naphthalene
 Concen: 0.76 ng
 RT: 10.58 min Scan# 557
 Delta R.T. 0.01 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57

Tgt Ion	128	Resp	34043
Ion Ratio	Lower	Upper	
128	100		
129	12.8	8.5	12.7#
127	12.1	10.6	16.0



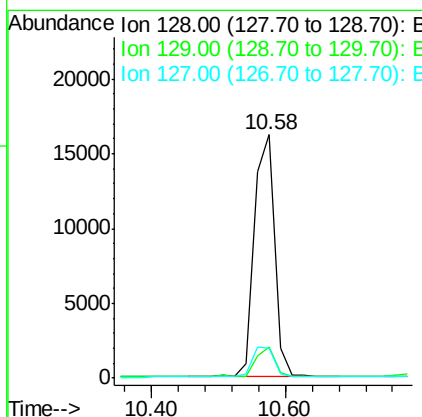
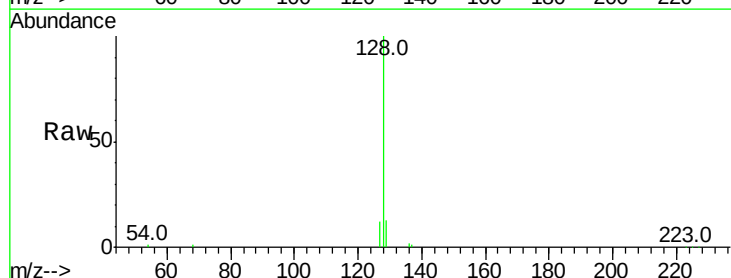


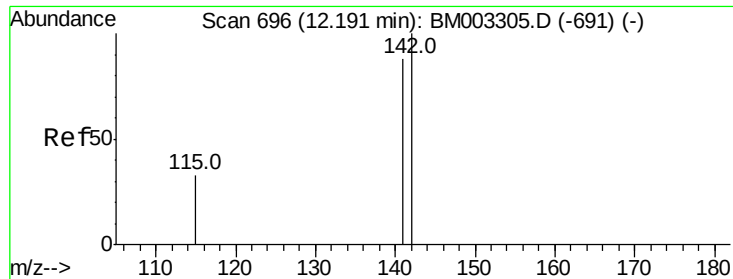

#12
2-Methylnaphthalene
Concen: 0.74 ng
RT: 12.19 min Scan# 696
Delta R.T. -0.00 min
Lab File: BM003314.D
Acq: 27 Nov 2015 20:57




Instrument :
BNA_M
ClientSampleId :
MW-14A-111815


Tot Ion:142 Resp: 20904
Ion Ratio Lower Upper
142 100
141 86.7 72.2 108.2
115 32.8 28.0 42.0

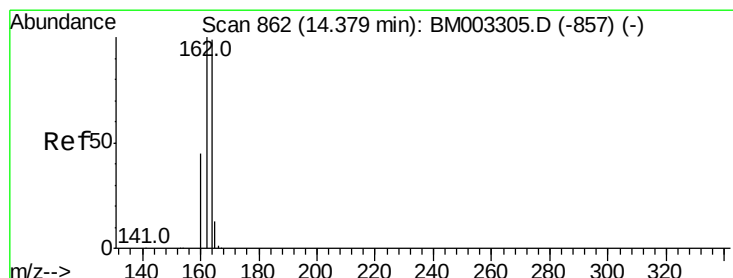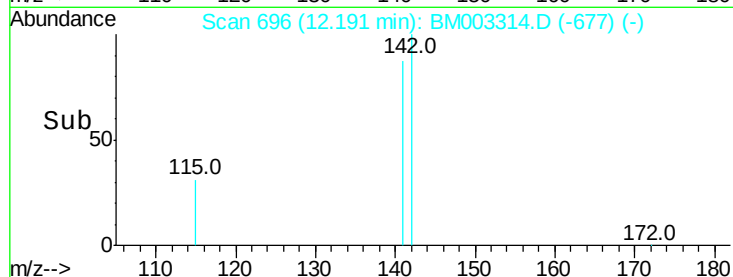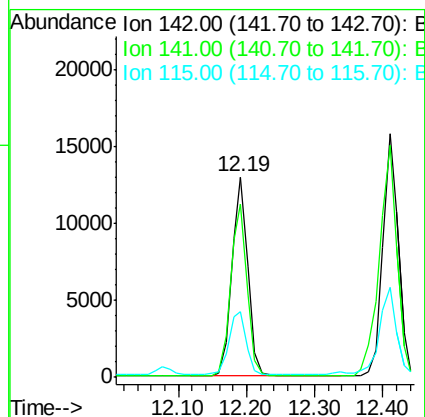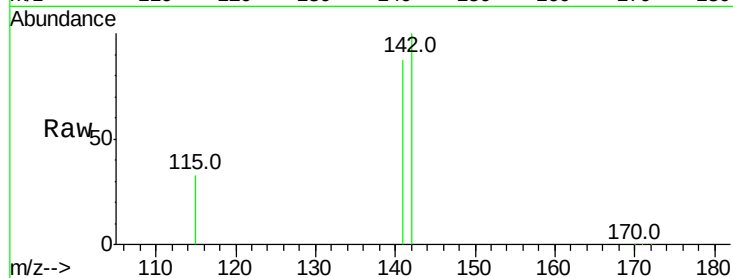

#13
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.38 min Scan# 862
Delta R.T. -0.00 min
Lab File: BM003314.D
Acq: 27 Nov 2015 20:57

Tgt Ion:164 Resp: 108443
Ion Ratio Lower Upper
164 100
162 98.1 78.3 117.5
160 42.7 33.8 50.6


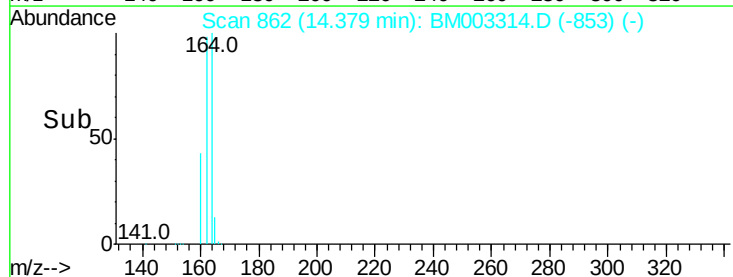
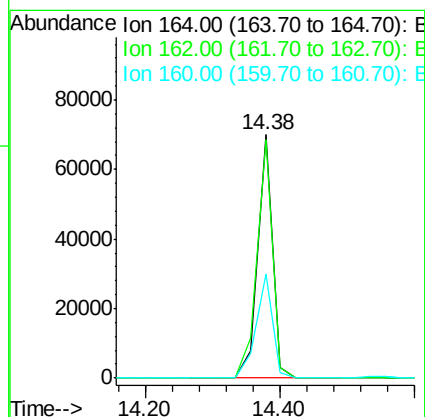
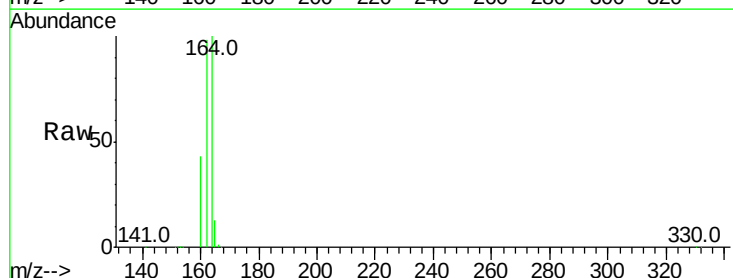




#14
 2,4,6-Tribromophenol
 Concen: 9.26 ng
 RT: 15.87 min Scan# 929
 Delta R.T. 0.00 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57




Instrument :
 BNA_M
 ClientSampleId :
 MW-14A-111815


Tot Ion:330 Resp: 23413
 Ion Ratio Lower Upper
 330 100
 332 93.1 76.0 114.0
 141 0.0 0.0 0.0

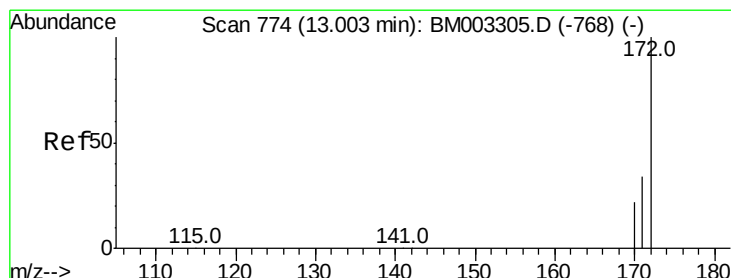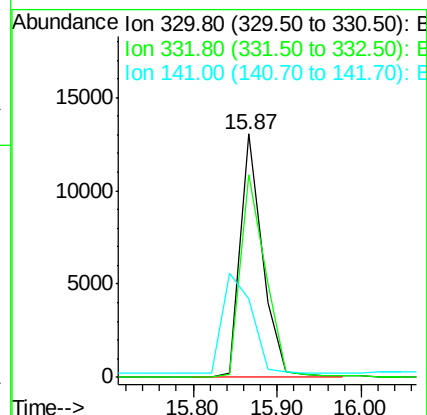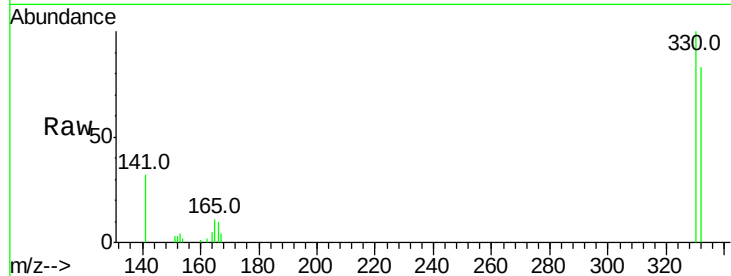

#15
 2-Fluorobiphenyl
 Concen: 3.52 ng
 RT: 13.00 min Scan# 774
 Delta R.T. -0.00 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57

Tgt Ion:172 Resp: 123297
 Ion Ratio Lower Upper
 172 100
 171 33.1 28.0 42.0
 170 21.1 18.9 28.3



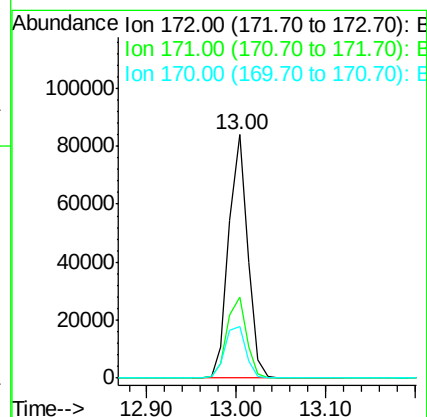
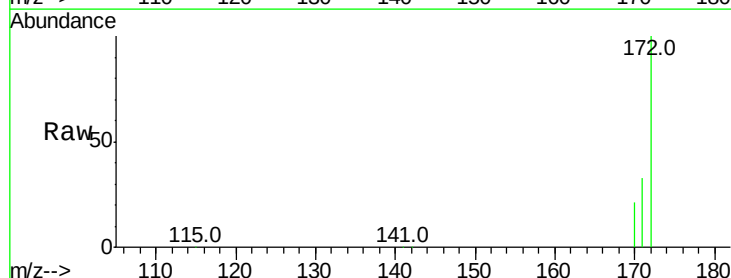




#18
 Fluorene
 Concen: 0.07 ng
 RT: 15.42 min Scan# 909
 Delta R.T. -0.00 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57




Instrument :
 BNA_M
 ClientSampleId :
 MW-14A-111815


Tot Ion:166 Resp: 2175
 Ion Ratio Lower Upper
 166 100
 165 96.3 80.8 121.2
 167 19.7 10.5 15.7#

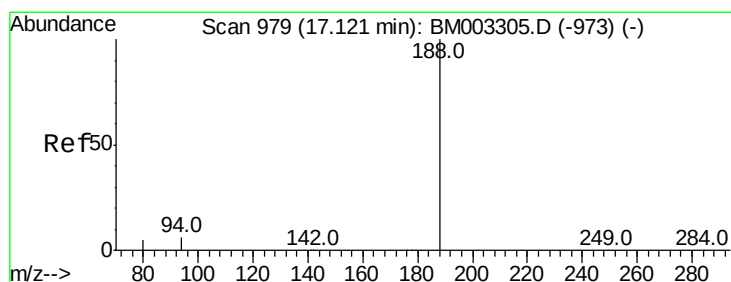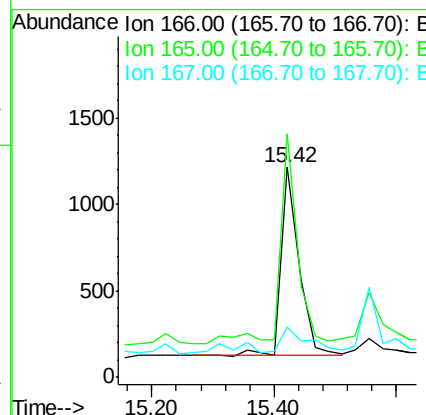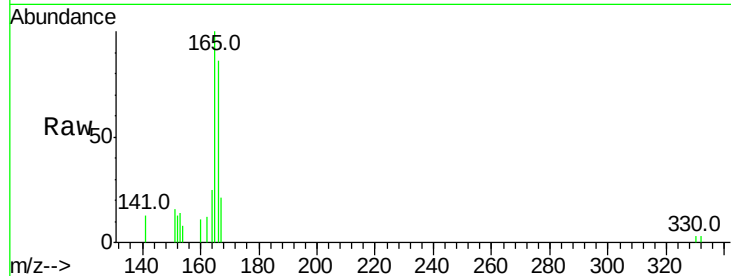

#19
 Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.12 min Scan# 979
 Delta R.T. -0.00 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57

Tgt Ion:188 Resp: 252794
 Ion Ratio Lower Upper
 188 100
 94 5.1 1.8 2.6#
 80 4.2 1.4 2.0#

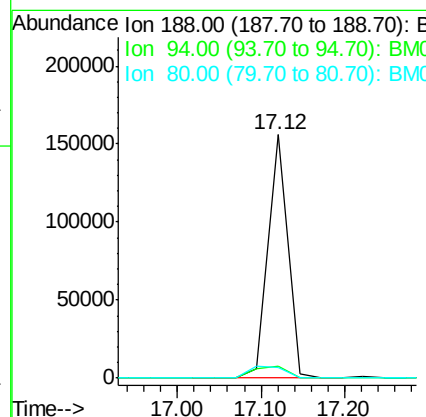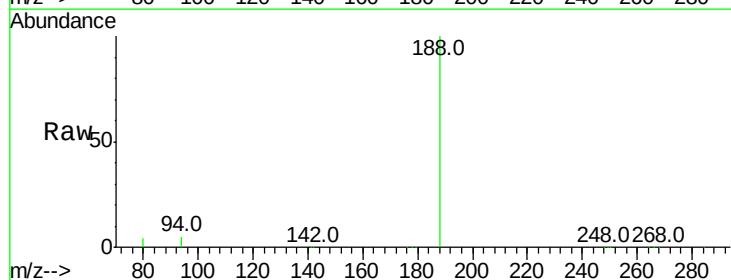



#22

Pentachlorophenol

Concen: 0.37 ng

RT: 16.79 min Scan# 966

Delta R.T. 0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57

Instrument :

BNA_M

ClientSampleId :

MW-14A-111815


Tot Ion:266 Resp: 797

Ion Ratio Lower Upper


266 100

268 77.2 45.8 68.8#



264 61.5 56.7 85.1

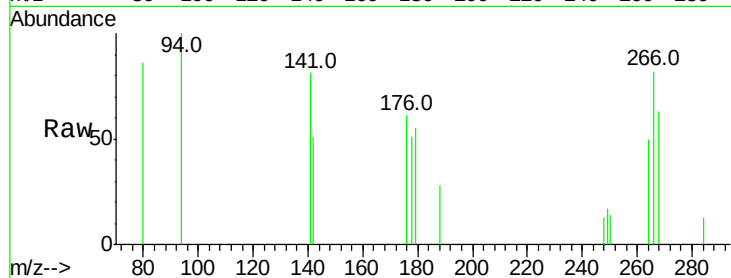

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

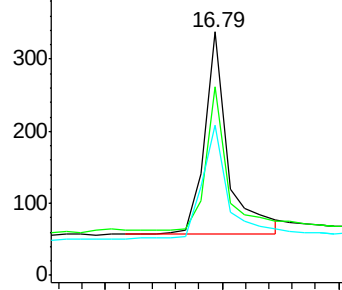

Time-->

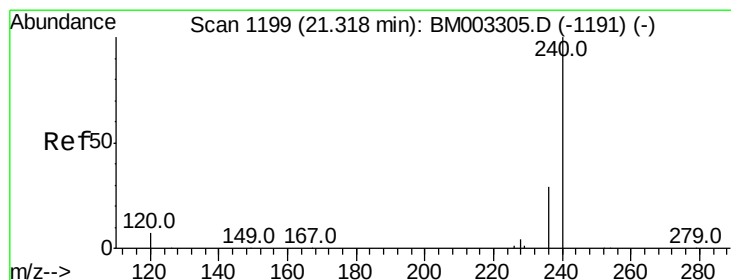

#26

Chrysene-d12

Concen: 5.00 ng

RT: 21.32 min Scan# 1199

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57


Tgt Ion:240 Resp: 218403

Ion Ratio Lower Upper


240 100

120 5.9 1.0 1.4#


236 28.1 17.9 26.9#

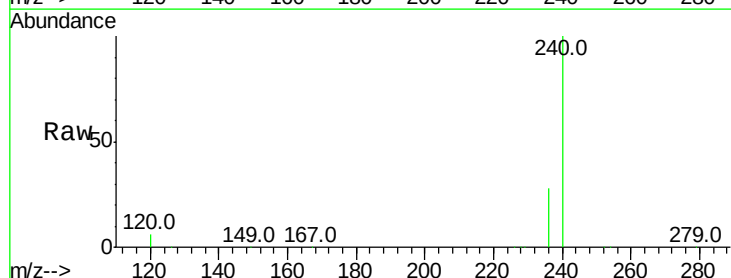


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

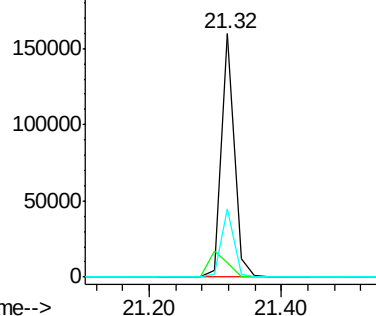

Time-->





#29

Terphenyl-d14

Concen: 4.13 ng

RT: 19.76 min Scan# 1116

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57

Instrument :

BNA_M

ClientSampleId :

MW-14A-111815


Tot Ion:244 Resp: 125816

Ion Ratio Lower Upper

244 100

212 9.2 6.5 9.7




122 3.9 2.0 3.0#

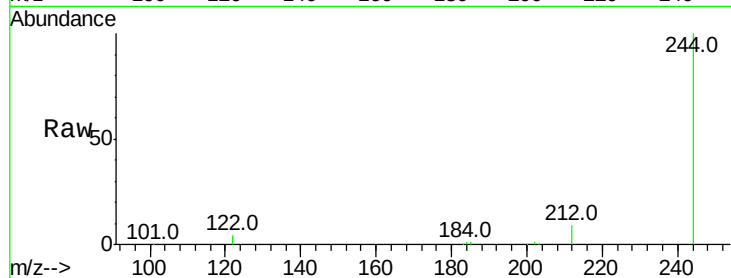

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

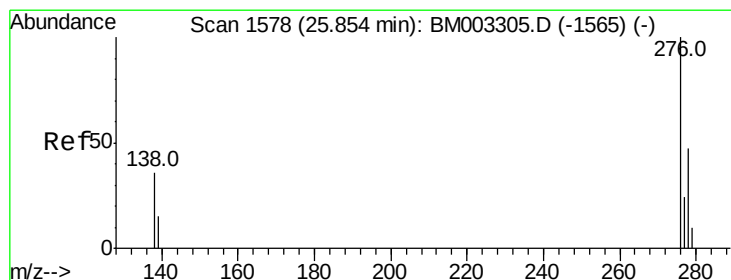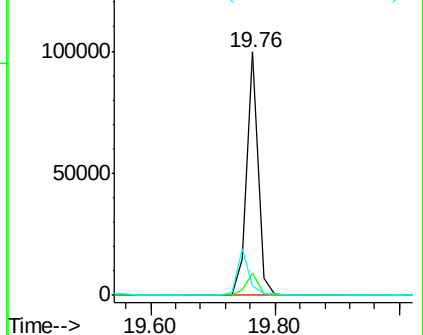

#34

Indeno(1,2,3-cd)pyrene

Concen: 0.05 ng

RT: 25.85 min Scan# 1578

Delta R.T. -0.00 min

Lab File: BM003314.D

Acq: 27 Nov 2015 20:57


Tgt Ion:276 Resp: 2781

Ion Ratio Lower Upper

276 100

138 40.6 19.1 28.7#



277 25.5 15.9 23.9#

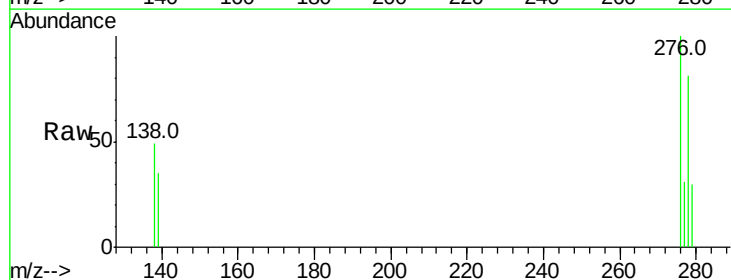


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




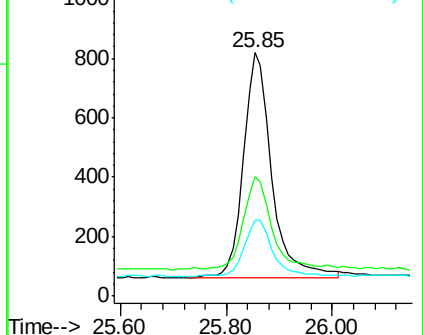


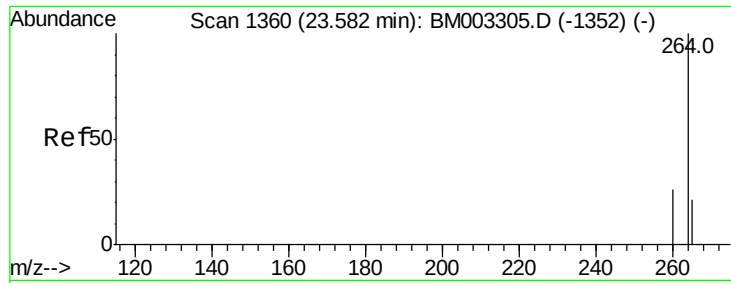

#35
 Pervlene-d12
 Concen: 5.00 ng
 RT: 23.58 min Scan# 1360
 Delta R.T. -0.00 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57




Instrument :
 BNA_M
 ClientSampleId :
 MW-14A-111815


Tot Ion:264 Resp: 172640
 Ion Ratio Lower Upper
 264 100
 260 25.1 19.6 29.4
 265 21.9 18.4 27.6

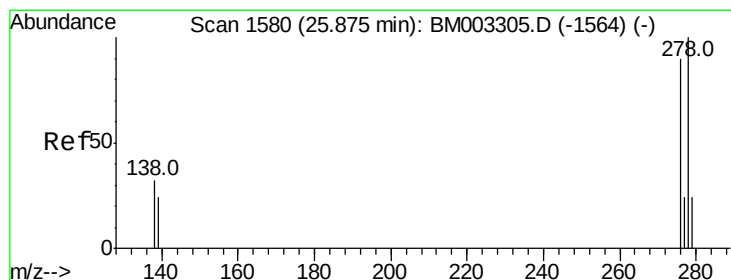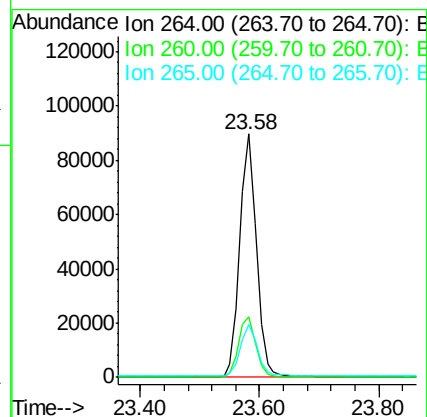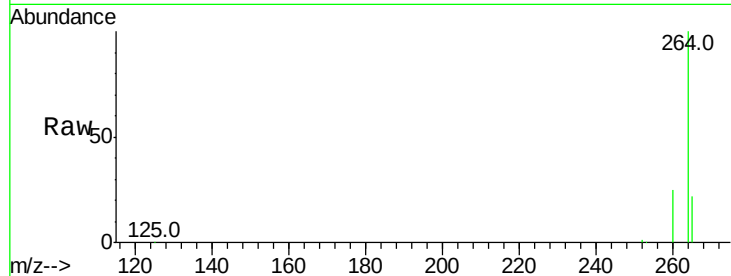

#39
 Dibenzo(a,h)anthracene
 Concen: 0.09 ng
 RT: 25.88 min Scan# 1580
 Delta R.T. -0.00 min
 Lab File: BM003314.D
 Acq: 27 Nov 2015 20:57

Tgt Ion:278 Resp: 3072
 Ion Ratio Lower Upper
 278 100
 139 32.7 18.2 27.4#
 279 34.7 18.8 28.2#

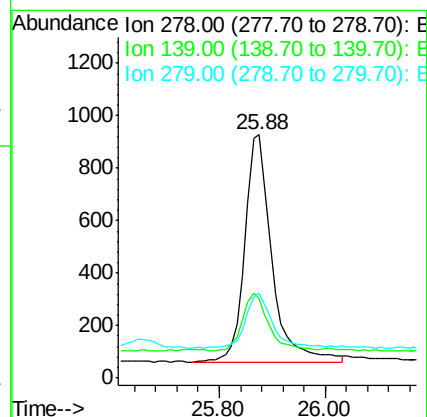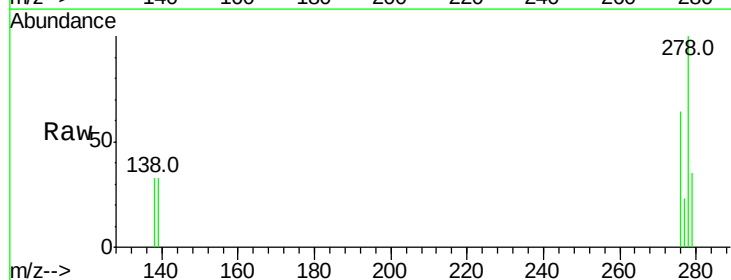

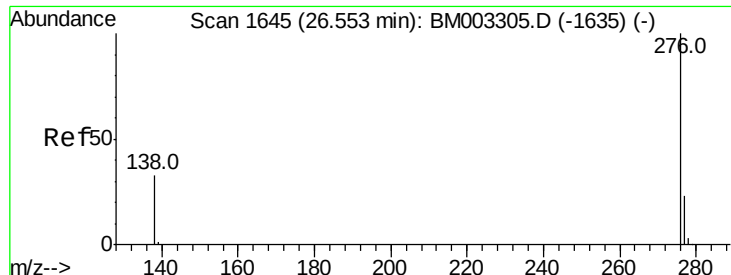

#40

Benzo(a,h,i)perylene

Concen: 0.04 ng

RT: 26.55 min Scan# 1645

Delta R.T. -0.00 min

Lab File: BM003314.D


Acq: 27 Nov 2015 20:57

Instrument :

BNA_M

ClientSampleId :

MW-14A-111815

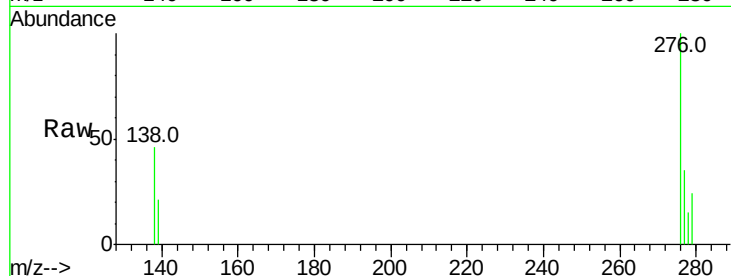


Tot Ion:276 Resp: 1542

Ion Ratio Lower Upper

276 100

277 34.9 19.0 28.6#

138 45.7 22.3 33.5#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

