


Data Path : Z:\HPCHEM1\BNA M\Data\BM112715\
 Data File : BM003300.D
 Acq On : 27 Nov 2015 09:51
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM112715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 27 16:36:40 2015

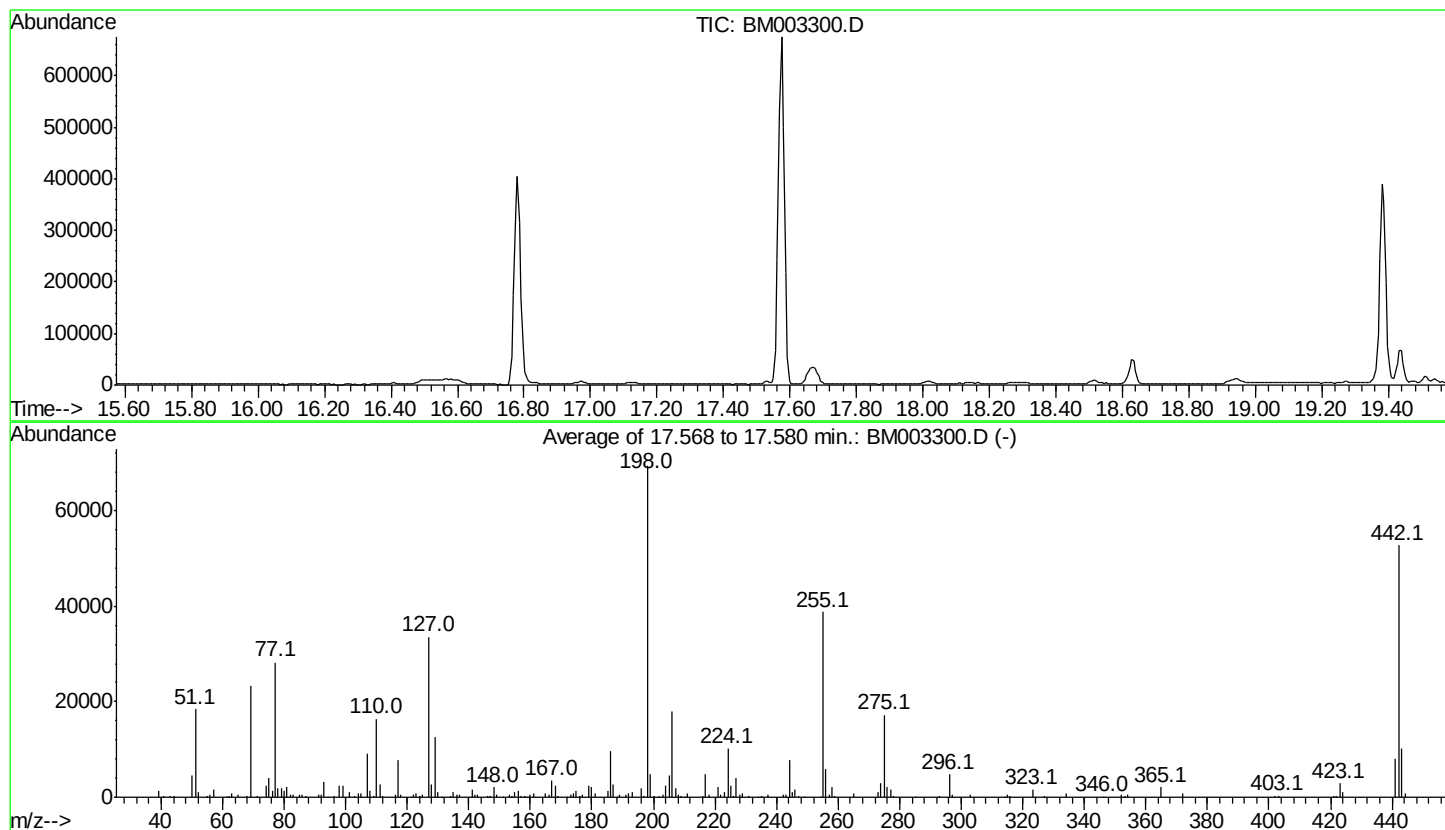

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	18411	PASS
68	69	0.00	2	1.7	405	PASS
69	198	0.00	100	33.5	23226	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	33562	PASS
197	198	0.00	2	0.5	359	PASS
198	198	100	100	100.0	69392	PASS
199	198	5	9	7.1	4949	PASS
275	198	10	60	24.8	17233	PASS
365	198	1	100	2.9	2027	PASS
441	442	0.01	24	15.4	8109	PASS
442	198	50	100	75.9	52693	PASS
443	442	15	24	19.6	10303	PASS