

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM112717\
 Data File : BM013122.D
 Acq On : 27 Nov 2017 21:59
 Operator : SJ/JU
 Sample : I6496-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AB7

Manual Integrations
 APPROVED

Sohil
 11/28/2017 2:54:01 PM

Quant Time: Nov 28 03:15:23 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 28 01:49:10 2017
 Response via : Initial Calibration

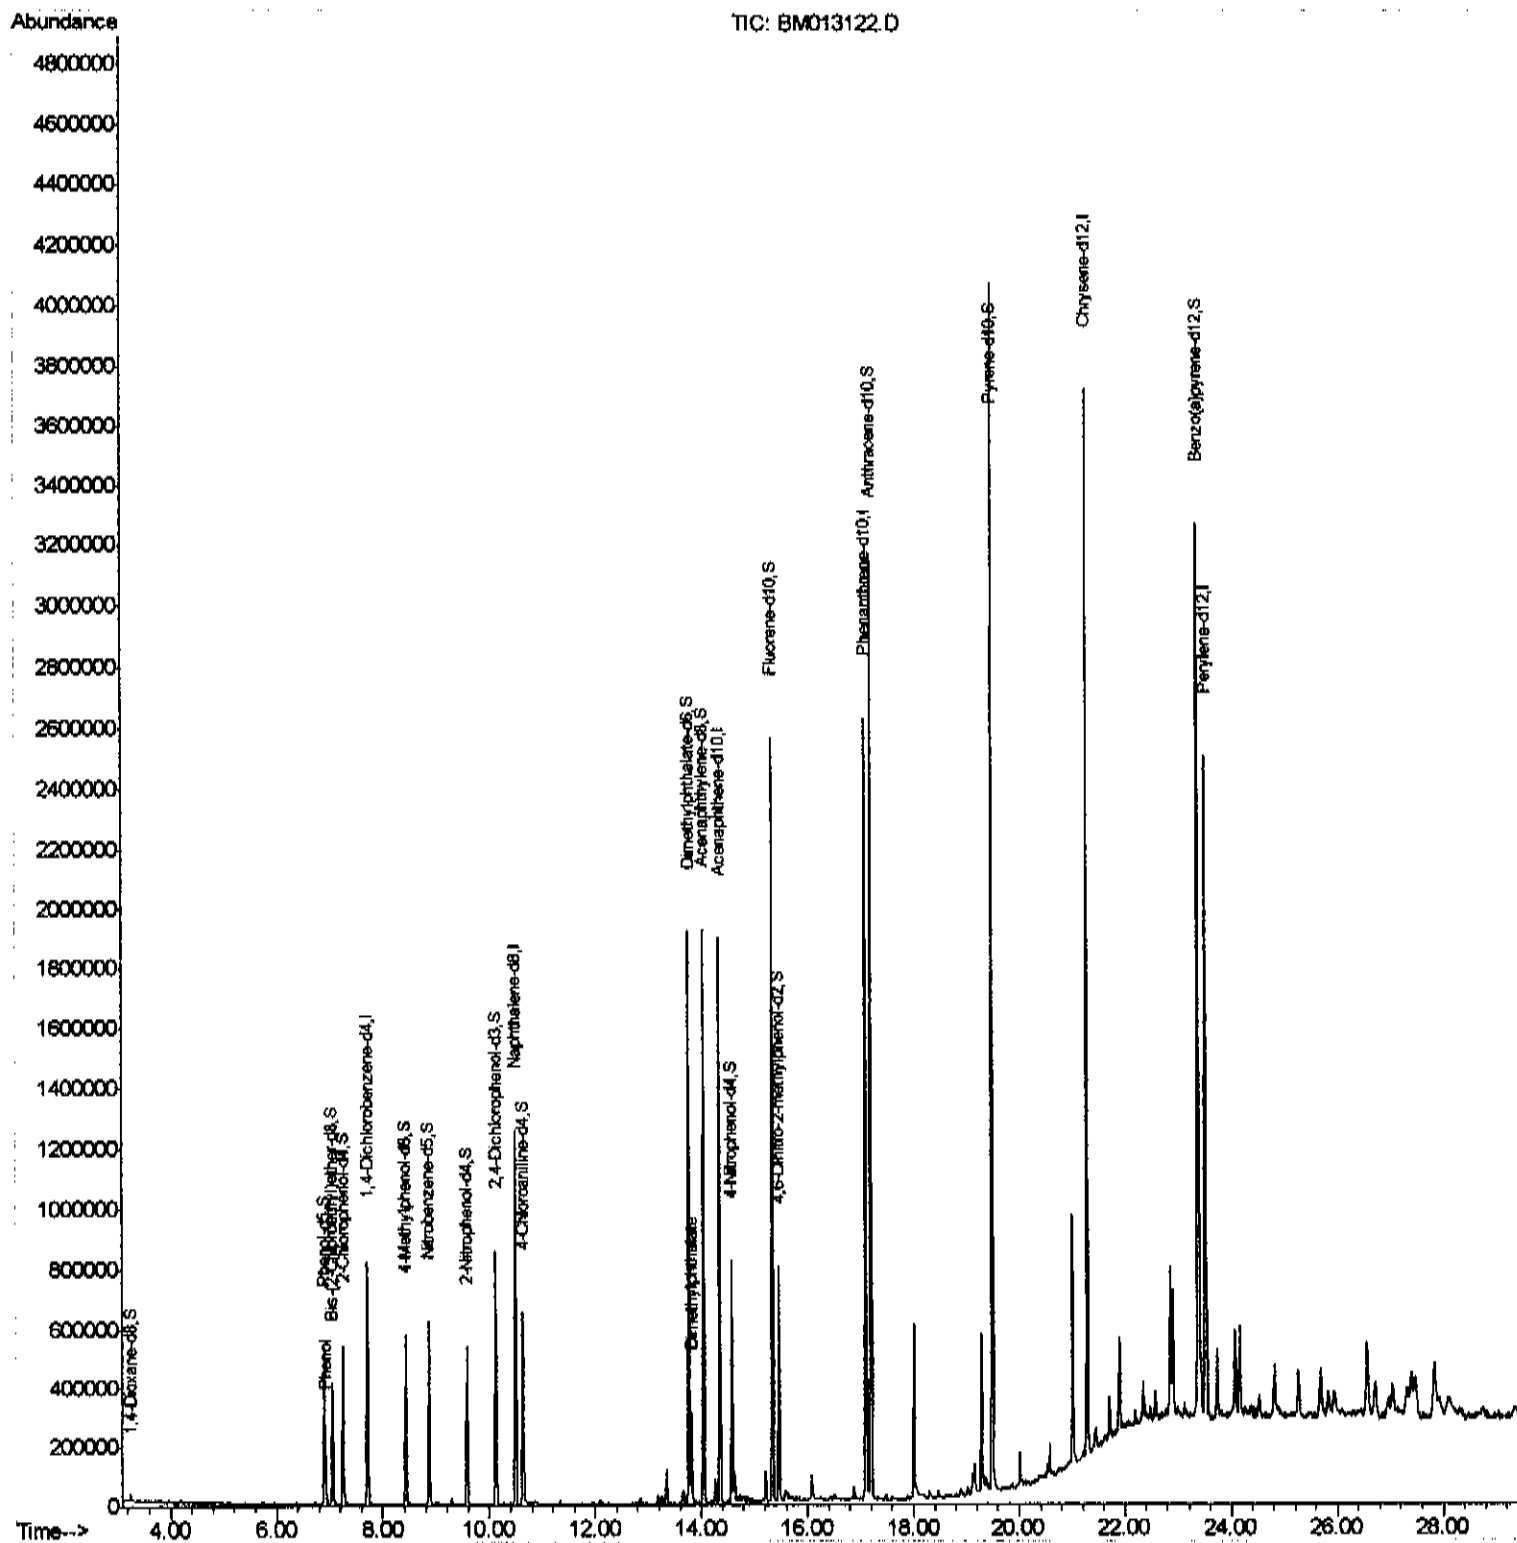

Instrument :

BNA M

ClientSampleId :

C0AB7

Manual Integrations


APPROVED

Sohil

11/28/2017 2:54:01 PM

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112717\
Data File : BM013122.D
Acq On : 27 Nov 2017 21:59
Operator : SJ/JU
Sample : I6496-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 28 01:53:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 28 01:49:10 2017
Response via : Initial Calibration

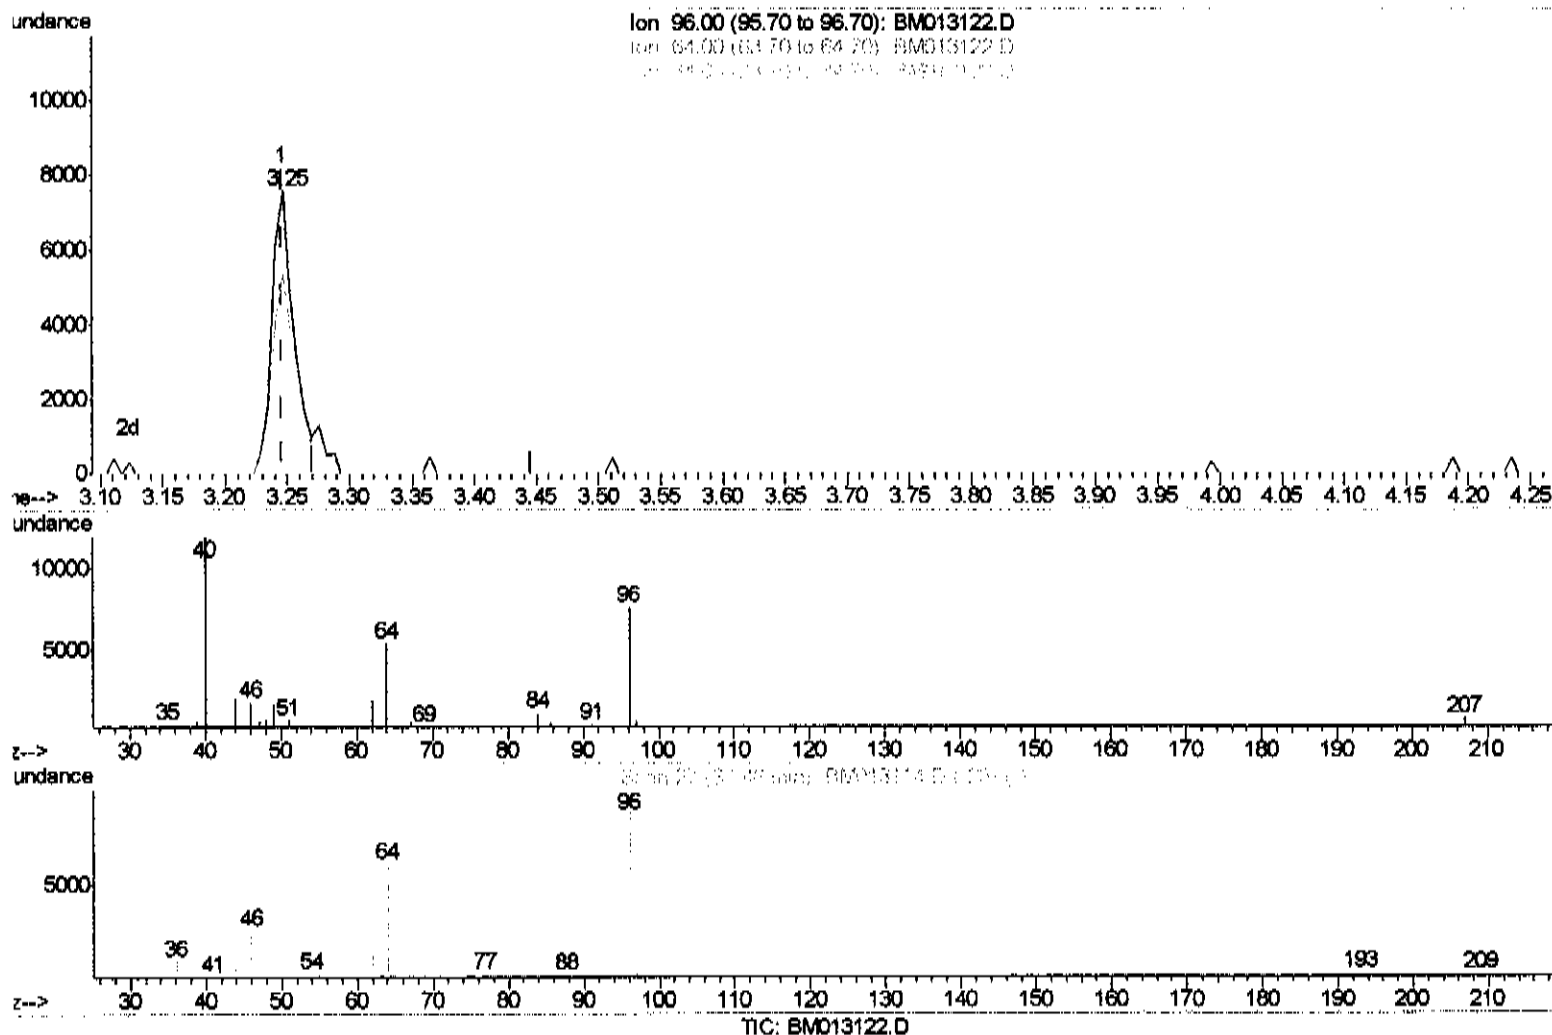

(3) 1,4-Dioxane-d8 (S)

3.246min (+0.001) 2.04ng/uL

гепропна 9395

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	78.02
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM112717\
 Data File : BM013122.D
 Acq On : 27 Nov 2017 21:59
 Operator : SJ/JU
 Sample : I6496-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AB7

Manual Integrations
 APPROVED

Sohil
 11/28/2017 2:54:01 PM

Quant Time: Nov 28 01:53:18 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 28 01:49:10 2017
 Response via : Initial Calibration

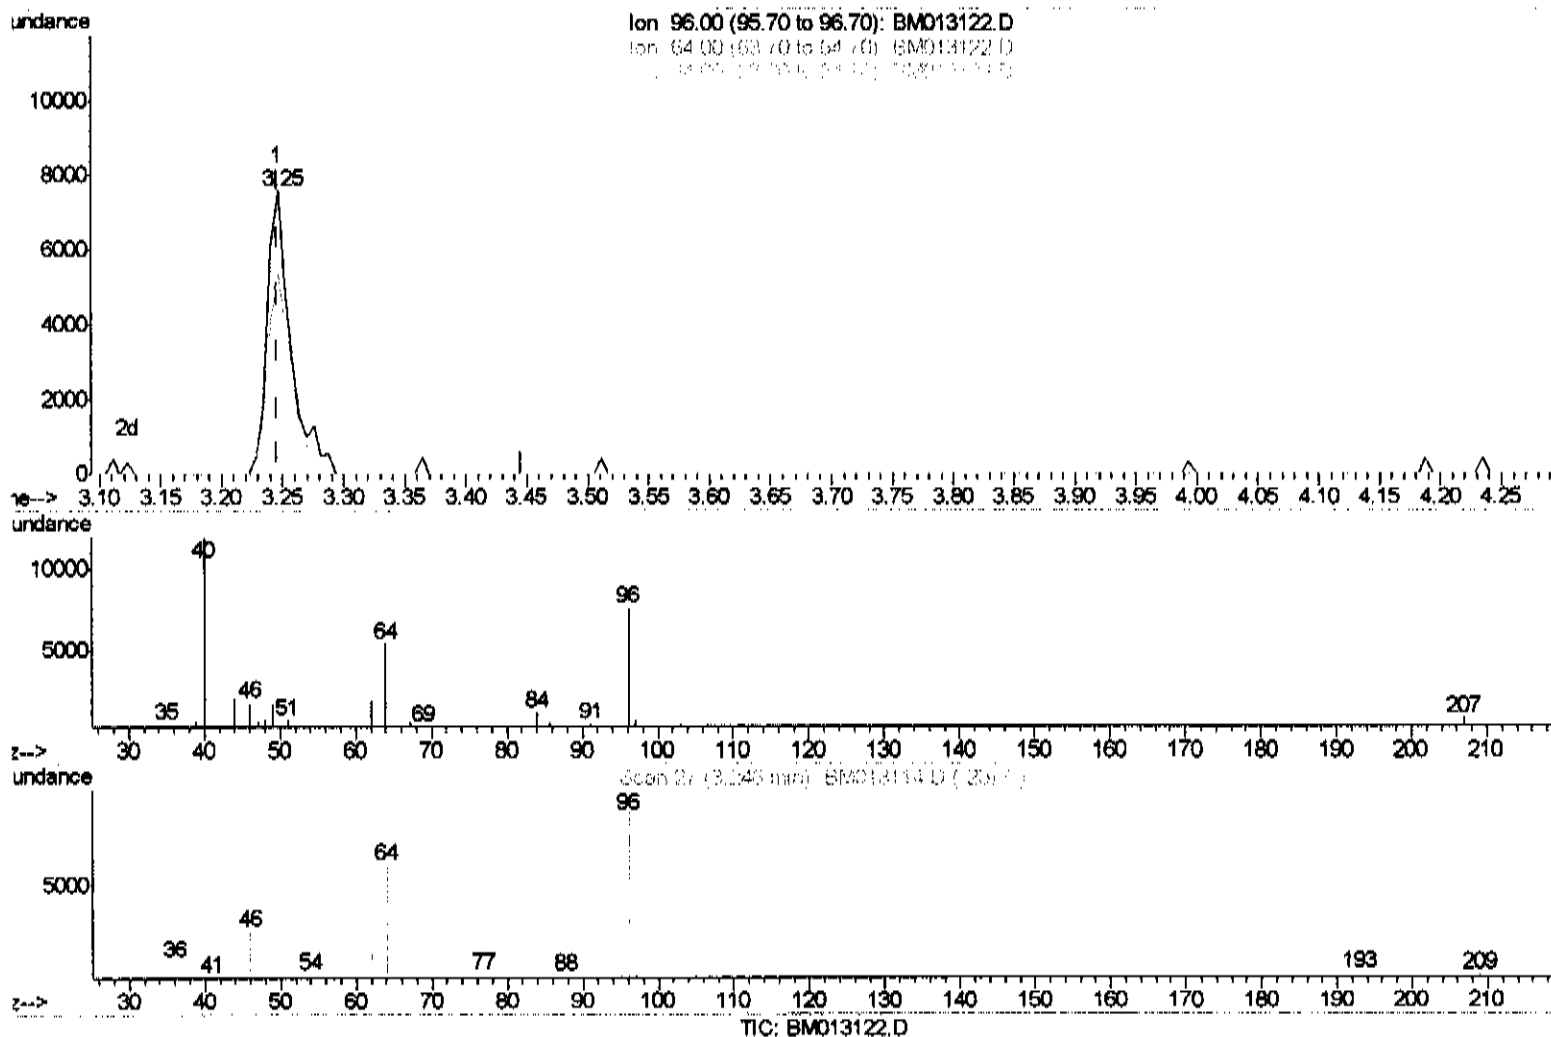

(3) 1,4-Dioxane-d8 (S)

3.246min (+0.001) 2.22ng/uL m

10/11/29/17

response 10224

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	71.69
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112717\
 Data File : BM013122.D
 Acq On : 27 Nov 2017 21:59
 Operator : SJ/JU
 Sample : I6496-07
 Disc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AB7

Manual Integrations
 APPROVED

Sohil
 11/28/2017 2:54:01 PM

Quant Time: Nov 28 03:15:23 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 Last Update : Tue Nov 28 01:49:10 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	213302	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	957314	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	596595	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	1420257	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1646413	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	1586024	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	10224m	2.22	ng/uL	0.00
5) Phenol-d5	6.89	99	265836	14.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	171079	16.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	216763	14.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	199940	13.21	ng/ul	-0.01
19) Nitrobenzene-d5	8.86	128	130256	19.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	142394	21.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	286266	17.38	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.63	131	309321	17.96	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	1185902	22.66	ng/ul	0.00
46) Acenaphthylene-d8	14.04	160	1343813	20.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	168451	21.22	ng/ul	-0.01
57) Fluorene-d10	15.34	176	992325	22.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	163313	26.52	ng/ul	-0.01
70) Anthracene-d10	17.19	188	1662607	22.87	ng/ul	0.00
76) Pyrene-d10	19.49	212	1993649	23.70	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	2119767	26.36	ng/ul	0.00

- 7011/24/17

Target Compounds

						Qvalue
6) Phenol	6.92	94	48043	2.63	ng/ul#	84
44) Dimethylphthalate	13.81	163	180963	3.62	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed