

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112717\
 Data File : BM013123.D
 Acq On : 27 Nov 2017 22:35
 Operator : SJ/JU
 Sample : I6496-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Quant Time: Nov 28 01:53:32 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 28 01:49:10 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	231165	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1045288	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	652977	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	1567272	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1816452	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	1688555	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	13865	2.78	ng/uL	0.00
5) Phenol-d5	6.89	99	326809	16.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	199395	17.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	267224	16.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	237574	14.48	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	144594	19.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	161413	22.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	292098	16.24	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.63	131	307153	16.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	1091055	19.05	ng/ul	0.00
46) Acenaphthylene-d8	14.04	160	1260309	17.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	172346	19.84	ng/ul	-0.01
57) Fluorene-d10	15.34	176	904921	18.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	152294	22.41	ng/ul	0.00
70) Anthracene-d10	17.19	188	1496153	18.65	ng/ul	0.00
76) Pyrene-d10	19.49	212	1798171	19.38	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	1817439	21.23	ng/ul	0.00
Target Compounds						
6) Phenol	6.92	94	45800	2.317	ng/ul#	86
44) Dimethylphthalate	13.81	163	147885	2.700	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112717\
Data File : BM013123.D
Acq On : 27 Nov 2017 22:35
Operator : SJ/JU
Sample : I6496-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB8

Quant Time: Nov 28 01:53:32 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 28 01:49:10 2017
Response via : Initial Calibration

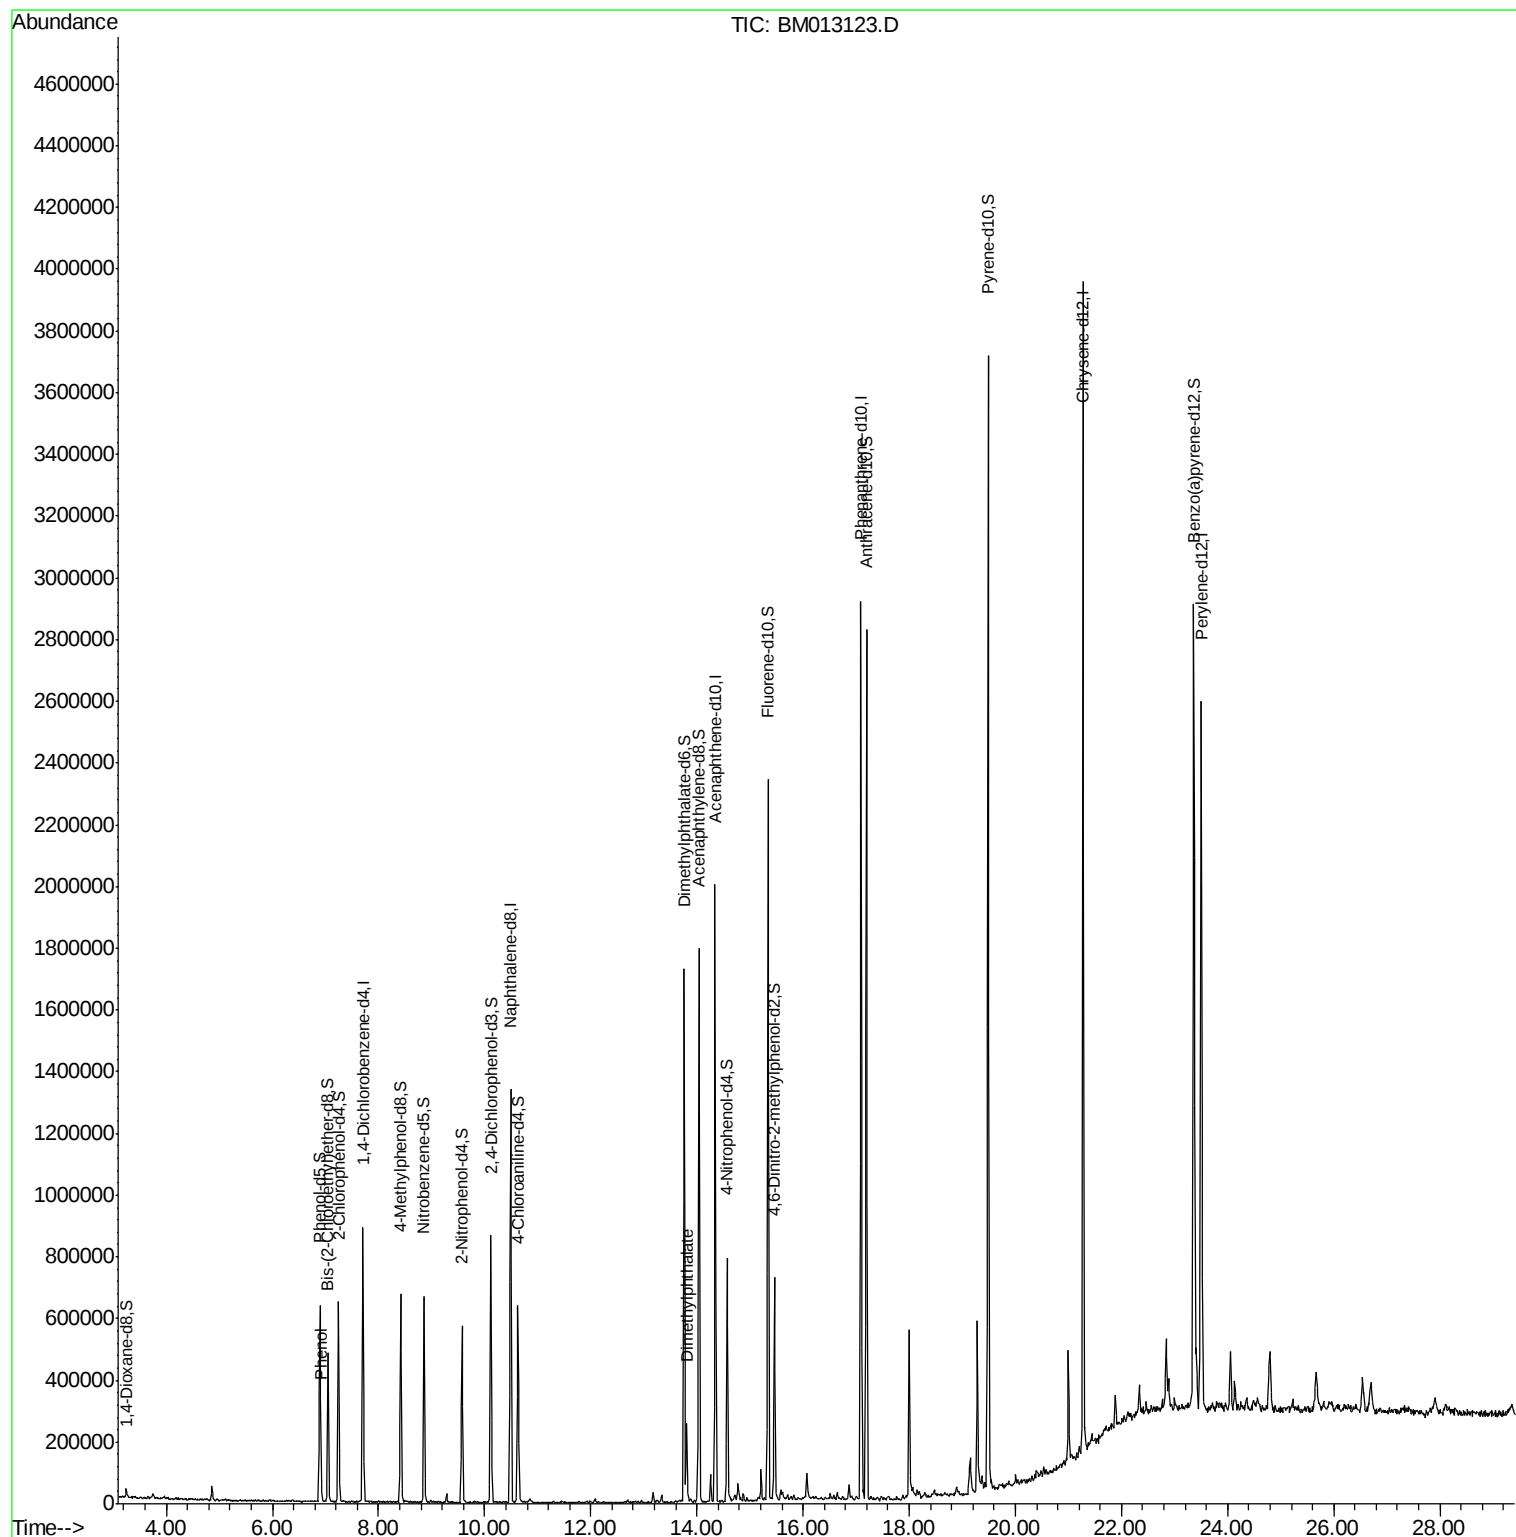

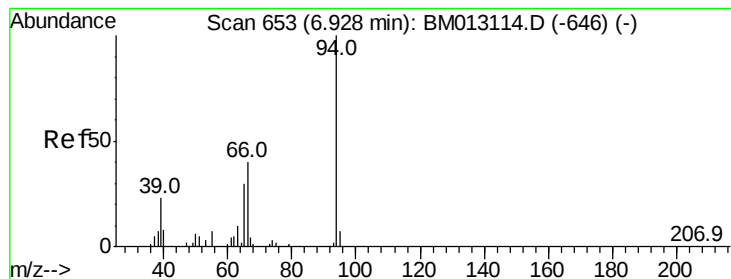





#6

Phenol

Concen: 2.317 ng/ul
 RT: 6.92 min Scan# 651
 Delta R.T. -0.01 min
 Lab File: BM013123.D
 Acq: 27 Nov 2017 22:35

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Tot Ion: 94 Resp: 45800
 Ion Ratio Lower Upper
 94 100
 65 35.8 28.2 42.4
 66 42.5 47.2 70.8#

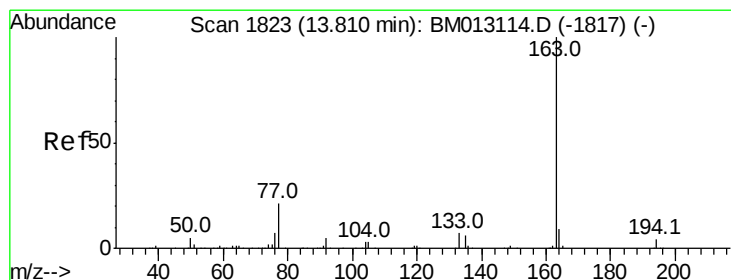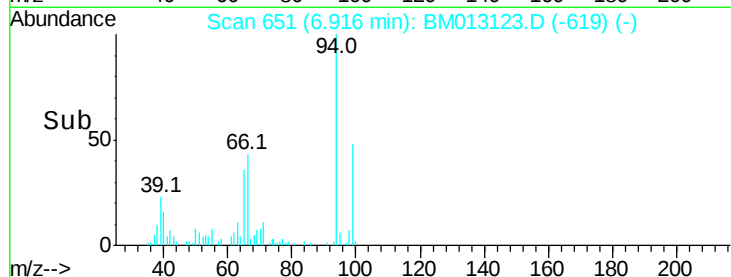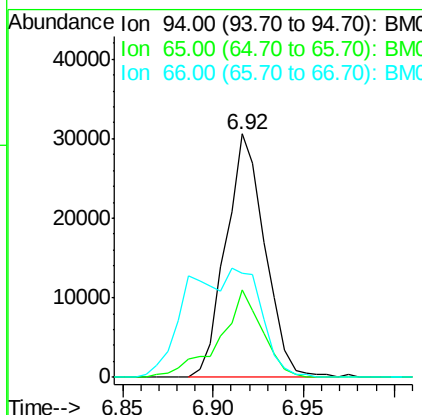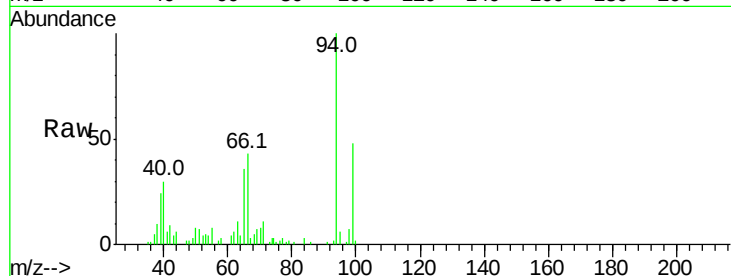

#44

Dimethylphthalate

Concen: 2.700 ng/ul
 RT: 13.81 min Scan# 1823
 Delta R.T. 0.00 min
 Lab File: BM013123.D
 Acq: 27 Nov 2017 22:35

Tgt Ion:163 Resp: 147885
 Ion Ratio Lower Upper
 163 100
 194 3.3 3.5 5.3#
 164 9.4 8.2 12.4

