

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112818\
 Data File : BM017774.D
 Acq On : 28 Nov 2018 15:42
 Operator : JU/SJ
 Sample : J5945-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETOA8

Manual Integrations
 APPROVED

mohammad
 11/29/2018 1:57:40 PM

Quant Time: Nov 29 00:49:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 29 00:30:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	186511	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	858583	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	519621	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1160104	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1305893	20.00	ng/ul	0.00
85) Perylene-d12	23.39	264	1282464	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	22827	5.60	ng/uL	0.00
5) Phenol-d5	6.77	99	445572	26.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	288114	28.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	377897	28.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	382092	27.45	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	190173	28.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	214254	28.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	373864m	25.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	551644	44.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	1356222	30.08	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	1624790	29.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	208070m	25.38	ng/ul	0.00
57) Fluorene-d10	15.24	176	1158317	29.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	234666	28.30	ng/ul	0.00
70) Anthracene-d10	17.09	188	1911197	33.09	ng/ul	0.00
78) Pyrene-d10	19.40	212	2565687	40.60	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	2865253	41.19	ng/ul	0.00

Target Compounds					Ovalue	
44) Dimethylphthalate	13.70	163	89906	2.058	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112818\
Data File : BM017774.D
Acq On : 28 Nov 2018 15:42
Operator : JU/SJ
Sample : J5945-17
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ETOA8

Quant Time: Nov 29 00:49:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 29 00:30:03 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
11/29/2018 1:57:40 PM

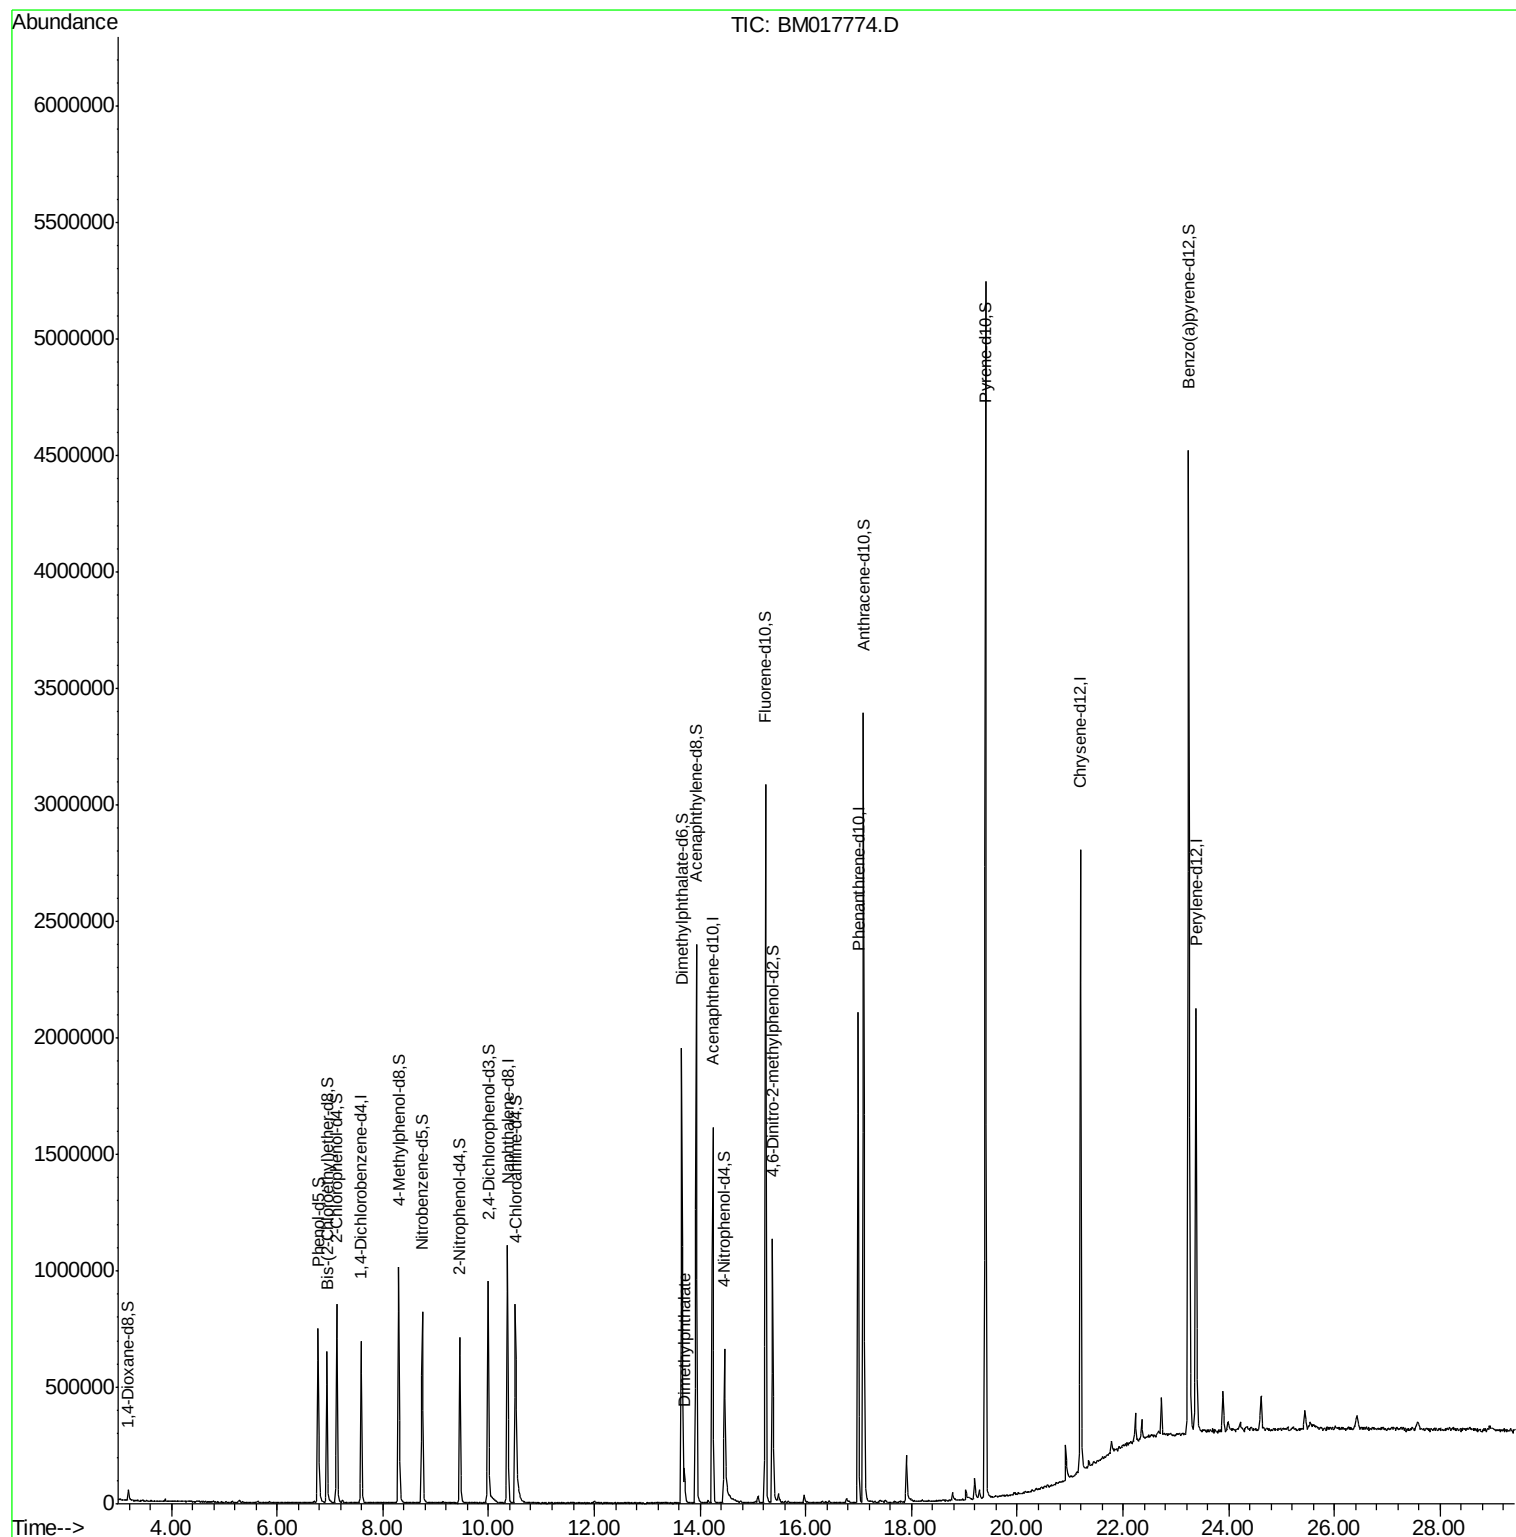

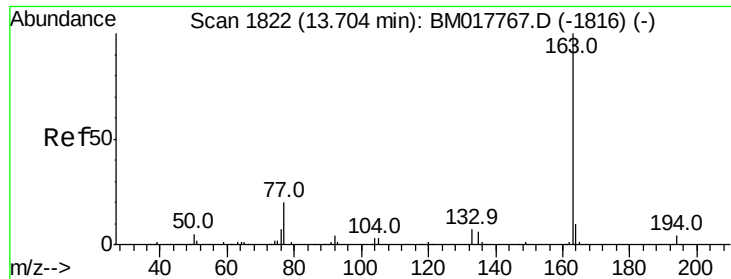


#44
 Dimethylphthalate
 Concen: 2.058 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.00 min
 Lab File: BM017774.D
 Acq: 28 Nov 2018 15:42

Instrument :
 BNA_M
 ClientSampleId :
 ETOA8

Tot Ion	Ratio	Resp	Lower	Upper
163	100	89906		
194	3.8		3.4	5.0
164	10.1		8.1	12.1

Manual Integrations
 APPROVED

mohammad
 11/29/2018 1:57:40 PM

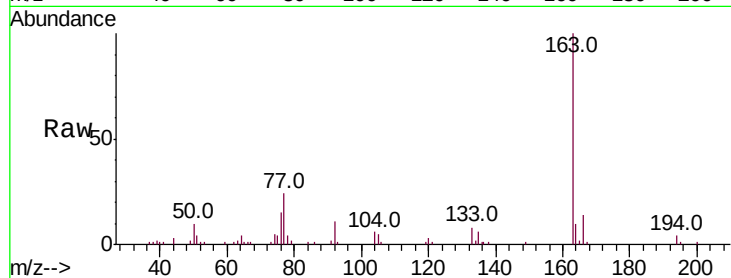

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

