

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112818\
 Data File : BM017775.D
 Acq On : 28 Nov 2018 16:19
 Operator : JU/SJ
 Sample : J5945-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETOB0

Quant Time: Nov 29 00:33:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 29 00:30:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	196997	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	868082	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	526350	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1217333	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1399205	20.00	ng/ul	0.00
85) Perylene-d12	23.39	264	1424587	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	16232	3.77	ng/uL	0.00
5) Phenol-d5	6.77	99	308395	17.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	213617	19.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	260598	18.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	242236	16.48	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	128487	19.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	148914	19.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	244485	16.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	340868	27.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	952029	20.85	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	1041991	18.85	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	115597	13.92	ng/ul	0.01
57) Fluorene-d10	15.24	176	797818	20.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	132815	15.26	ng/ul	0.00
70) Anthracene-d10	17.09	188	1208319	19.94	ng/ul	0.00
78) Pyrene-d10	19.39	212	1325988	19.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	1439809	18.64	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	284073	6.420	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112818\
Data File : BM017775.D
Acq On : 28 Nov 2018 16:19
Operator : JU/SJ
Sample : J5945-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETOB0

Quant Time: Nov 29 00:33:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 29 00:30:03 2018
Response via : Initial Calibration

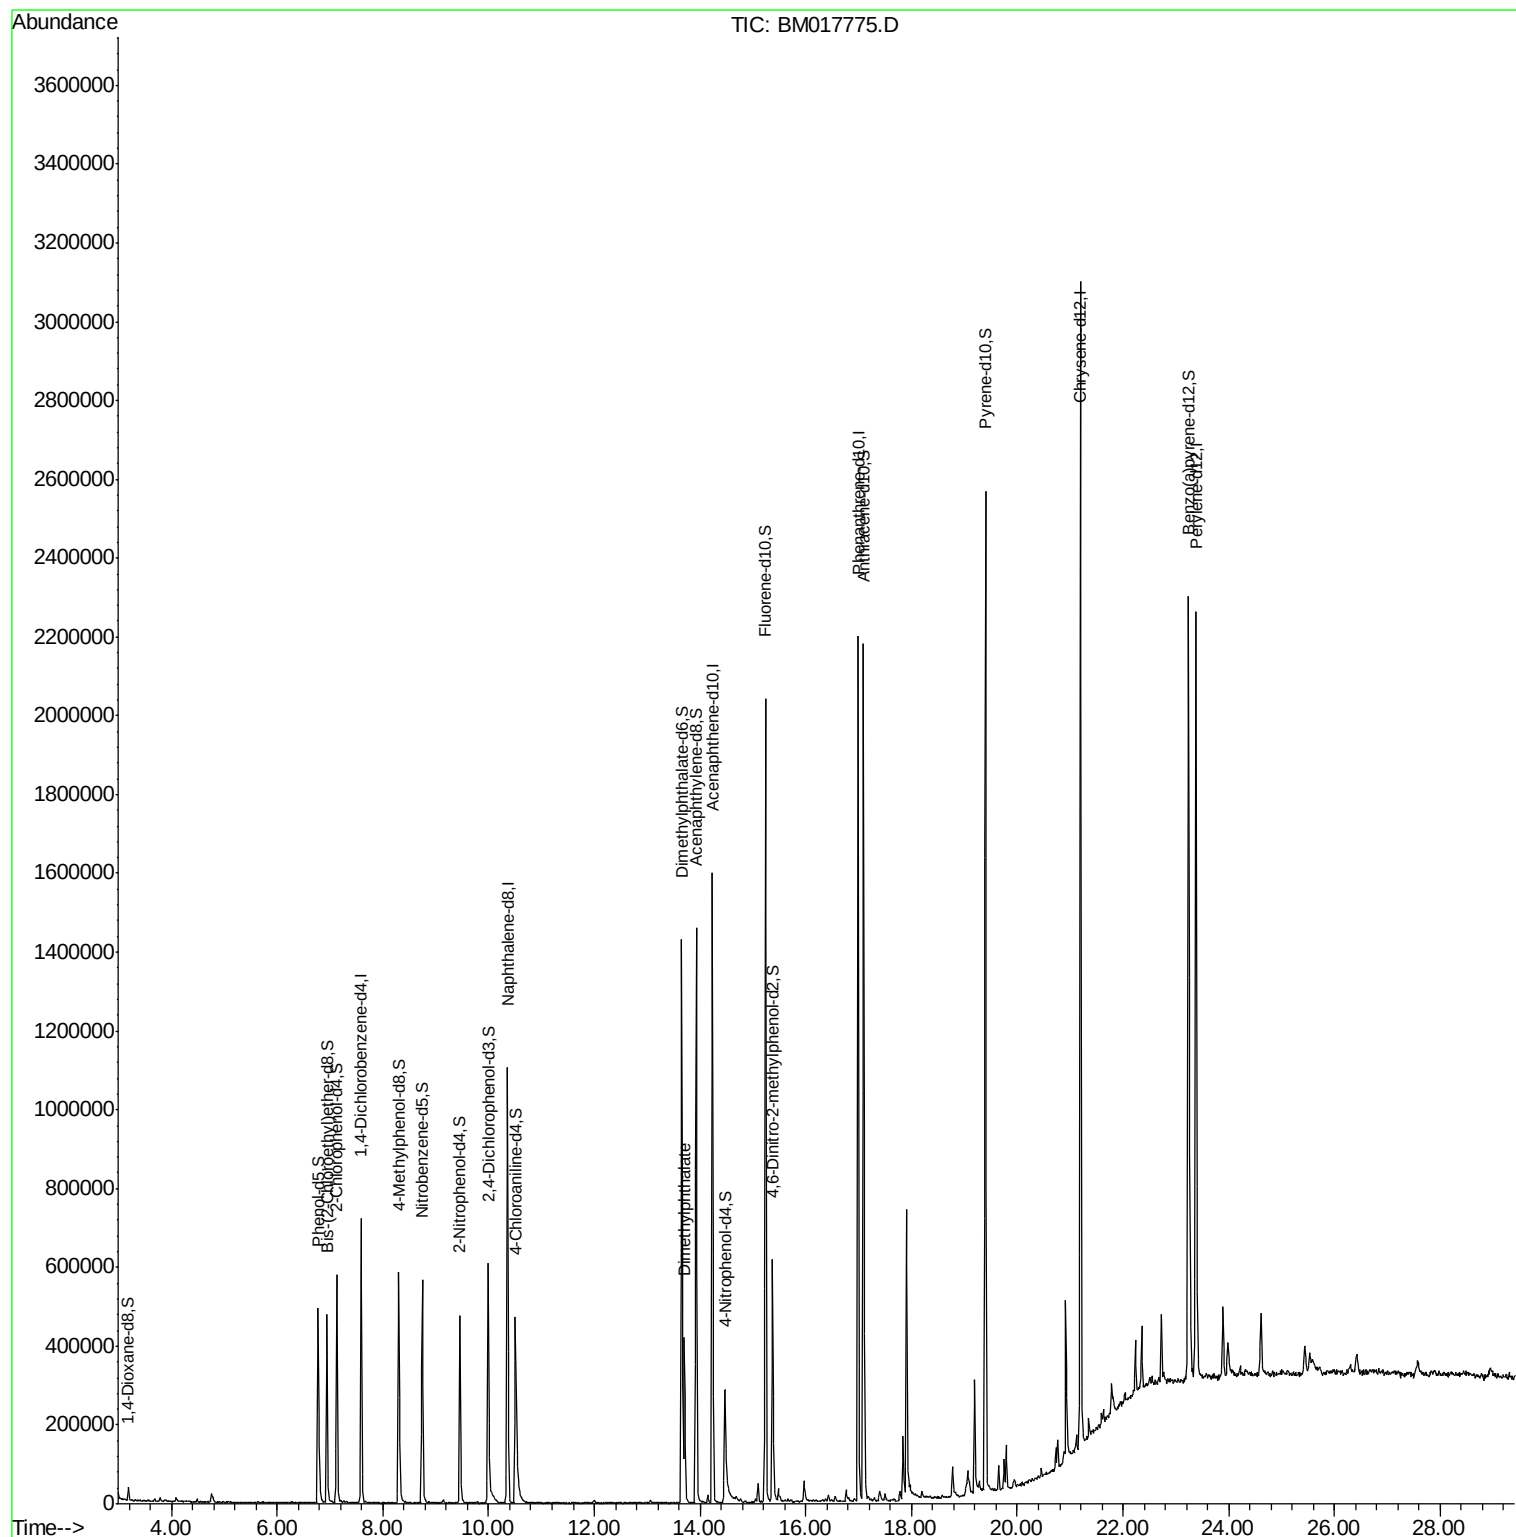

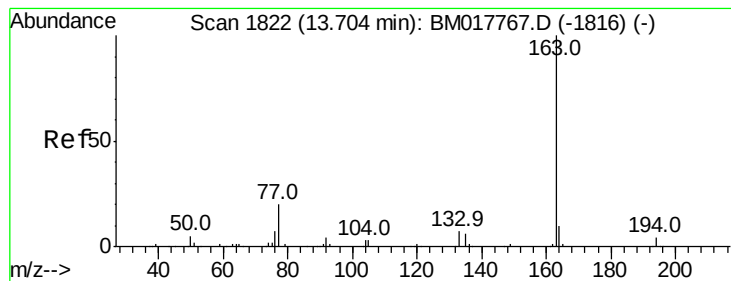

#44

Dimethylphthalate

Concen: 6.420 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.00 min

Lab File: BM017775.D

Acq: 28 Nov 2018 16:19

Instrument :

BNA_M

ClientSampleId :

ETOB0


Tot Ion:163 Resp: 284073

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.7 8.1 12.1

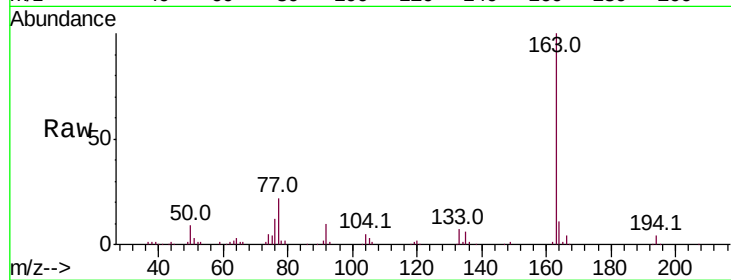

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

