

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112916\
 Data File : BM008108.D
 Acq On : 29 Nov 2016 18:51
 Operator : UM/SJ
 Sample : SSTD16039
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16039

Quant Time: Nov 30 00:13:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 30 00:08:34 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	149546	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	556057	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	353031	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	671470	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	831023	20.00	ng/ul	0.00
83) Perylene-d12	23.53	264	846124	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	196865	57.86	ng/uL	0.00
5) Phenol-d5	6.89	99	1779936	155.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	1005506	148.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	1411767	160.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	1358855	152.00	ng/ul	0.02
19) Nitrobenzene-d5	8.87	128	667477	167.62	ng/ul	0.01
22) 2-Nitrophenol-d4	9.58	143	775768	180.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	1361246	164.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	1227504	134.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	3585433	150.12	ng/ul	0.00
46) Acenaphthylene-d8	14.04	160	4452545	154.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.59	143	613042	161.66	ng/ul	0.02
57) Fluorene-d10	15.34	176	3083762	147.86	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.49	200	720734	179.42	ng/ul	0.00
70) Anthracene-d10	17.20	188	4662428	155.85	ng/ul	0.00
76) Pyrene-d10	19.50	212	5185925	153.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.39	264	5737192	156.73	ng/ul	0.01

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.29	88	217753	57.75	ng/uL	96
4) Benzaldehyde	6.86	77	1229400	168.99	ng/ul	99
6) Phenol	6.92	94	1819807	154.72	ng/ul	98
8) Bis(2-Chloroethyl)ether	7.15	93	1376862	152.78	ng/ul	97
10) 2-Chlorophenol	7.27	128	1433371	159.34	ng/ul	98
11) 2-Methylphenol	8.15	108	1345257	156.58	ng/ul	97
12) 2,2'-oxybis(1-Chloropropan	8.23	45	1469502	146.85	ng/ul	97
14) Acetophenone	8.53	105	2158457	153.38	ng/ul	97
15) N-Nitroso-di-n-propylamine	8.54	70	1079508	153.57	ng/ul	98
16) 4-Methylphenol	8.49	108	1421855	153.78	ng/ul	99
17) Hexachloroethane	8.76	117	626619	156.90	ng/ul	90
20) Nitrobenzene	8.91	77	1638279	160.43	ng/ul	96
21) Isophorone	9.44	82	2873023	162.51	ng/ul	99
23) 2-Nitrophenol	9.62	139	780864	175.57	ng/ul	99
24) 2,4-Dimethylphenol	9.67	107	1612022	160.48	ng/ul	100
25) Bis(2-Chloroethoxy)methane	9.91	93	1689005	157.79	ng/ul	96
27) 2,4-Dichlorophenol	10.14	162	1346680	165.19	ng/ul	98
28) Naphthalene	10.53	128	4137250	154.19	ng/ul	99
30) 4-Chloroaniline	10.66	127	1241746	134.20	ng/ul	97
31) Hexachlorobutadiene	10.80	225	1061460	159.43	ng/ul	96
32) Caprolactam	11.49	113	237447	101.48	ng/ul	98
33) 4-Chloro-3-methylphenol	11.80	107	1410682	163.91	ng/ul	100
34) 2-Methylnaphthalene	12.15	142	2935423	154.23	ng/ul	98


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM112916\
 Data File : BM008108.D
 Acq On : 29 Nov 2016 18:51
 Operator : UM/SJ
 Sample : SSTD16039
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16039

Quant Time: Nov 30 00:13:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 30 00:08:34 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 1,2,4,5-Tetrachlorobenzene	12.52	216	1761190	155.25	ng/ul	98
37) Hexachlorocyclopentadiene	12.49	237	1087264	169.37	ng/ul	97
38) 2,4,6-Trichlorophenol	12.77	196	1066578	167.01	ng/ul	99
39) 2,4,5-Trichlorophenol	12.85	196	1144526	164.00	ng/ul	99
40) 1,1'-Biphenyl	13.17	154	3747592	152.15	ng/ul	99
41) 2-Chloronaphthalene	13.22	162	2888238	152.70	ng/ul	99
42) 2-Nitroaniline	13.44	65	872777	170.76	ng/ul	95
44) Dimethylphthalate	13.81	163	3505608	150.72	ng/ul	100
45) 2,6-Dinitrotoluene	13.94	165	769666	173.60	ng/ul	94
47) Acenaphthylene	14.07	152	4433137	151.89	ng/ul	99
48) 3-Nitroaniline	14.27	138	635750	146.73	ng/ul	95
49) Acenaphthene	14.41	153	3022456	149.99	ng/ul	98
50) 2,4-Dinitrophenol	14.49	184	532630	192.99	ng/ul	99
52) 4-Nitrophenol	14.60	109	573356	154.05	ng/ul	94
53) Dibenzofuran	14.74	168	4242678	147.31	ng/ul	97
54) 2,4-Dinitrotoluene	14.74	165	1078426	169.52	ng/ul	90
55) 2,3,4,6-Tetrachlorophenol	14.98	232	1042605	167.29	ng/ul	98
56) Diethylphthalate	15.18	149	3485458	149.87	ng/ul	98
58) Fluorene	15.40	166	3453982	149.76	ng/ul	98
59) 4-Chlorophenyl-phenylether	15.39	204	1855079	150.79	ng/ul	98
60) 4-Nitroaniline	15.46	138	727559	164.28	ng/ul	96
63) 4,6-Dinitro-2-methylphenol	15.51	198	729515	175.65	ng/ul#	98
64) N-Nitrosodiphenylamine	15.62	169	2996072	157.74	ng/ul	100
65) 4-Bromophenyl-phenylether	16.29	248	1226913	161.46	ng/ul	95
66) Hexachlorobenzene	16.40	284	1339939	159.32	ng/ul	97
67) Atrazine	16.57	200	1202194	162.41	ng/ul	97
68) Pentachlorophenol	16.75	266	835218	173.59	ng/ul	99
69) Phenanthrene	17.14	178	5351890	151.49	ng/ul	99
71) Anthracene	17.23	178	5477338	152.26	ng/ul	98
72) Carbazole	17.51	167	4820787	154.52	ng/ul	99
73) Di-n-butylphthalate	18.06	149	5742178	163.61	ng/ul	100
74) Fluoranthene	19.16	202	6326796	152.59	ng/ul	98
77) Pyrene	19.53	202	6433913	151.34	ng/ul	99
78) Butylbenzylphthalate	20.42	149	2684079	173.21	ng/ul	95
79) 3,3'-Dichlorobenzidine	21.21	252	2309595	156.04	ng/ul	98
80) Benzo(a)anthracene	21.27	228	6703138	151.86	ng/ul	98
81) Bis(2-ethylhexyl)phthalate	21.19	149	3892495	170.40	ng/ul	98
82) Chrysene	21.33	228	6251739	147.81	ng/ul	97
84) Di-n-octyl phthalate	22.07	149	6824122	157.63	ng/ul	99
85) Benzo(b)fluoranthene	22.86	252	7440037	155.65	ng/ul	98
86) Benzo(k)fluoranthene	22.91	252	6605639	150.09	ng/ul	100
88) Benzo(a)pyrene	23.44	252	7000845	155.24	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.81	276	8688886	159.98	ng/ul	96
90) Dibenzo(a,h)anthracene	25.81	278	7303201	159.56	ng/ul	100
91) Benzo(g,h,i)perylene	26.50	276	7243614	159.05	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 57.75 ng/uL

RT: 3.29 min Scan# 119

Delta R.T. -0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51

Instrument :

BNA_M

ClientSampleId :

SSTD16039


Tgt Ion: 88 Resp: 217753

Ion Ratio Lower Upper

88 100

43 24.2 20.7 31.1




58 68.1 51.6 77.4

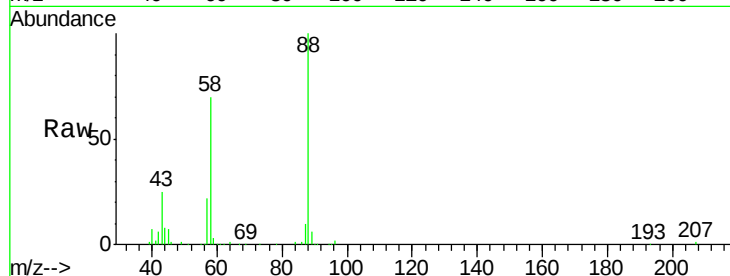

Abundance Ion 88.00 (87.70 to 88.70): BM008108.D (-115) (-)

Ion 43.00 (42.70 to 43.70): BM008108.D (-115) (-)

Ion 58.00 (57.70 to 58.70): BM008108.D (-115) (-)

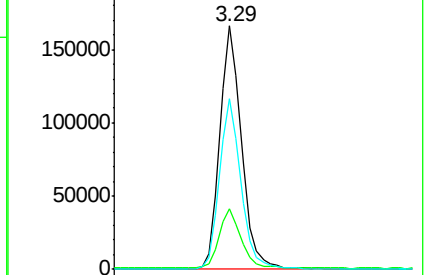

#4

Benzaldehyde

Concen: 168.99 ng/uL

RT: 6.86 min Scan# 727

Delta R.T. 0.00 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51


Tgt Ion: 77 Resp: 1229400

Ion Ratio Lower Upper

77 100

105 96.4 76.5 114.7



106 91.0 71.3 106.9




Abundance Ion 77.00 (76.70 to 77.70): BM008108.D (-693) (-)

Ion 105.00 (104.70 to 105.70): BM008108.D (-693) (-)

Ion 106.00 (105.70 to 106.70): BM008108.D (-693) (-)

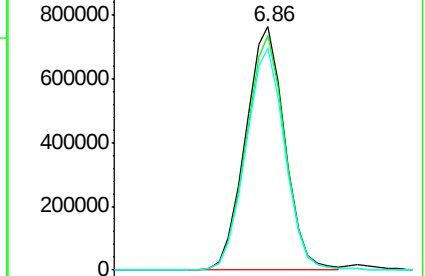

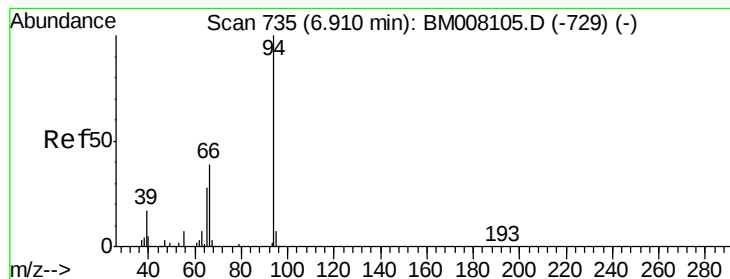

#6

Phenol

Concen: 154.72 ng/ul

RT: 6.92 min Scan# 737

Delta R.T. 0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51

Instrument :

BNA_M

ClientSampleId :

SSTD16039


Tgt Ion: 94 Resp: 1819807

Ion Ratio Lower Upper

94 100

65 28.5 23.1 34.7




66 40.6 33.7 50.5



Abundance Ion 94.00 (93.70 to 94.70): BM008108.D (-737) (-)

Ion 65.00 (64.70 to 65.70): BM008108.D (-737) (-)

Ion 66.00 (65.70 to 66.70): BM008108.D (-737) (-)

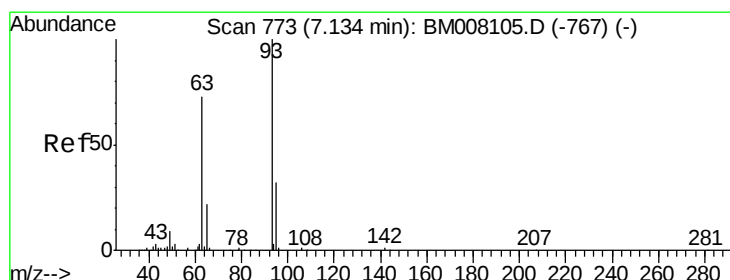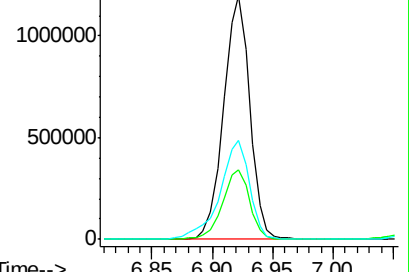

#8

Bis(2-Chloroethyl)ether

Concen: 152.78 ng/ul

RT: 7.15 min Scan# 775

Delta R.T. 0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51


Tgt Ion: 93 Resp: 1376862

Ion Ratio Lower Upper

93 100

63 70.4 58.4 87.6



95 32.6 25.4 38.2




Abundance Ion 93.00 (92.70 to 93.70): BM008108.D (-775) (-)

Ion 63.00 (62.70 to 63.70): BM008108.D (-775) (-)

Ion 95.00 (94.70 to 95.70): BM008108.D (-775) (-)

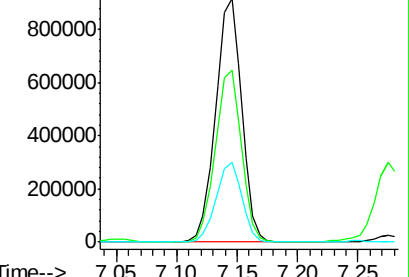



#10

2-Chlorophenol

Concen: 159.34 ng/ul

RT: 7.27 min Scan# 797

Delta R.T. 0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51

Instrument :

BNA_M

ClientSampleId :

SSTD16039


Tgt Ion:128 Resp: 1433371

Ion Ratio Lower Upper

128 100

64 47.8 38.7 58.1




130 32.1 26.9 40.3



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 130.00 (129.70 to 130.70): E

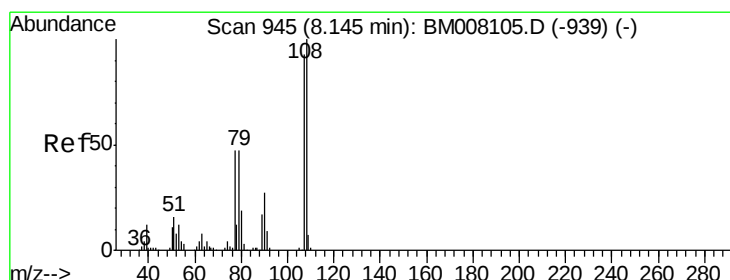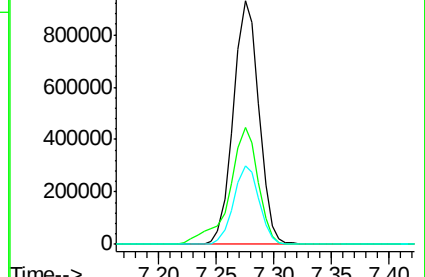

#11

2-Methylphenol

Concen: 156.58 ng/ul

RT: 8.15 min Scan# 946

Delta R.T. 0.01 min

Lab File: BM008108.D


Acq: 29 Nov 2016 18:51

Tgt Ion:108 Resp: 1345257

Ion Ratio Lower Upper



108 100


107 89.9 74.6 111.8



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E




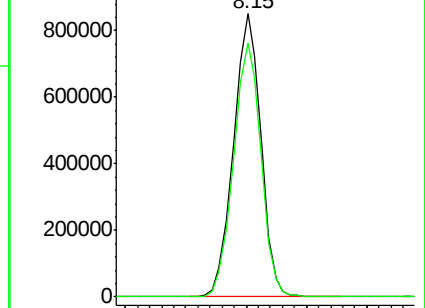




#12
 2,2'-oxybis(1-chloropropane)
 Concen: 146.85 ng/ul
 RT: 8.23 min Scan# 960
 Delta R.T. 0.00 min
 Lab File: BM008108.D
 Acq: 29 Nov 2016 18:51




Instrument :
 BNA_M
 ClientSampleId :
 SSTD16039


Tgt Ion: 45 Resp: 1469502
 Ion Ratio Lower Upper
 45 100
 77 18.7 13.8 20.6
 79 14.0 12.1 18.1

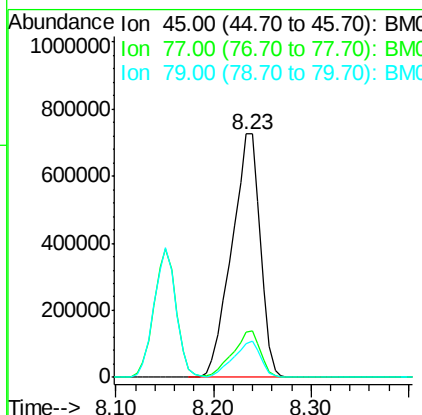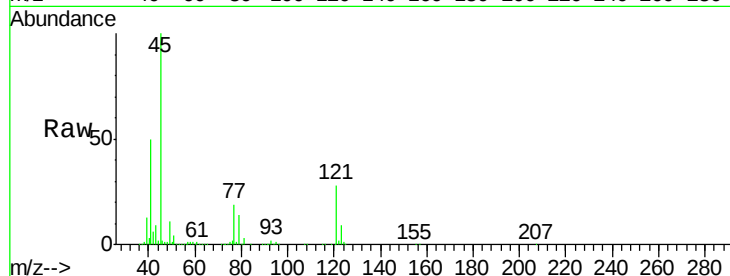

#14
 Acetophenone
 Concen: 153.38 ng/ul
 RT: 8.53 min Scan# 1011
 Delta R.T. 0.01 min
 Lab File: BM008108.D
 Acq: 29 Nov 2016 18:51

Tgt Ion: 105 Resp: 2158457
 Ion Ratio Lower Upper
 105 100
 77 77.9 64.2 96.4
 51 23.0 19.8 29.6



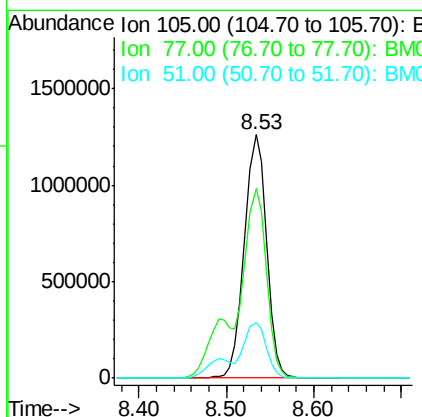



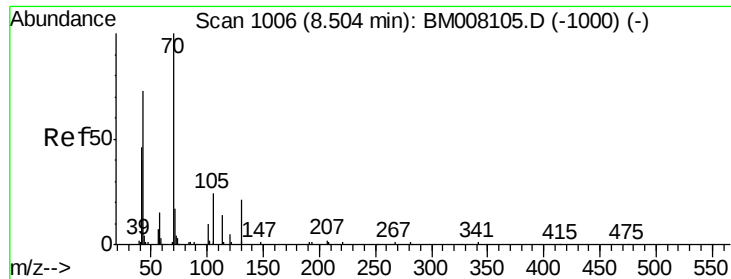

#15
N-Nitroso-di-n-propylamine
Concen: 153.57 ng/ul
RT: 8.54 min Scan# 1012
Delta R.T. 0.04 min
Lab File: BM008108.D
Acq: 29 Nov 2016 18:51




Instrument :
BNA_M
ClientSampleId :
SSTD16039


Tgt Ion: 70 Resp: 1079508
Ion Ratio Lower Upper
70 100
42 44.9 37.5 56.3
101 10.2 7.8 11.8
130 21.0 16.6 25.0

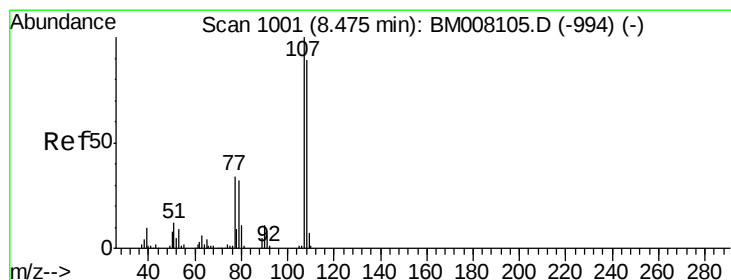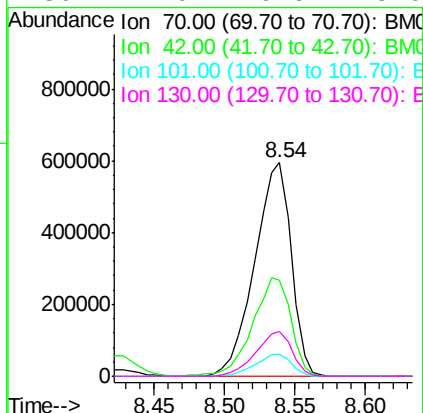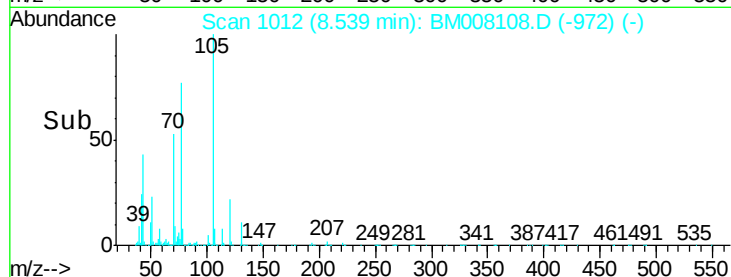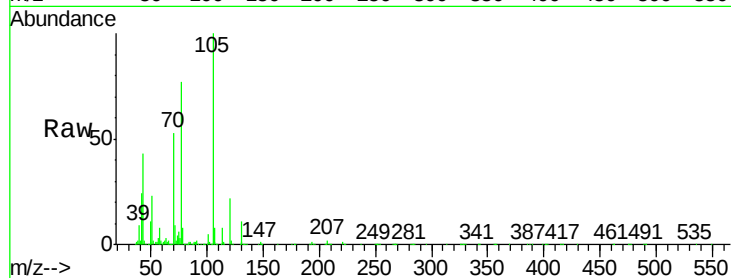

#16
4-Methylphenol
Concen: 153.78 ng/ul
RT: 8.49 min Scan# 1004
Delta R.T. 0.02 min
Lab File: BM008108.D
Acq: 29 Nov 2016 18:51

Tgt Ion: 108 Resp: 1421855
Ion Ratio Lower Upper
108 100
107 111.7 90.3 135.5

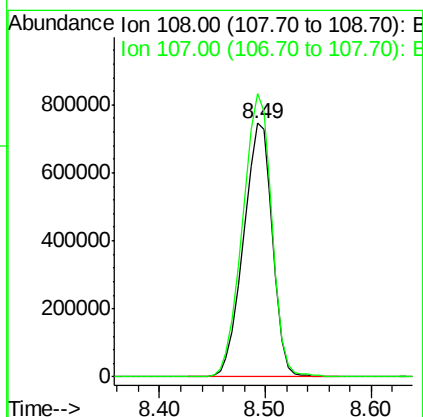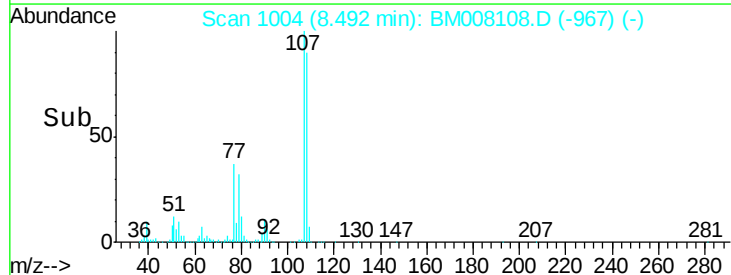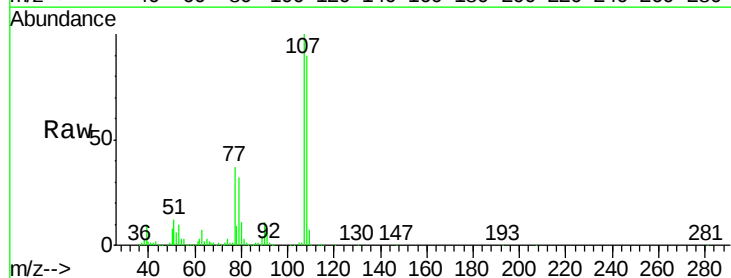

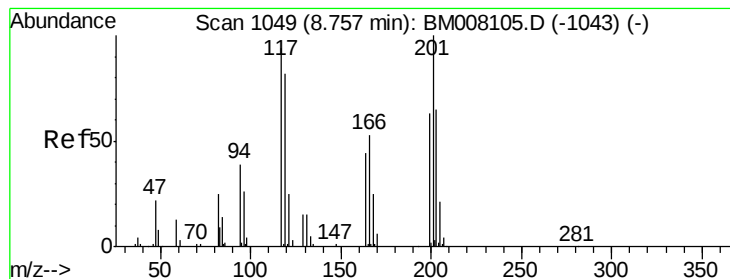

#17

Hexachloroethane

Concen: 156.90 ng/ul

RT: 8.76 min Scan# 1050

Delta R.T. 0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51

Instrument :

BNA_M

ClientSampleId :

SSTD16039


Tgt Ion: 117 Resp: 626619

Ion Ratio Lower Upper

117 100

201 116.6 85.4 128.2




199 75.5 54.1 81.1



Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

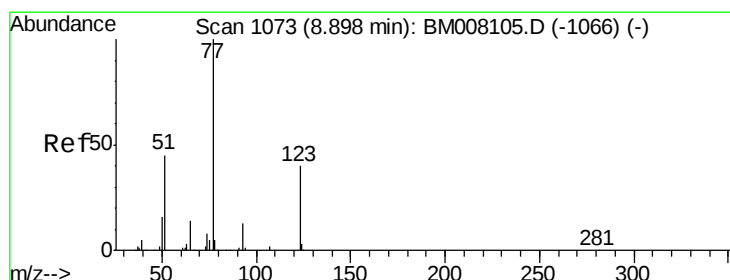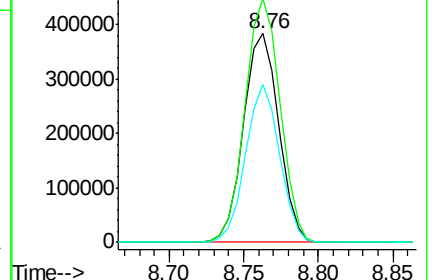

#20

Nitrobenzene

Concen: 160.43 ng/ul

RT: 8.91 min Scan# 1075

Delta R.T. 0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51


Tgt Ion: 77 Resp: 1638279

Ion Ratio Lower Upper

77 100

123 43.4 32.2 48.2



65 14.0 11.0 16.6




Abundance Ion 77.00 (76.70 to 77.70): BM

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BM

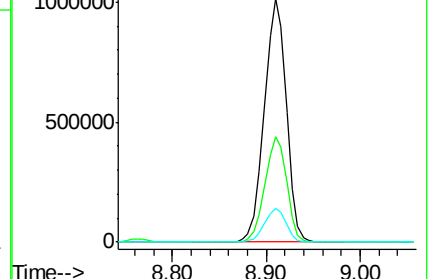



#21

Isophorone

Concen: 162.51 ng/ul

RT: 9.44 min Scan# 1165

Delta R.T. 0.02 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51

Instrument :

BNA_M

ClientSampleId :

SSTD16039


Tgt Ion: 82 Resp: 2873023

Ion Ratio Lower Upper

82 100

95 8.1 6.1 9.1

138 17.2 13.4 20.2




Abundance Ion 82.00 (81.70 to 82.70): BM008108.D (-1160) (-)

Ion 95.00 (94.70 to 95.70): BM008108.D (-1160) (-)

Ion 138.00 (137.70 to 138.70): BM008108.D (-1160) (-)

Time-->

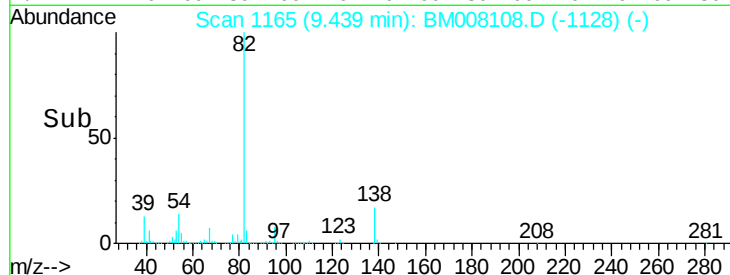


Abundance

Ion 82.00 (81.70 to 82.70): BM008108.D (-1160) (-)

Ion 95.00 (94.70 to 95.70): BM008108.D (-1160) (-)

Ion 138.00 (137.70 to 138.70): BM008108.D (-1160) (-)

Time-->



#23

2-Nitrophenol

Concen: 175.57 ng/ul

RT: 9.62 min Scan# 1195

Delta R.T. 0.01 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51


Tgt Ion: 139 Resp: 780864

Ion Ratio Lower Upper

139 100

65 52.8 42.3 63.5

109 36.3 29.7 44.5




Abundance Ion 139.00 (138.70 to 139.70): BM008108.D (-1160) (-)

Ion 65.00 (64.70 to 65.70): BM008108.D (-1160) (-)

Ion 109.00 (108.70 to 109.70): BM008108.D (-1160) (-)

Time-->




Abundance

Ion 139.00 (138.70 to 139.70): BM008108.D (-1160) (-)

Ion 65.00 (64.70 to 65.70): BM008108.D (-1160) (-)

Ion 109.00 (108.70 to 109.70): BM008108.D (-1160) (-)





Time-->



#24
 2,4-Dimethylphenol
 Concen: 160.48 ng/ul
 RT: 9.67 min Scan# 1205
 Delta R.T. 0.01 min
 Lab File: BM008108.D
 Acq: 29 Nov 2016 18:51




Instrument :
 BNA_M
 ClientSampleId :
 SSTD16039


Tgt Ion: 107 Resp: 1612022
 Ion Ratio Lower Upper
 107 100
 121 47.2 38.0 57.0
 122 78.1 62.2 93.2

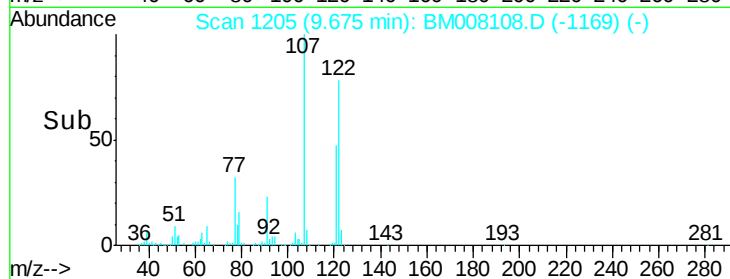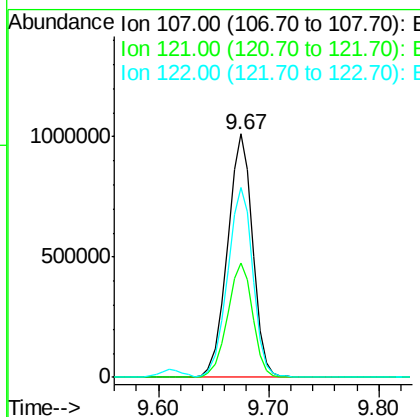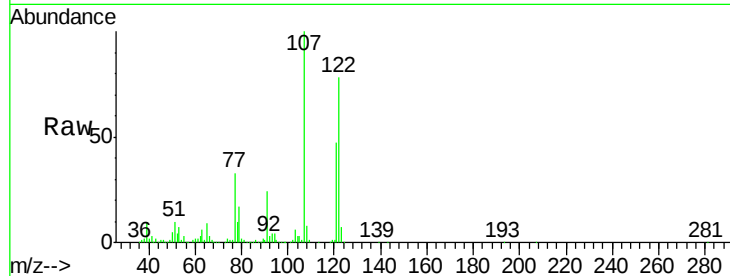

#25
 Bis(2-Chloroethoxy)methane
 Concen: 157.79 ng/ul
 RT: 9.91 min Scan# 1245
 Delta R.T. 0.01 min
 Lab File: BM008108.D
 Acq: 29 Nov 2016 18:51

Tgt Ion: 93 Resp: 1689005
 Ion Ratio Lower Upper
 93 100
 95 32.5 24.2 36.2
 123 10.9 8.2 12.2


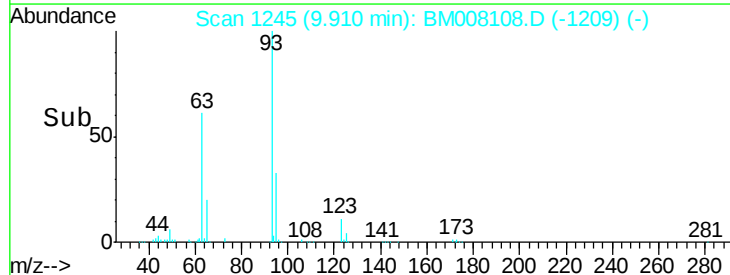
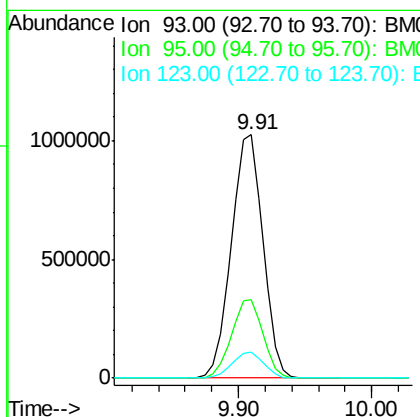





#27
2,4-Dichlorophenol
Concen: 165.19 ng/ul
RT: 10.14 min Scan# 1284
Delta R.T. 0.01 min
Lab File: BM008108.D
Acq: 29 Nov 2016 18:51




Instrument :
BNA_M
ClientSampleId :
SSTD16039


Tgt Ion:162 Resp: 1346680
Ion Ratio Lower Upper
162 100
164 65.2 50.8 76.2
98 38.3 29.8 44.6

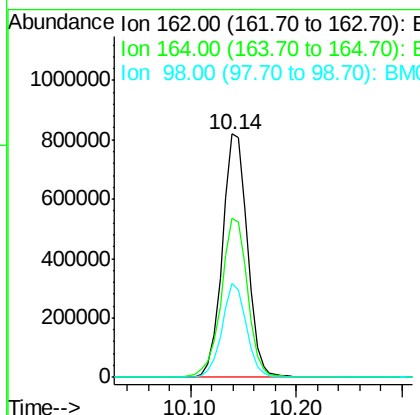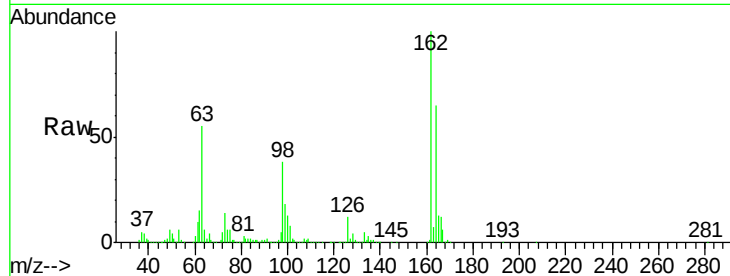

#28
Naphthalene
Concen: 154.19 ng/ul
RT: 10.53 min Scan# 1351
Delta R.T. 0.01 min
Lab File: BM008108.D
Acq: 29 Nov 2016 18:51

Tgt Ion:128 Resp: 4137250
Ion Ratio Lower Upper
128 100
129 11.0 8.3 12.5
127 13.0 10.6 16.0


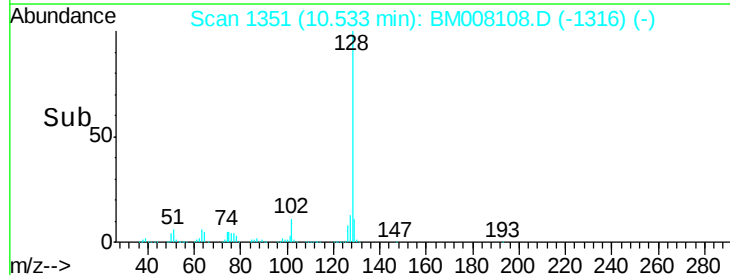
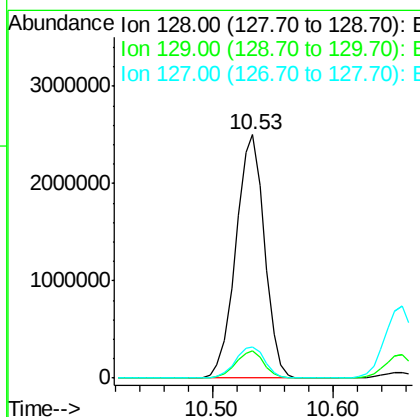





#30
4-Chloroaniline
Concen: 134.20 ng/ul
RT: 10.66 min Scan# 1372
Delta R.T. 0.01 min
Lab File: BM008108.D
Acq: 29 Nov 2016 18:51




Instrument :
BNA_M
ClientSampleId :
SSTD16039


Tgt Ion:127 Resp: 1241746
Ion Ratio Lower Upper
127 100
129 32.2 27.1 40.7

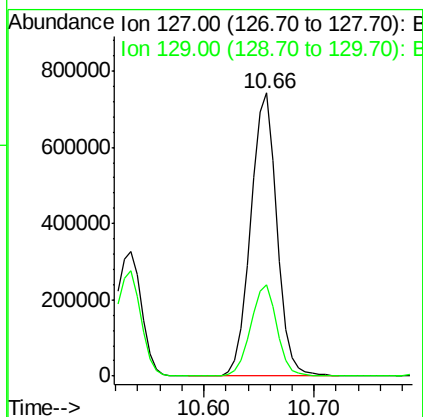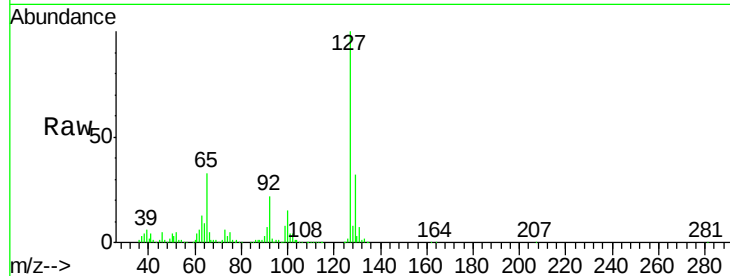

#31
Hexachlorobutadiene
Concen: 159.43 ng/ul
RT: 10.80 min Scan# 1397
Delta R.T. -0.00 min
Lab File: BM008108.D
Acq: 29 Nov 2016 18:51

Tgt Ion:225 Resp: 1061460
Ion Ratio Lower Upper
225 100
223 62.7 47.8 71.8
227 63.8 53.2 79.8

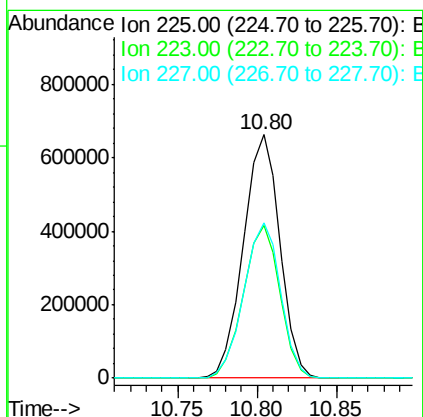



#32

Caprolactam

Concen: 101.48 ng/ul

RT: 11.49 min Scan# 1513

Delta R.T. 0.05 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51

Instrument :

BNA_M

ClientSampleId :

SSTD16039


Tgt Ion:113 Resp: 237447

Ion Ratio Lower Upper

113 100

55 147.5 117.0 175.4




56 119.5 97.7 146.5

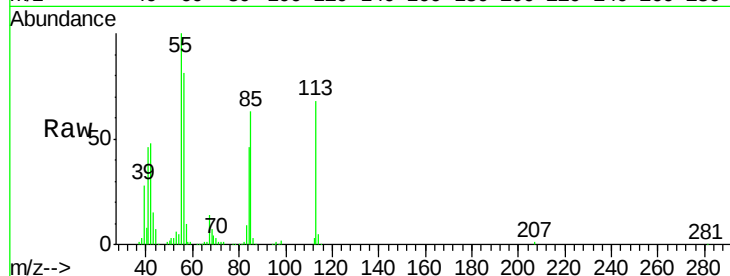

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM

Ion 56.00 (55.70 to 56.70): BM

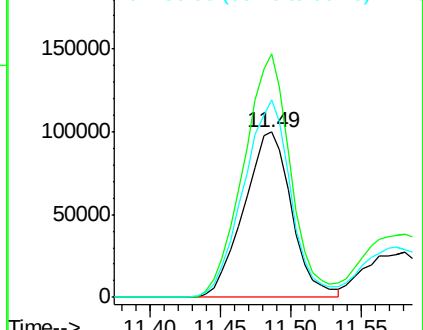

#33

4-Chloro-3-methylphenol

Concen: 163.91 ng/ul

RT: 11.80 min Scan# 1566

Delta R.T. 0.02 min

Lab File: BM008108.D

Acq: 29 Nov 2016 18:51


Tgt Ion:107 Resp: 1410682

Ion Ratio Lower Upper

107 100

144 24.2 19.4 29.2



142 73.0 58.0 87.0




Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E



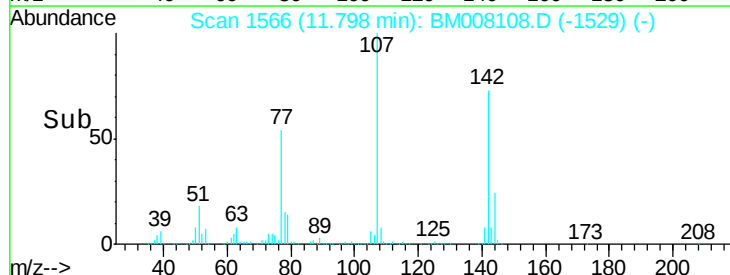
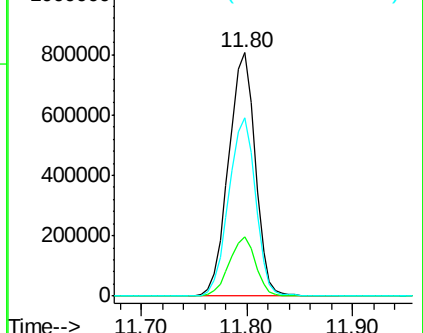


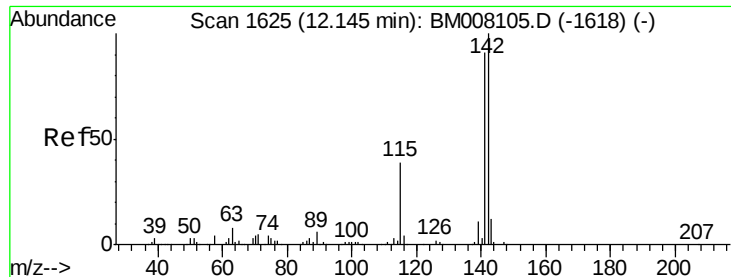

#34
 2-Methylnaphthalene
 Concen: 154.23 ng/ul
 RT: 12.15 min Scan# 1625
 Delta R.T. -0.00 min
 Lab File: BM008108.D
 Acq: 29 Nov 2016 18:51

Instrument :
 BNA_M
 ClientSampleId :
 SSTD16039

Tgt Ion:142 Resp: 2935423
 Ion Ratio Lower Upper
 142 100
 141 89.5 73.0 109.4

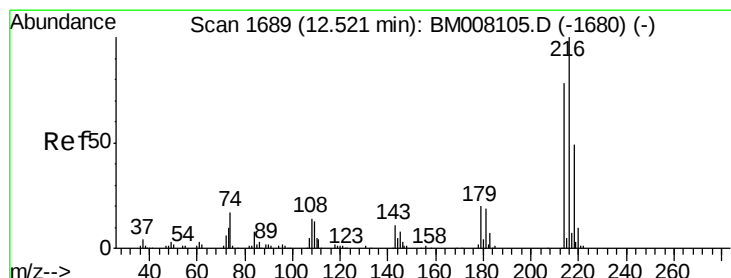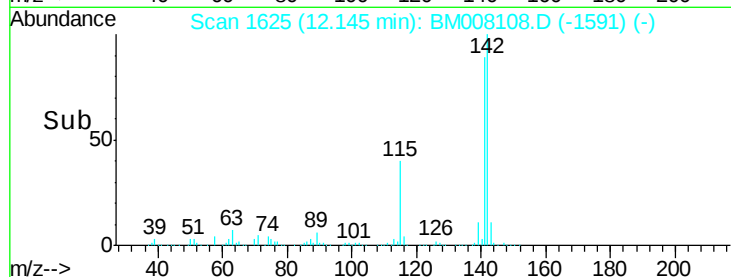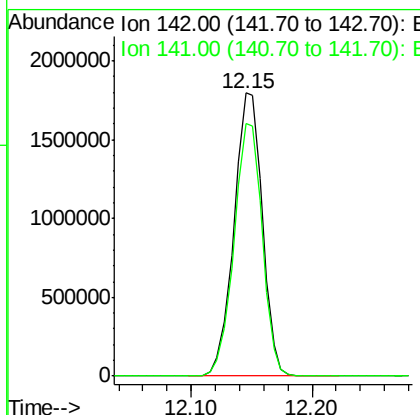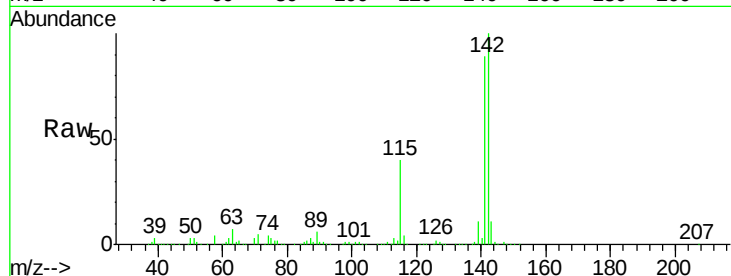

#36
 1,2,4,5-Tetrachlorobenzene
 Concen: 155.25 ng/ul
 RT: 12.52 min Scan# 1689
 Delta R.T. -0.00 min
 Lab File: BM008108.D
 Acq: 29 Nov 2016 18:51

Tgt Ion:216 Resp: 1761190
 Ion Ratio Lower Upper
 216 100
 214 79.4 62.0 93.0
 179 20.4 16.2 24.4
 108 15.6 11.8 17.6

