

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037785.D
 Acq On : 29 Nov 2022 11:17
 Operator : CG/JU
 Sample : PB149029BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK029

Quant Time: Nov 29 23:35:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	4651	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	15086	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	8059	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.463	188	14751	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.629	240	9380	0.400	ng/ul	# 0.00
23) Perylene-d12	24.114	264	8479	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	38020	7.031	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.500	152	6577	0.263	ng/ul	0.00
18) Fluoranthene-d10	19.477	212	10421	0.336	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.716	166	2524	0.067	ng/ul#	15
20) Pyrene	19.845	202	2343	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.956	252	3944	0.117	ng/ul#	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037785.D
Acq On : 29 Nov 2022 11:17
Operator : CG/JU
Sample : PB149029BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK029

Quant Time: Nov 29 23:35:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration




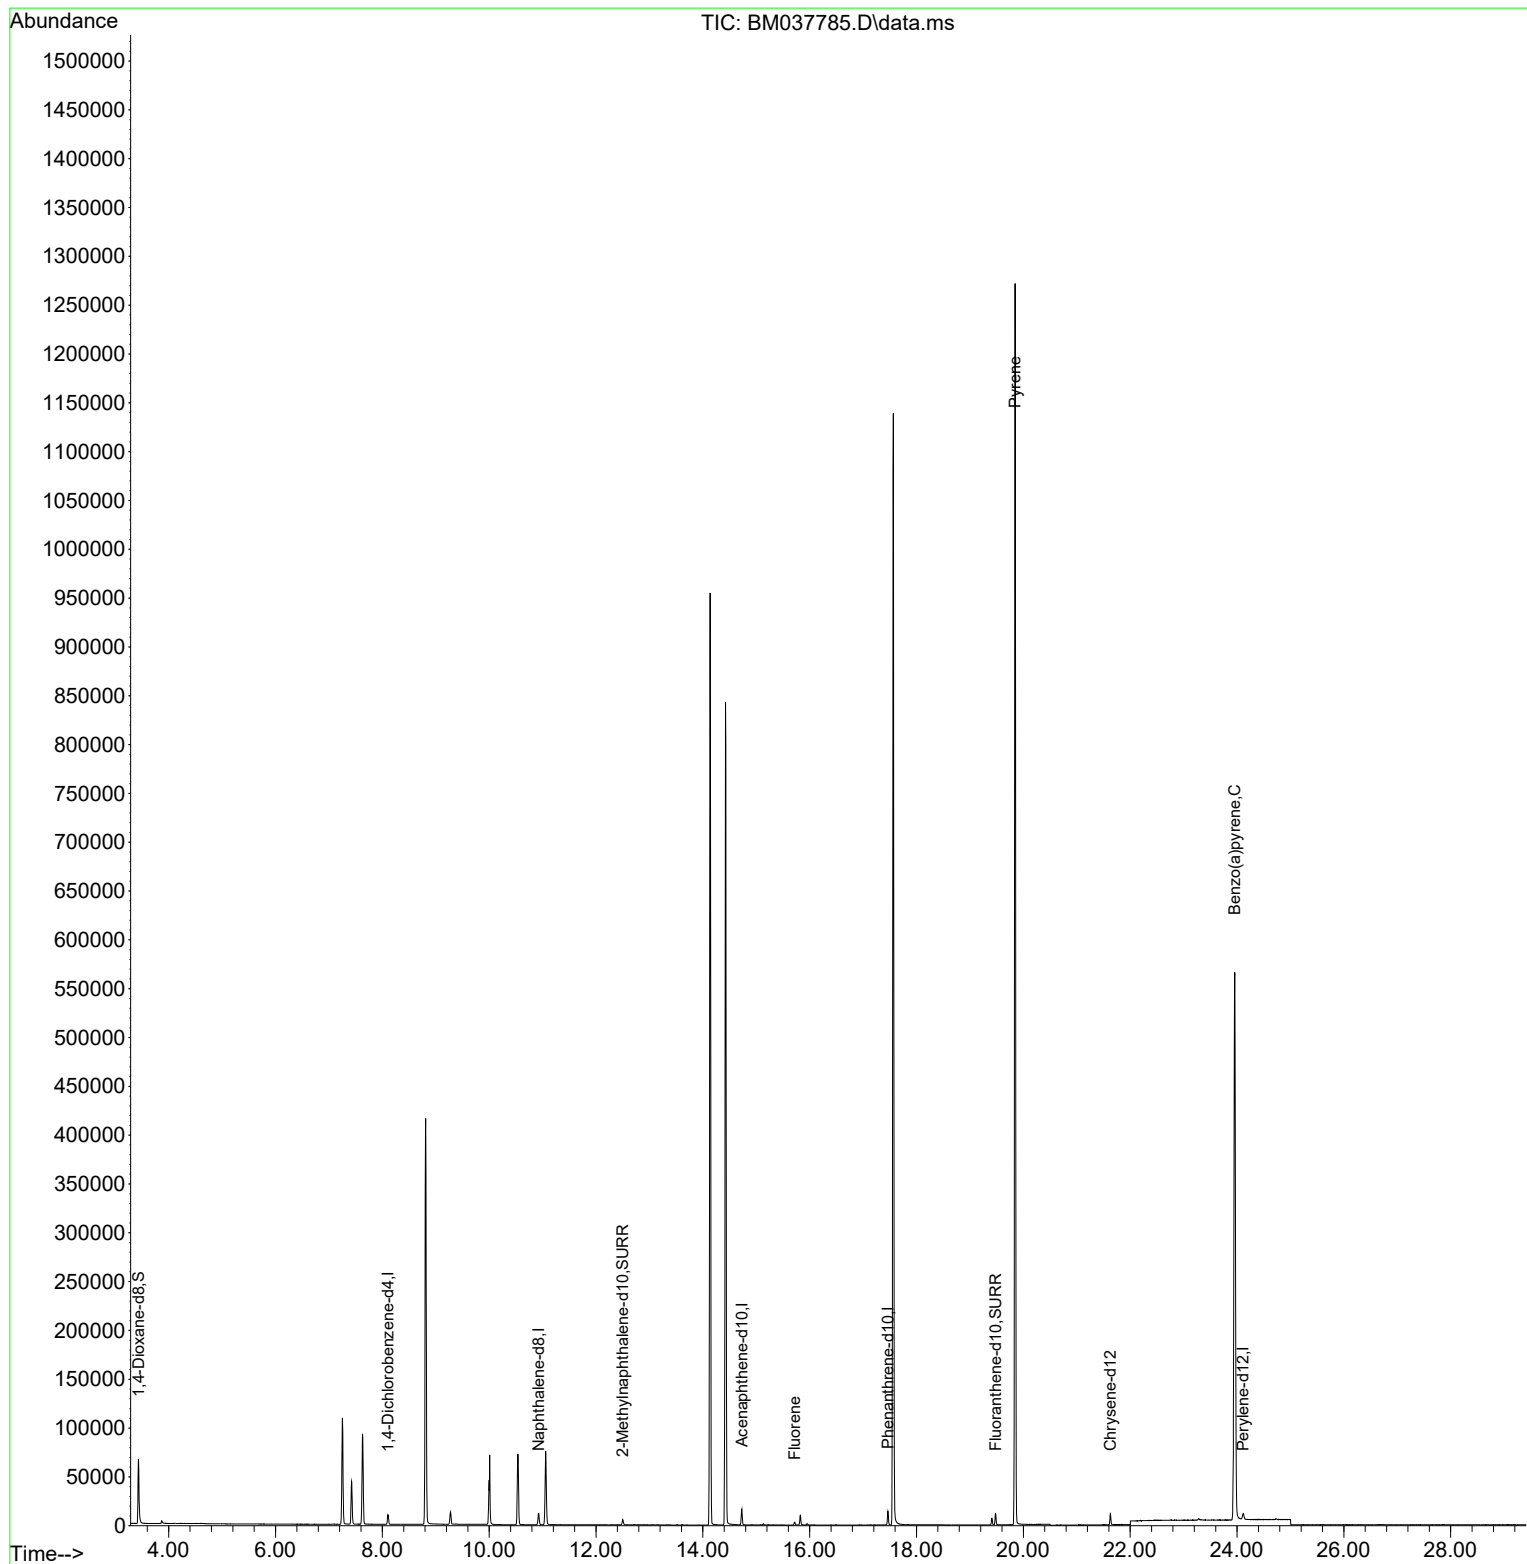


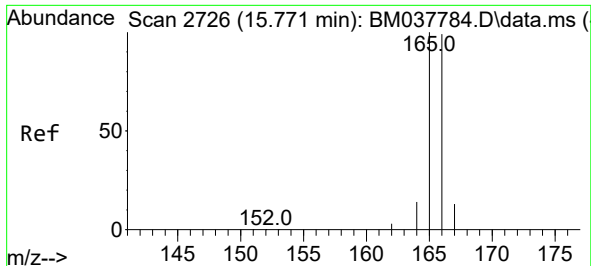

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.716 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM037785.D
Acq: 29 Nov 2022 11:17




Instrument :
BNA_M
ClientSampleId :
SBLK029


Tgt Ion:166 Resp: 2524
Ion Ratio Lower Upper
166 100
165 9.2 78.7 118.1#
167 33.7 11.3 16.9#

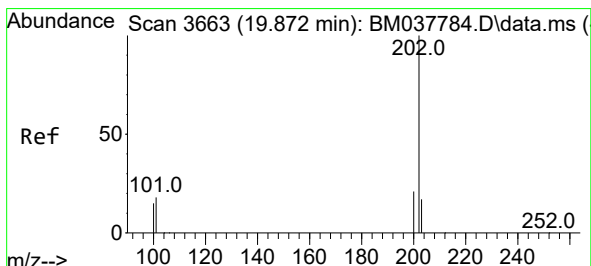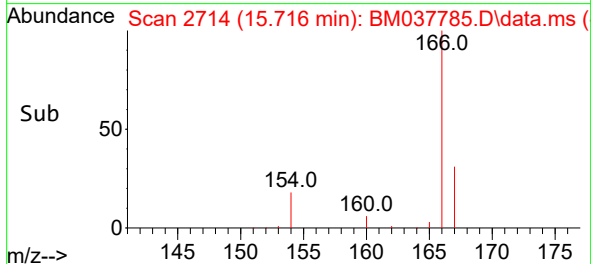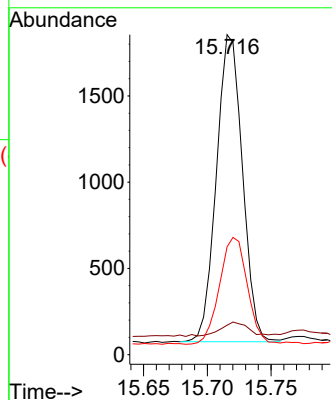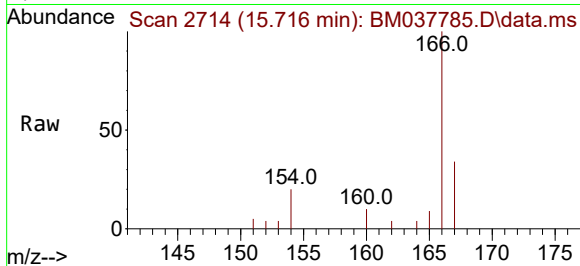

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.845 min Scan# 3657
Delta R.T. -0.027 min
Lab File: BM037785.D
Acq: 29 Nov 2022 11:17


Tgt Ion:202 Resp: 2343
Ion Ratio Lower Upper
202 100
101 240.5 10.1 15.1#
100 1872.9 8.0 12.0#

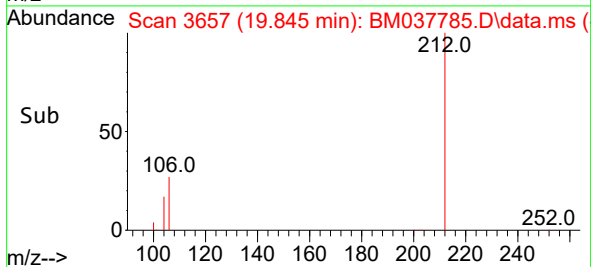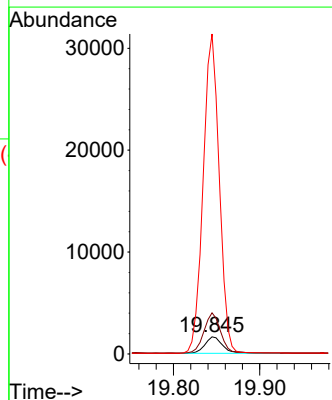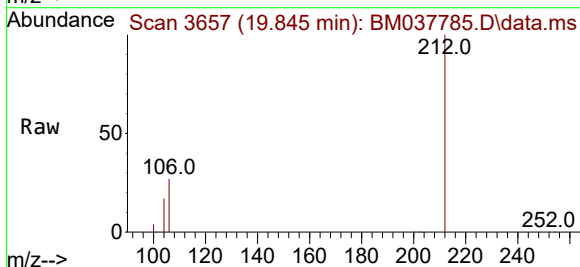

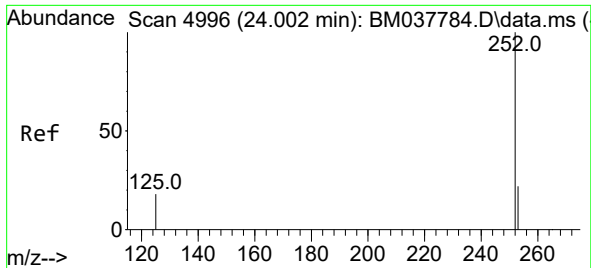

#26
Benzo(a)pyrene
Concen: 0.117 ng/ul
RT: 23.956 min Scan# 49
Delta R.T. -0.046 min
Lab File: BM037785.D
Acq: 29 Nov 2022 11:17

Instrument :
BNA_M
ClientSampleId :
SBLK029

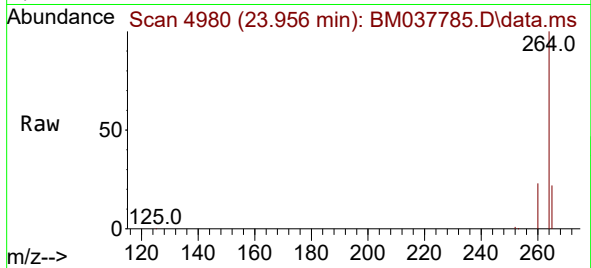

Tgt Ion:252 Resp: 3944
Ion Ratio Lower Upper
252 100
253 57.1 18.8 28.2#
125 70.1 10.5 15.7#

