

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037786.D
 Acq On : 29 Nov 2022 11:54
 Operator : CG/JU
 Sample : PB149031BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK031

Quant Time: Nov 29 23:35:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	4842	0.400	ng/ul	0.00
4) Naphthalene-d8	10.926	136	15923	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	8619	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.467	188	15870	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.631	240	9746	0.400	ng/ul	# 0.00
23) Perylene-d12	24.113	264	8493	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	41882	7.440	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	7660	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	12147	0.377	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.720	166	2865	0.071	ng/ul#	14
20) Pyrene	19.849	202	2663	0.054	ng/ul#	1
26) Benzo(a)pyrene	23.958	252	4074	0.121	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037786.D
Acq On : 29 Nov 2022 11:54
Operator : CG/JU
Sample : PB149031BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK031

Quant Time: Nov 29 23:35:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration




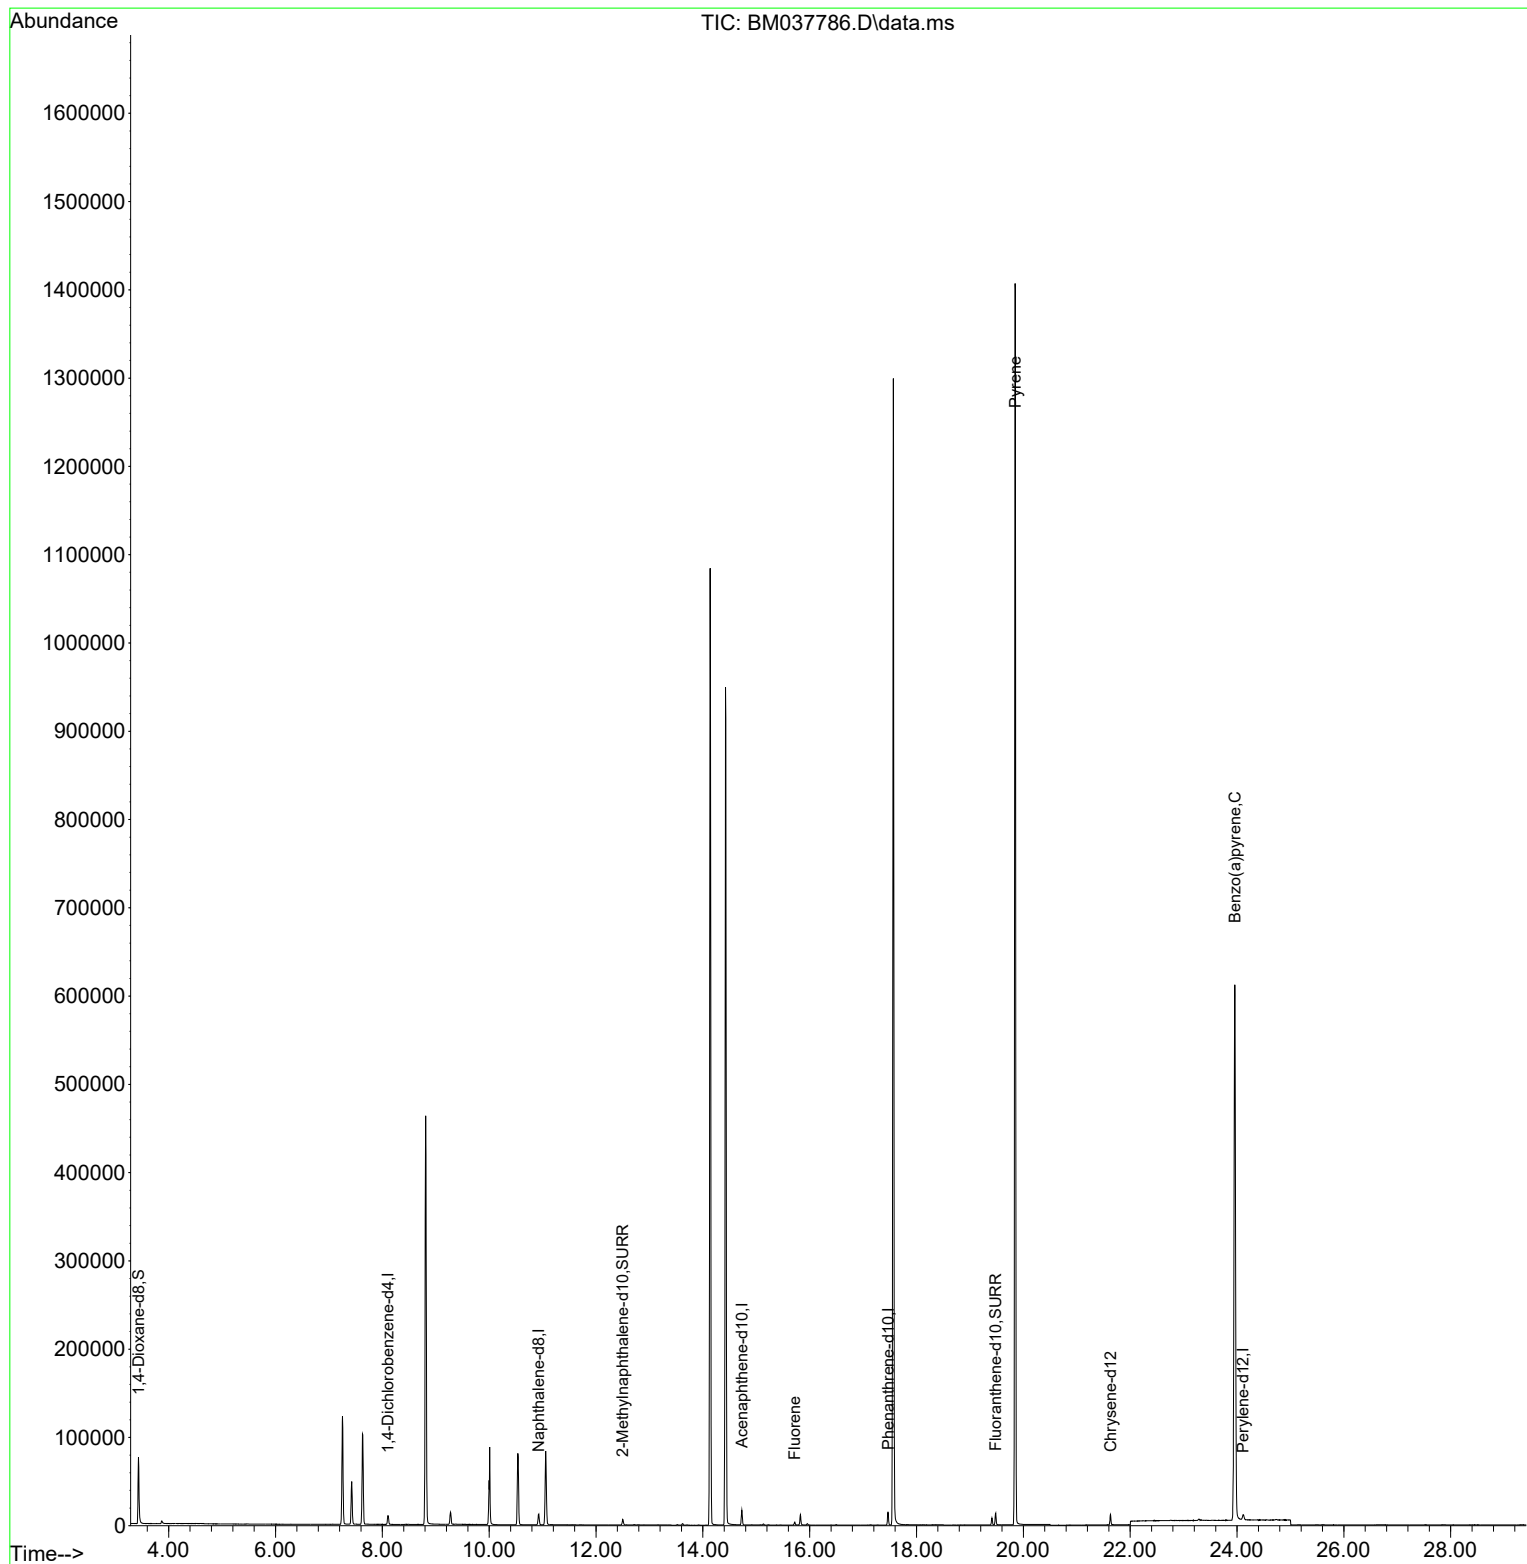


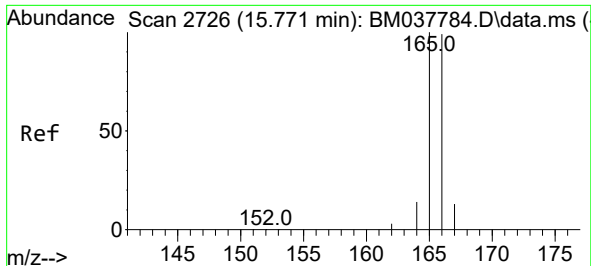

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.720 min Scan# 21
Delta R.T. -0.051 min
Lab File: BM037786.D
Acq: 29 Nov 2022 11:54




Instrument :
BNA_M
ClientSampleId :
SBLK031


Tgt Ion:166 Resp: 2865
Ion Ratio Lower Upper
166 100
165 8.7 78.7 118.1#
167 34.9 11.3 16.9#

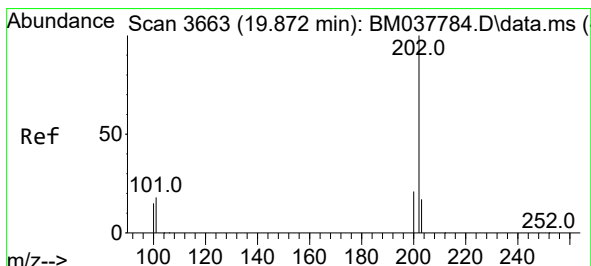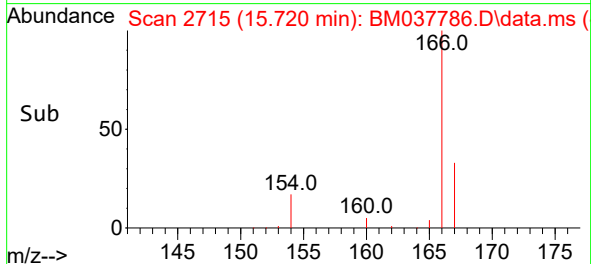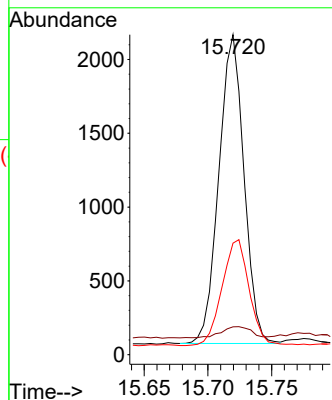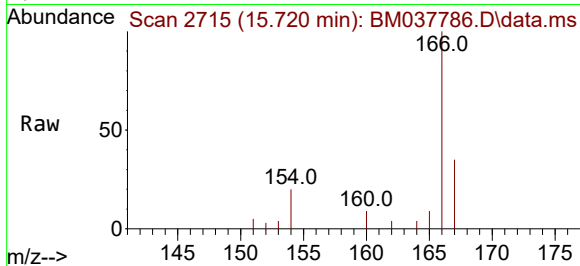

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.849 min Scan# 3658
Delta R.T. -0.023 min
Lab File: BM037786.D
Acq: 29 Nov 2022 11:54


Tgt Ion:202 Resp: 2663
Ion Ratio Lower Upper
202 100
101 208.9 10.1 15.1#
100 1539.9 8.0 12.0#

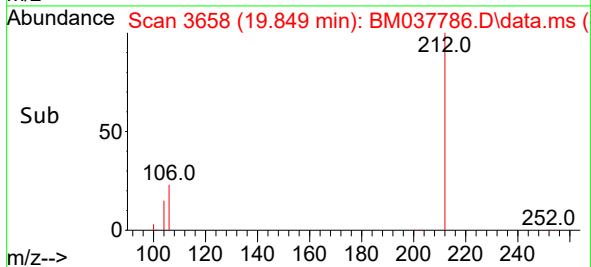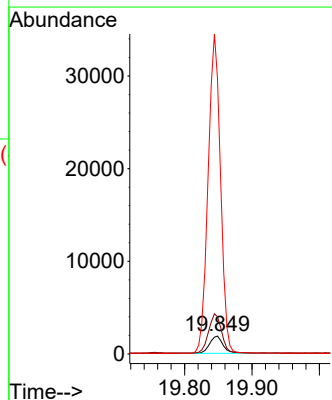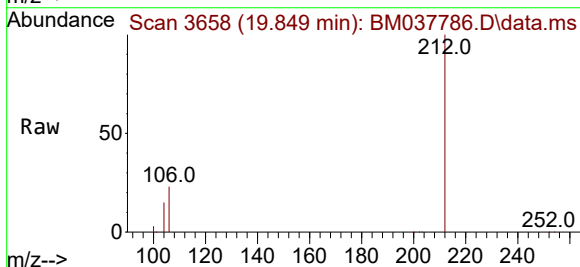

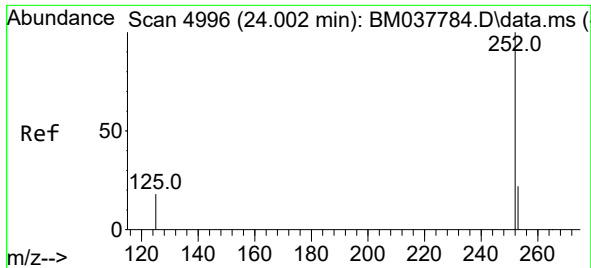

#26
Benzo(a)pyrene
Concen: 0.121 ng/ul
RT: 23.958 min Scan# 4996
Delta R.T. -0.044 min
Lab File: BM037786.D
Acq: 29 Nov 2022 11:54

Instrument :
BNA_M
ClientSampleId :
SBLK031

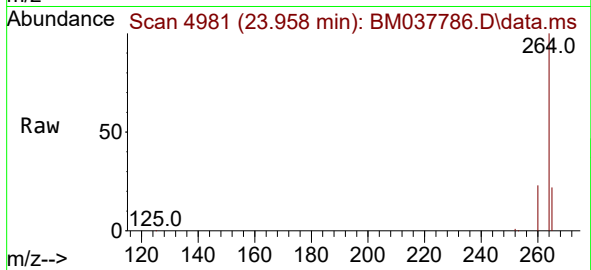

Tgt Ion:252 Resp: 4074
Ion Ratio Lower Upper
252 100
253 60.0 18.8 28.2#
125 70.3 10.5 15.7#

