

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037793.D
 Acq On : 29 Nov 2022 16:17
 Operator : CG/JU
 Sample : PB149262BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK262

Quant Time: Nov 29 23:36:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	5845	0.400	ng/ul	0.00
4) Naphthalene-d8	10.925	136	19537	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.728	164	10504	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.466	188	19480	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.633	240	12016	0.400	ng/ul	# 0.00
23) Perylene-d12	24.121	264	10707	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	34731	5.111	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.498	152	6428	0.198	ng/ul	0.00
18) Fluoranthene-d10	19.480	212	10262	0.258	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.718	166	2414	0.049	ng/ul#	15
20) Pyrene	19.848	202	2185	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.963	252	3494	0.082	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037793.D
Acq On : 29 Nov 2022 16:17
Operator : CG/JU
Sample : PB149262BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Quant Time: Nov 29 23:36:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration




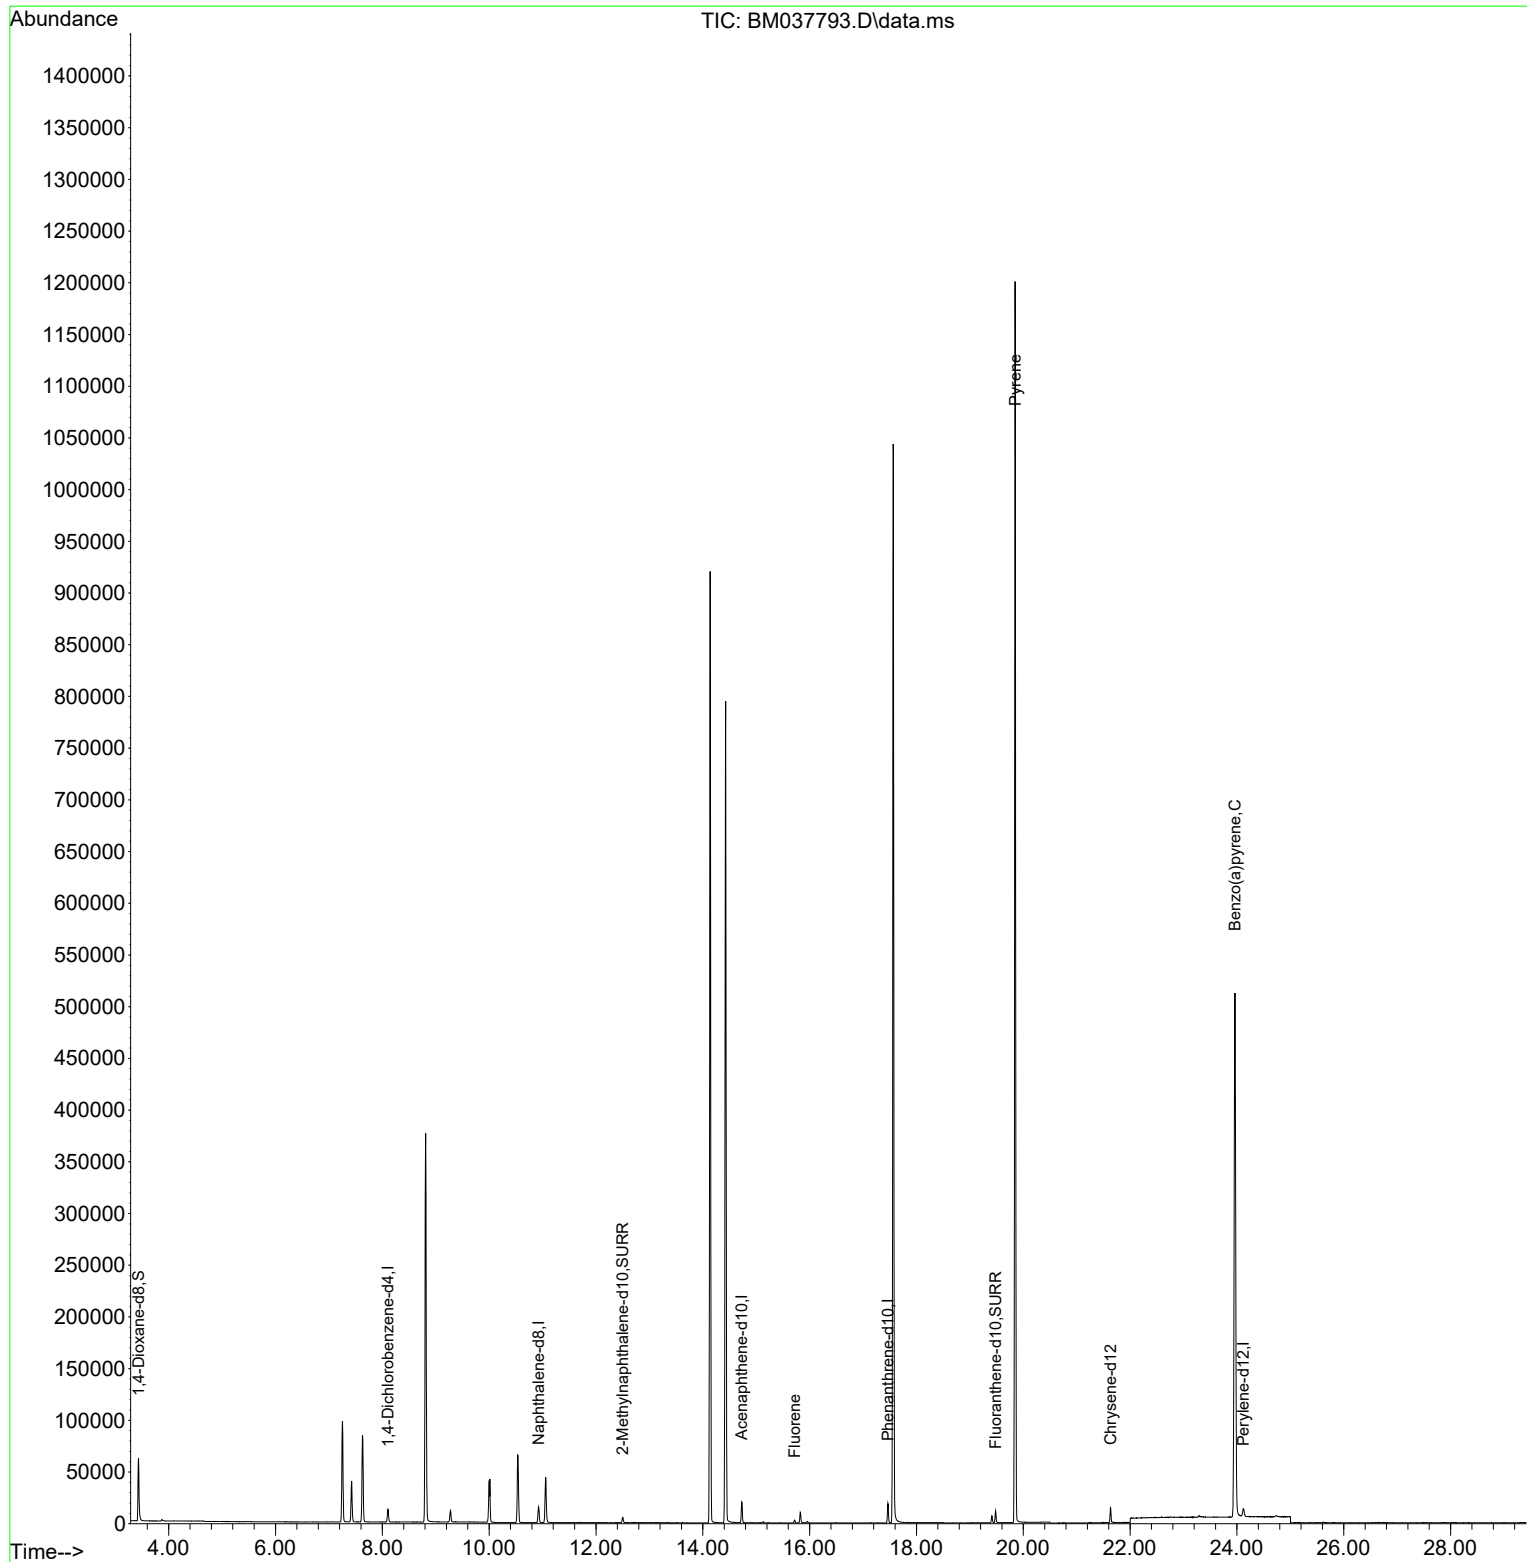


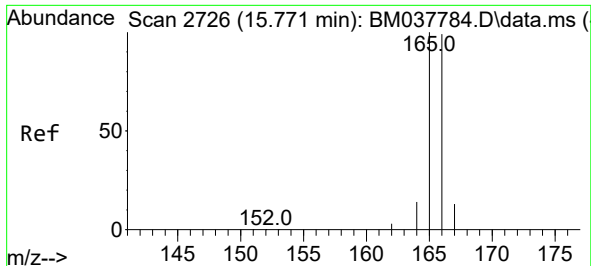

#12
Fluorene
Concen: 0.049 ng/ul
RT: 15.718 min Scan# 21
Delta R.T. -0.052 min
Lab File: BM037793.D
Acq: 29 Nov 2022 16:17




Instrument :
BNA_M
ClientSampleId :
SBLK262


Tgt Ion:166 Resp: 2414
Ion Ratio Lower Upper
166 100
165 9.9 78.7 118.1#
167 35.3 11.3 16.9#

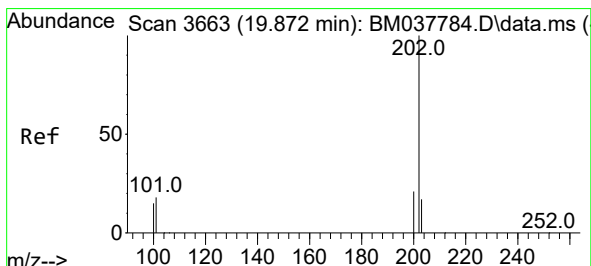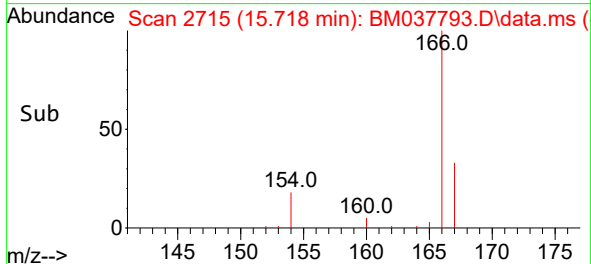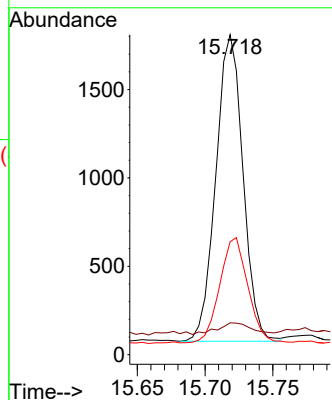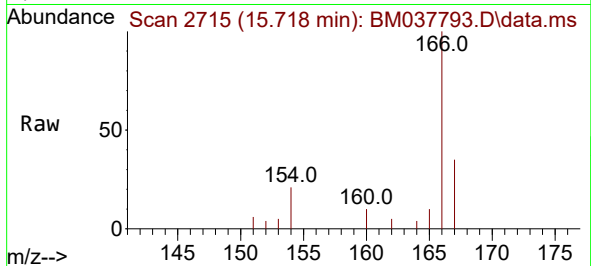

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.848 min Scan# 3658
Delta R.T. -0.024 min
Lab File: BM037793.D
Acq: 29 Nov 2022 16:17


Tgt Ion:202 Resp: 2185
Ion Ratio Lower Upper
202 100
101 229.8 10.1 15.1#
100 1745.6 8.0 12.0#

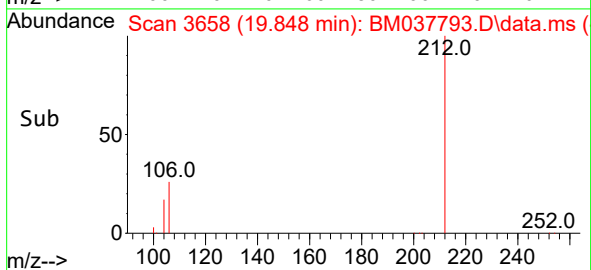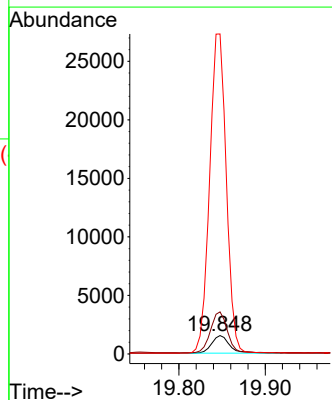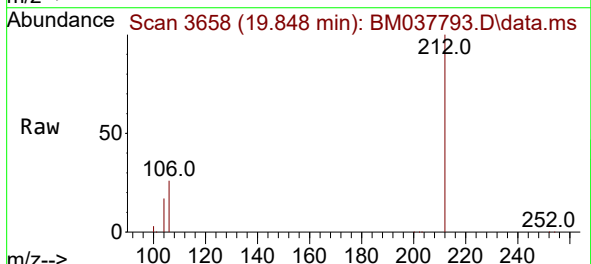

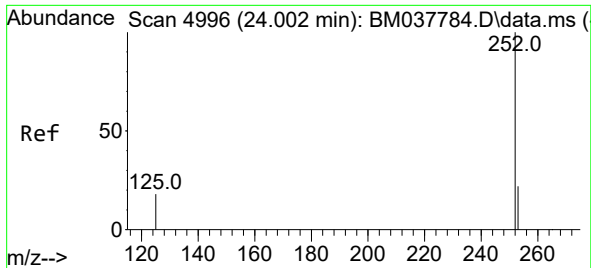

#26
Benzo(a)pyrene
Concen: 0.082 ng/ul
RT: 23.963 min Scan# 4983
Delta R.T. -0.039 min
Lab File: BM037793.D
Acq: 29 Nov 2022 16:17

Instrument :
BNA_M
ClientSampleId :
SBLK262

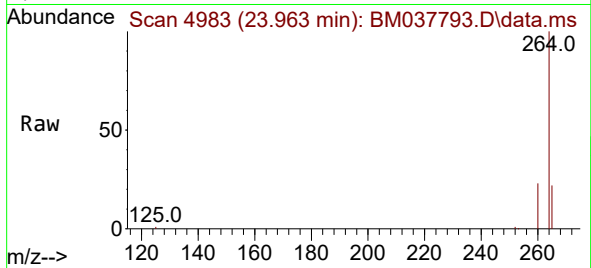

Tgt Ion:252 Resp: 3494
Ion Ratio Lower Upper
252 100
253 63.4 18.8 28.2#
125 82.1 10.5 15.7#

