

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037794.D
 Acq On : 29 Nov 2022 16:54
 Operator : CG/JU
 Sample : N5661-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9823

Quant Time: Nov 29 23:36:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	6358	0.400	ng/ul	0.00
4) Naphthalene-d8	10.926	136	21415	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	11459	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.467	188	21350	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.631	240	14112	0.400	ng/ul	# 0.00
23) Perylene-d12	24.116	264	12412	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	54889	7.425	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	10705	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	17364	0.372	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.720	166	3775	0.071	ng/ul#	14
20) Pyrene	19.849	202	3624	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.958	252	5853	0.119	ng/ul#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037794.D
Acq On : 29 Nov 2022 16:54
Operator : CG/JU
Sample : N5661-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9823

Quant Time: Nov 29 23:36:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration




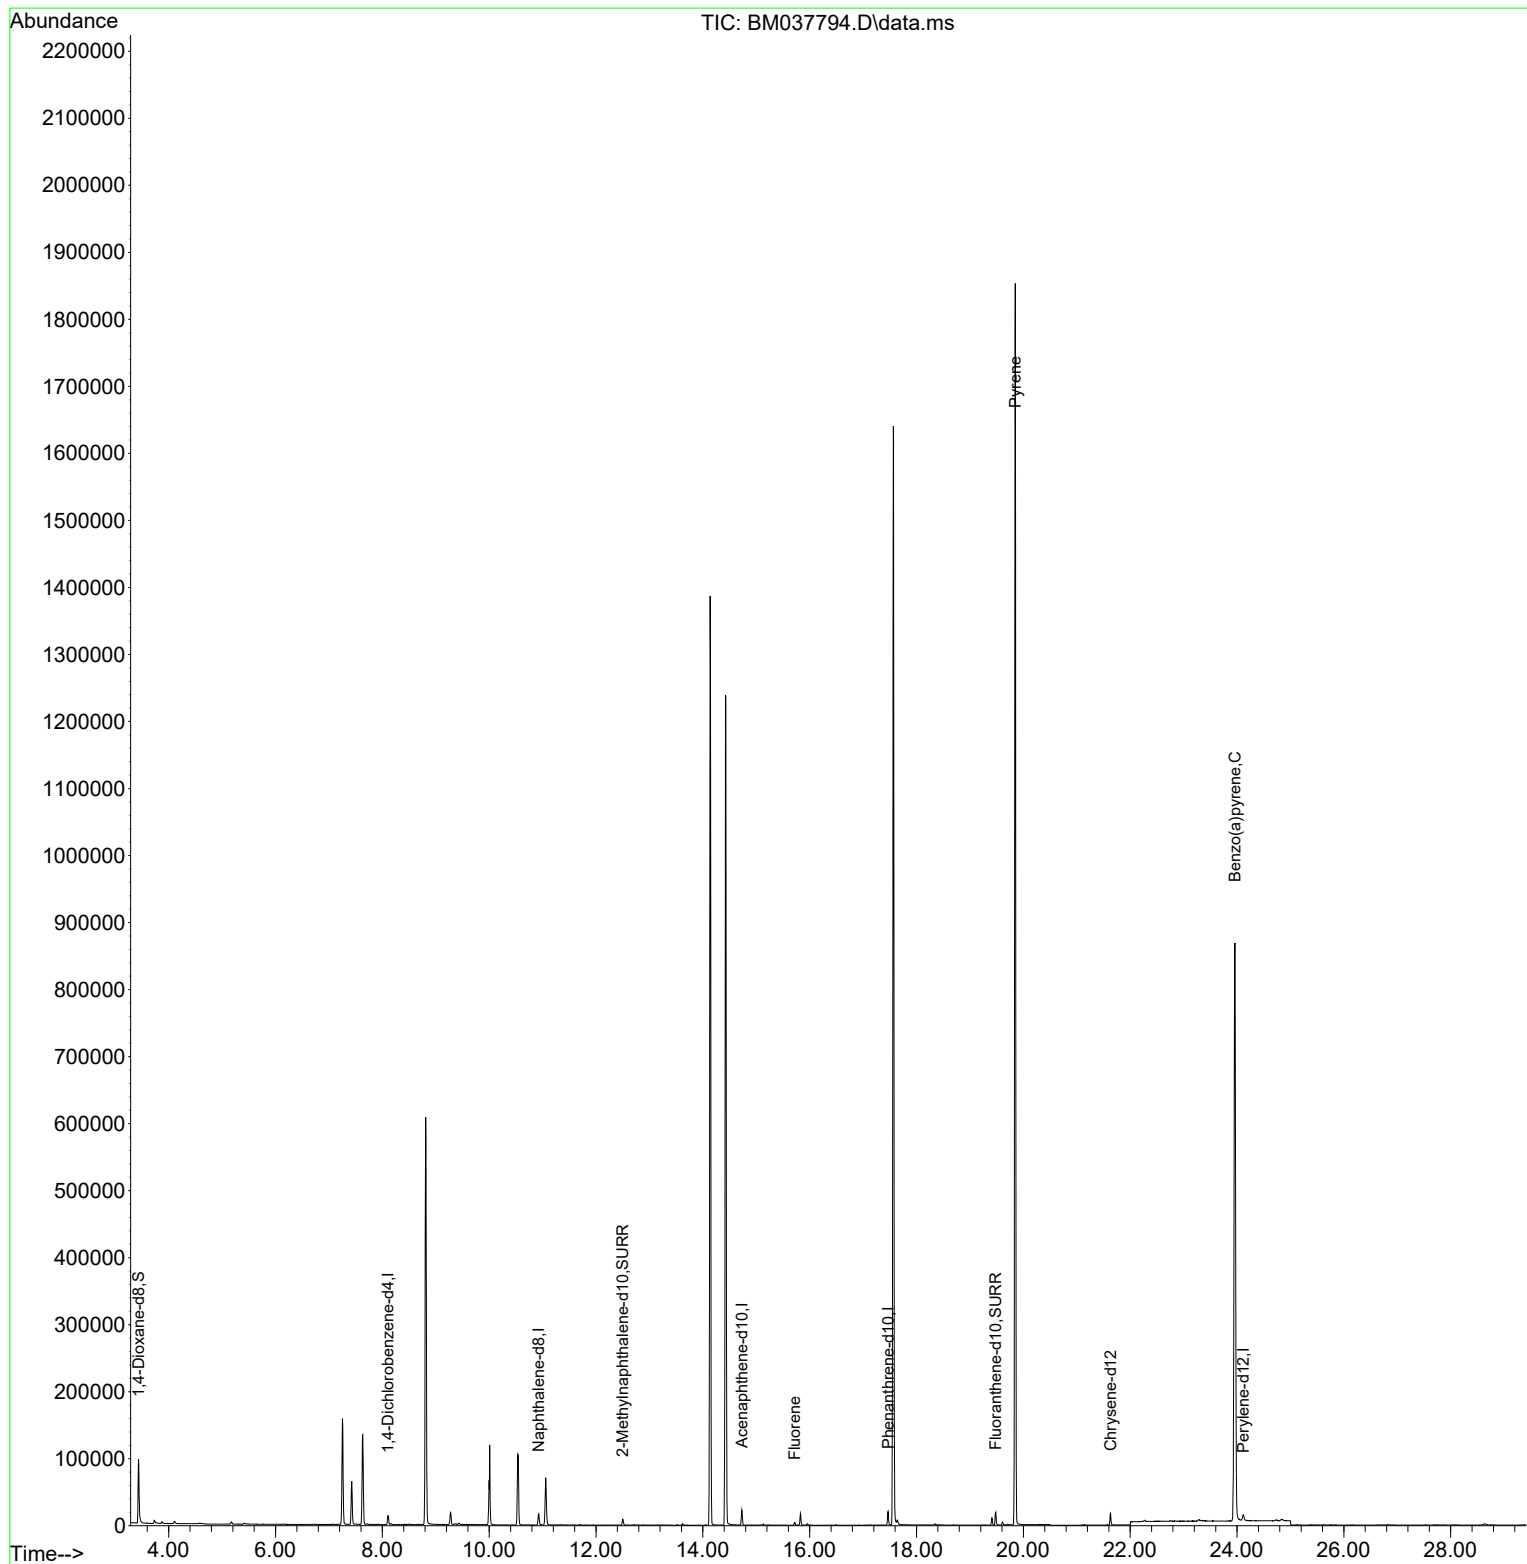


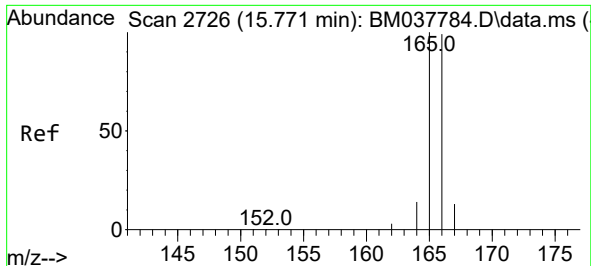

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.720 min Scan# 21
Delta R.T. -0.051 min
Lab File: BM037794.D
Acq: 29 Nov 2022 16:54




Instrument :
BNA_M
ClientSampleId :
C9823


Tgt Ion:166 Resp: 3775
Ion Ratio Lower Upper
166 100
165 7.9 78.7 118.1#
167 33.2 11.3 16.9#

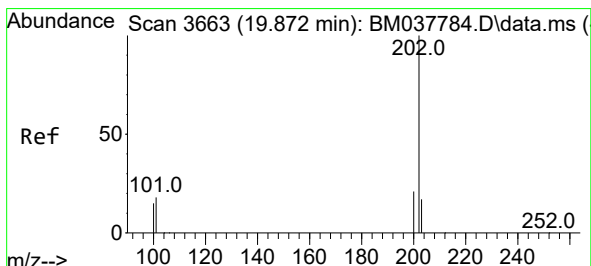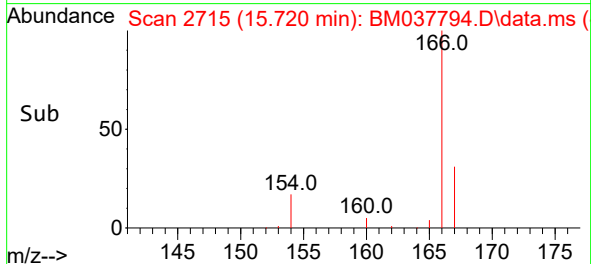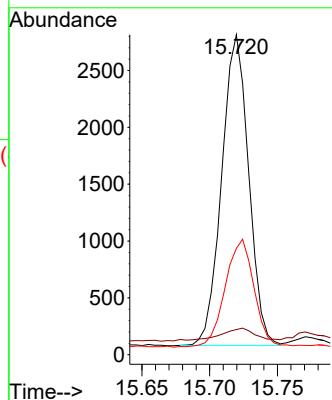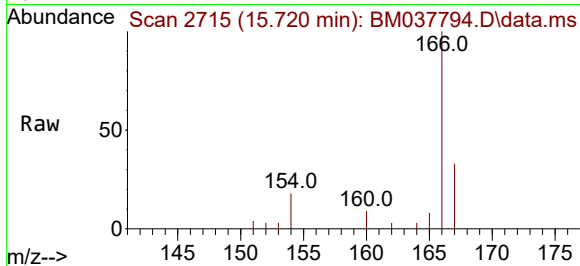

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.849 min Scan# 3658
Delta R.T. -0.023 min
Lab File: BM037794.D
Acq: 29 Nov 2022 16:54


Tgt Ion:202 Resp: 3624
Ion Ratio Lower Upper
202 100
101 214.6 10.1 15.1#
100 1634.5 8.0 12.0#

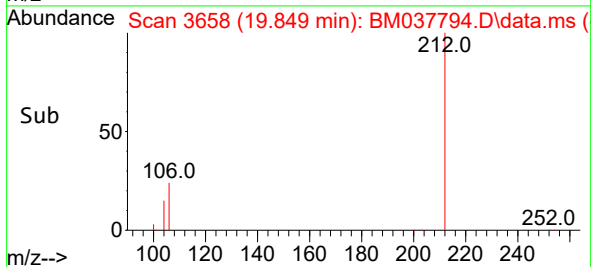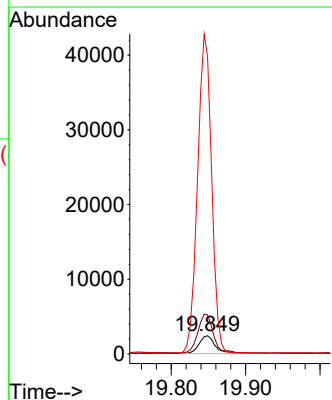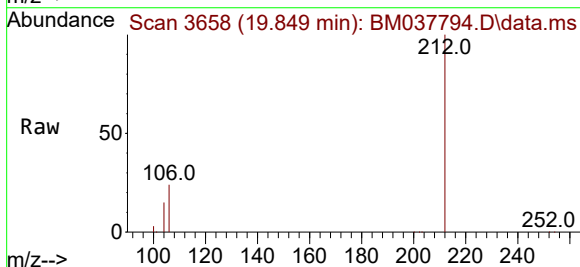

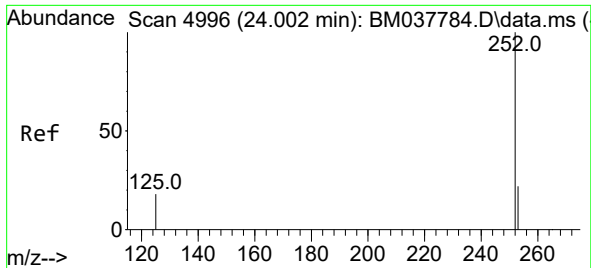

#26
Benzo(a)pyrene
Concen: 0.119 ng/ul
RT: 23.958 min Scan# 4996
Delta R.T. -0.044 min
Lab File: BM037794.D
Acq: 29 Nov 2022 16:54

Instrument :
BNA_M
ClientSampleId :
C9823

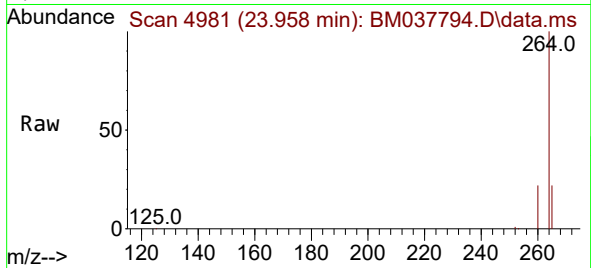

Tgt Ion:252 Resp: 5853
Ion Ratio Lower Upper
252 100
253 54.5 18.8 28.2#
125 67.1 10.5 15.7#

