

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037788.D
 Acq On : 29 Nov 2022 13:07
 Operator : CG/JU
 Sample : N5592-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AA3

Quant Time: Nov 29 23:36:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	7112	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	23509	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	12470	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.463	188	23298	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.632	240	14549	0.400	ng/ul	# 0.00
23) Perylene-d12	24.116	264	12782	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.439	96	33106	4.004	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	8164	0.209	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	16294	0.339	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.472	88	7934	0.922	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037788.D
Acq On : 29 Nov 2022 13:07
Operator : CG/JU
Sample : N5592-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AA3


Quant Time: Nov 29 23:36:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration

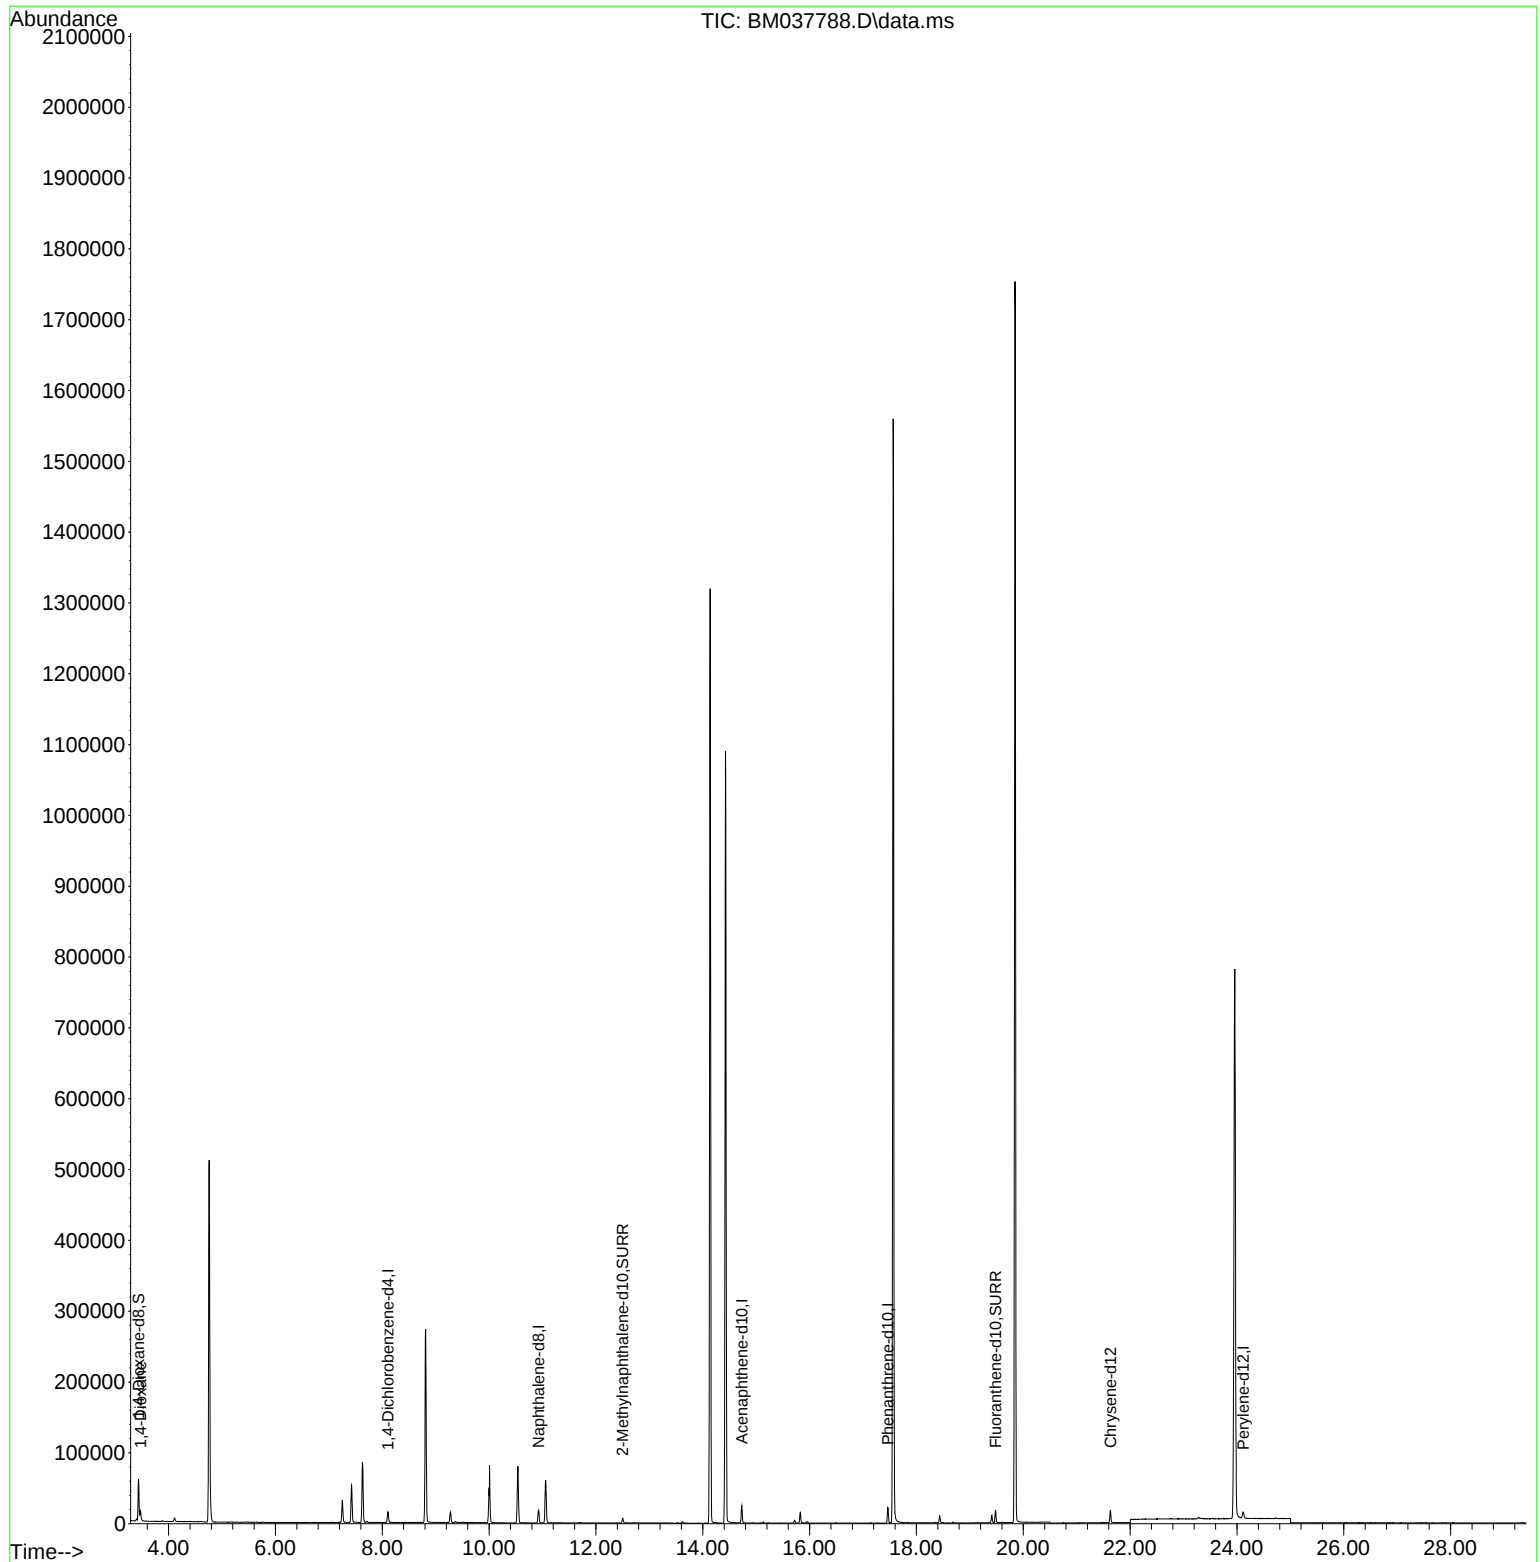

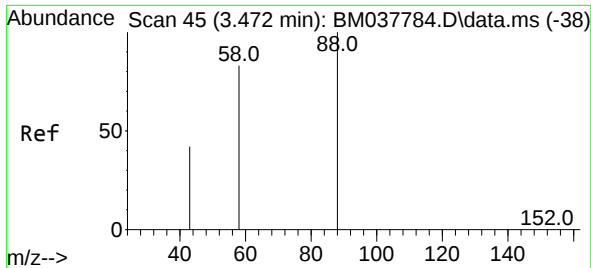

#2
 1,4-Dioxane
 Concen: 0.922 ng/ul
 RT: 3.472 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BM037788.D
 Acq: 29 Nov 2022 13:07

Instrument :
 BNA_M
 ClientSampleId :
 H0AA3

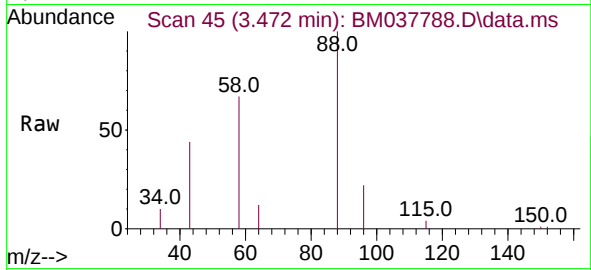

Tgt Ion:	88	Resp:	7934
Ion Ratio	Lower	Upper	
88	100		
43	44.3	102.8	154.2#
58	66.5	67.3	100.9#

