

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037790.D
 Acq On : 29 Nov 2022 14:21
 Operator : CG/JU
 Sample : N5592-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB2

Quant Time: Nov 29 23:36:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	5809	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	19063	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	10292	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.467	188	19519	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.632	240	12710	0.400	ng/ul	# 0.00
23) Perylene-d12	24.113	264	11717	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	30865	4.570	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	8172	0.259	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	15463	0.368	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.472	88	1298	0.185	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037790.D
Acq On : 29 Nov 2022 14:21
Operator : CG/JU
Sample : N5592-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB2


Quant Time: Nov 29 23:36:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration

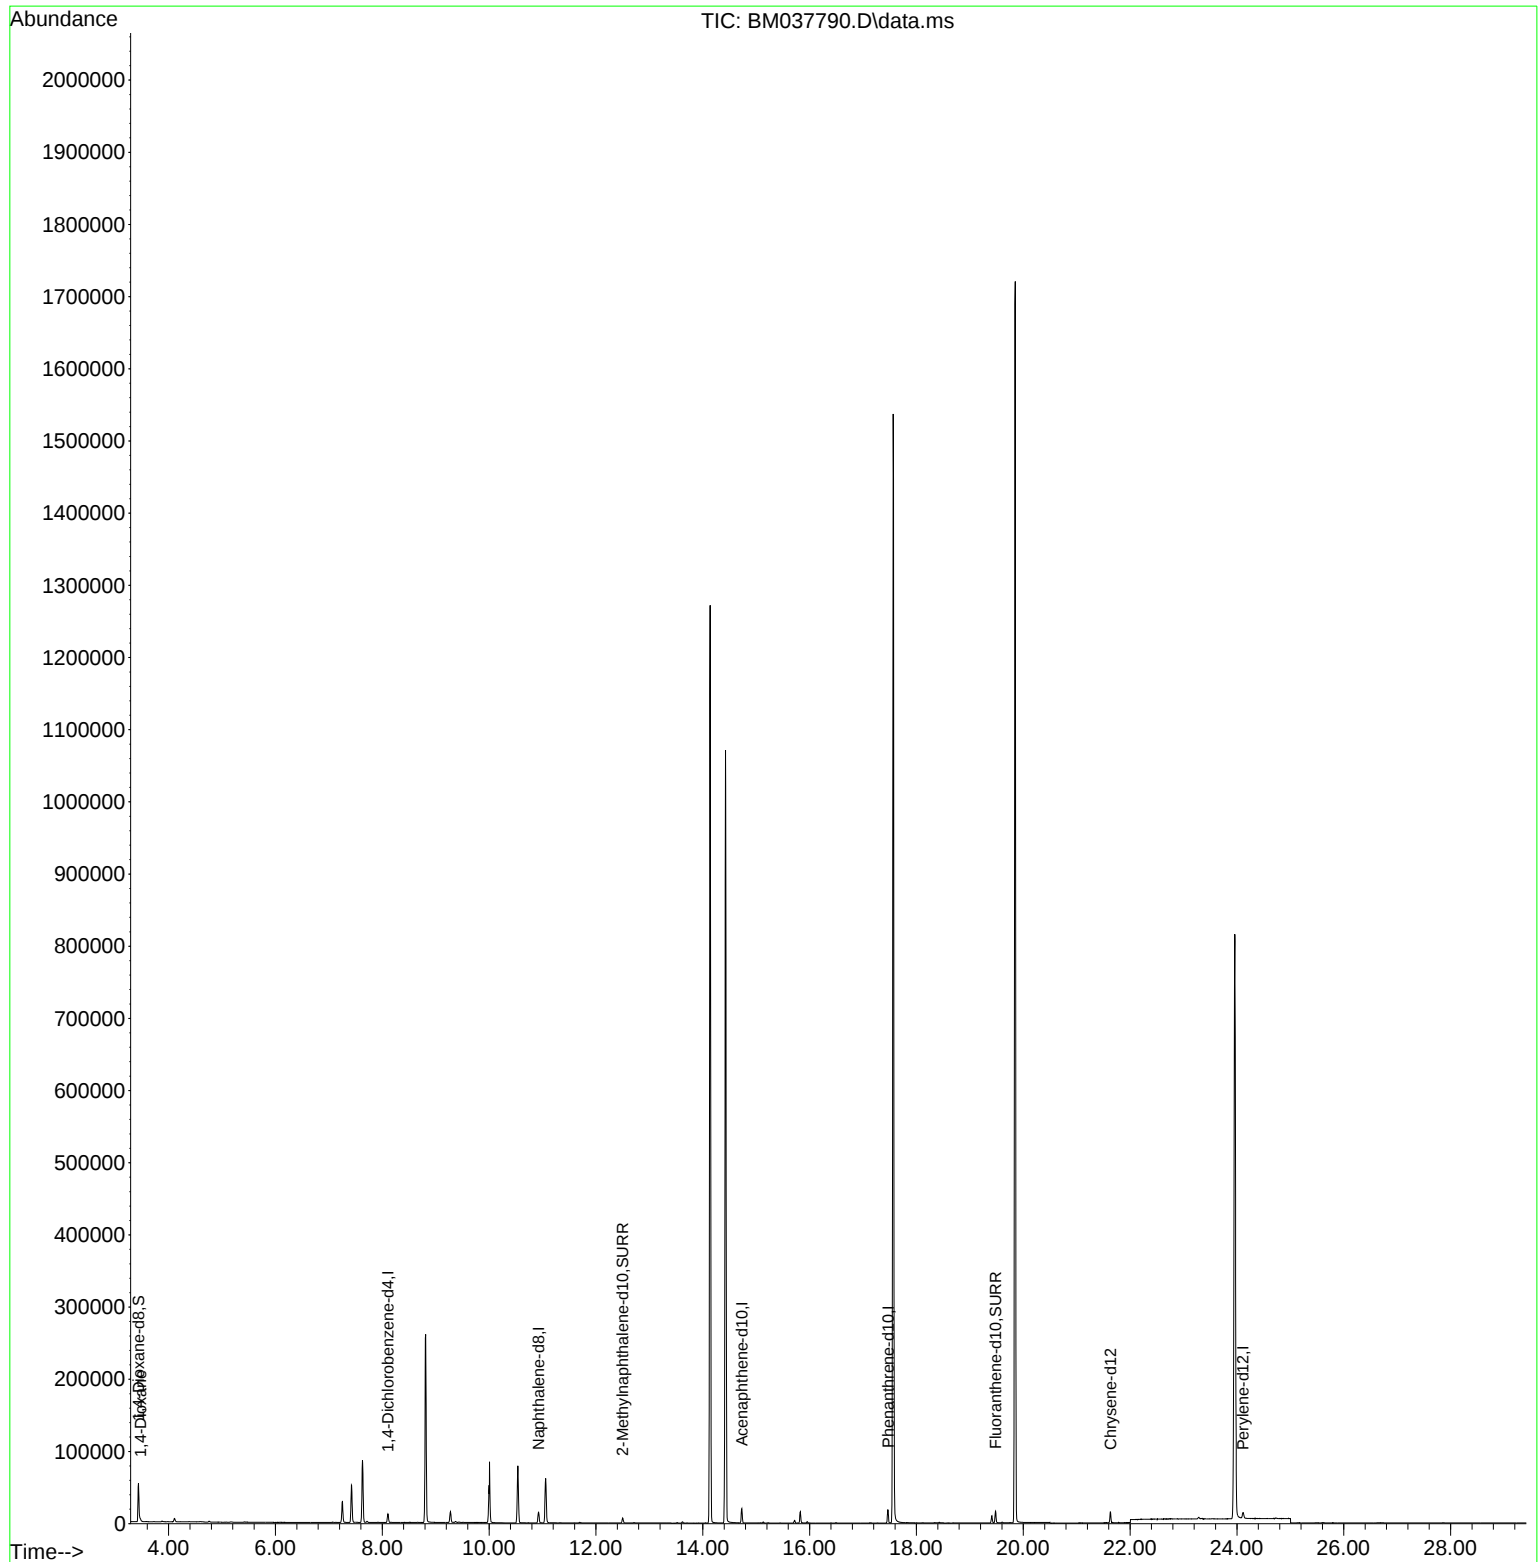

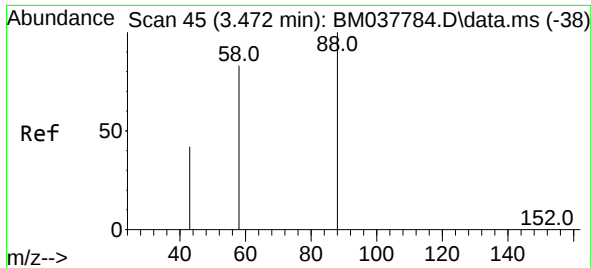

#2
 1,4-Dioxane
 Concen: 0.185 ng/ul
 RT: 3.472 min Scan# 45
 Delta R.T. 0.000 min
 Lab File: BM037790.D
 Acq: 29 Nov 2022 14:21

Instrument :
 BNA_M
 ClientSampleId :
 H0AB2

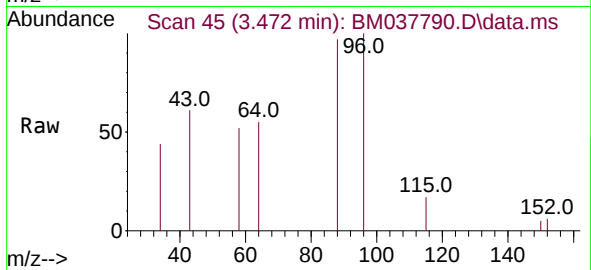

Tgt Ion: 88	Resp: 1298
Ion Ratio	Lower Upper
88 100	
43 63.1	102.8 154.2#
58 53.2	67.3 100.9#

