

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
 Data File : BM037791.D
 Acq On : 29 Nov 2022 14:58
 Operator : CG/JU
 Sample : N5592-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB3

Quant Time: Nov 29 23:36:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 23:34:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	5811	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	19284	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.730	164	10618	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.467	188	20295	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.632	240	13607	0.400	ng/ul	# 0.00
23) Perylene-d12	24.116	264	12204	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	30667	4.539	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.499	152	8034	0.251	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	18208	0.405	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.472	88	1340	0.191	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112922\
Data File : BM037791.D
Acq On : 29 Nov 2022 14:58
Operator : CG/JU
Sample : N5592-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB3


Quant Time: Nov 29 23:36:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 23:34:25 2022
Response via : Initial Calibration

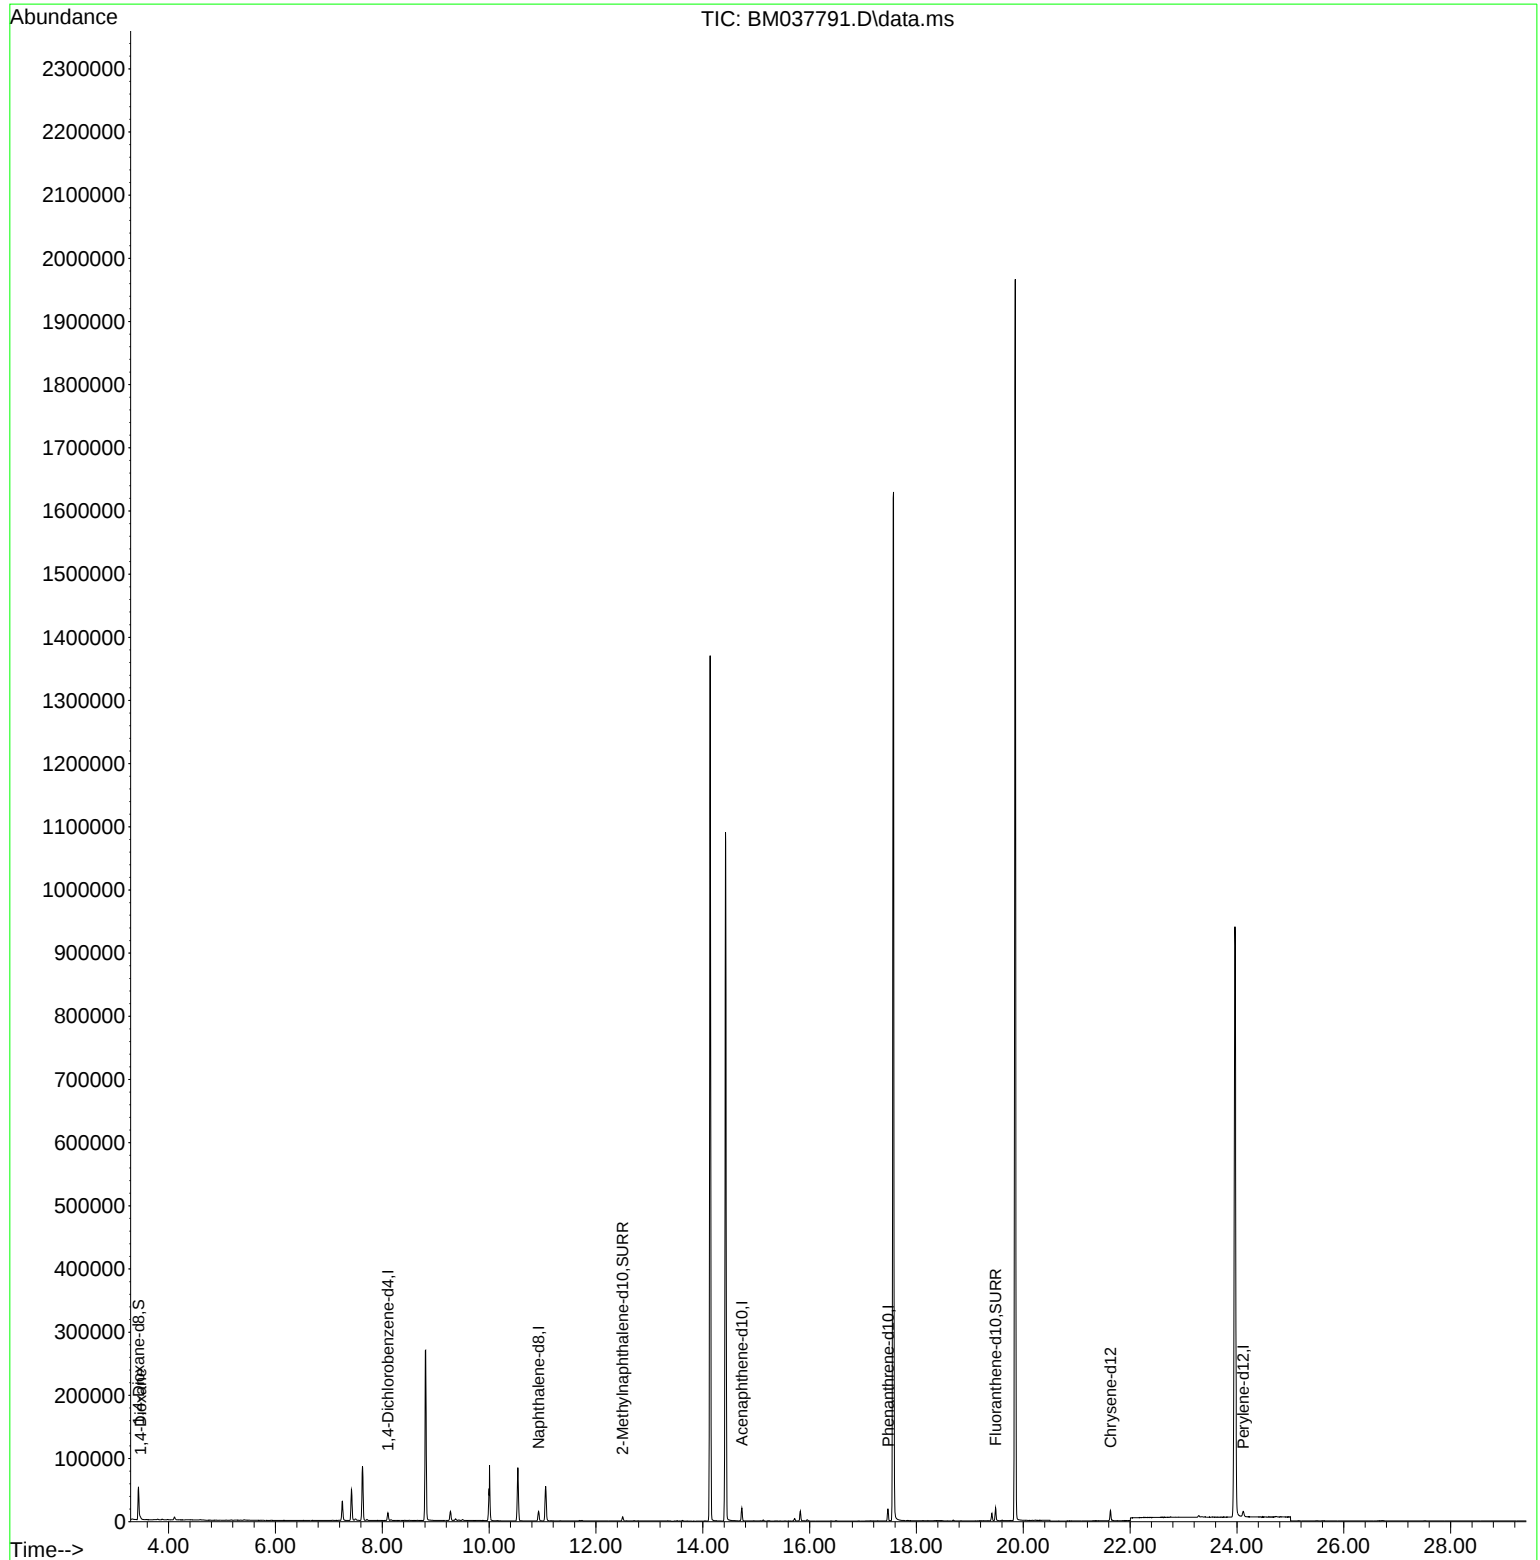

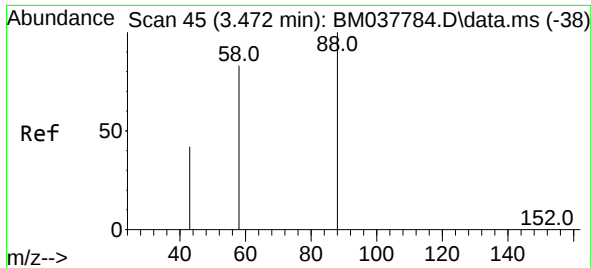

#2
 1,4-Dioxane
 Concen: 0.191 ng/ul
 RT: 3.472 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BM037791.D
 Acq: 29 Nov 2022 14:58

Instrument :
 BNA_M
 ClientSampleId :
 H0AB3

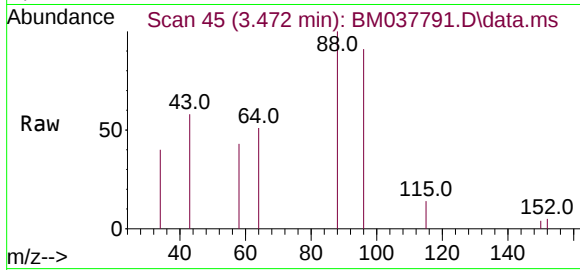

Tgt Ion:	88	Resp:	1340
Ion	Ratio	Lower	Upper
88	100		
43	58.3	102.8	154.2#
58	43.3	67.3	100.9#

