


Data Path : Z:\HPCHEM1\BNA M\Data\BM113015\
 Data File : BM003320.D
 Acq On : 30 Nov 2015 11:39
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM112715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 13:09:54 2015

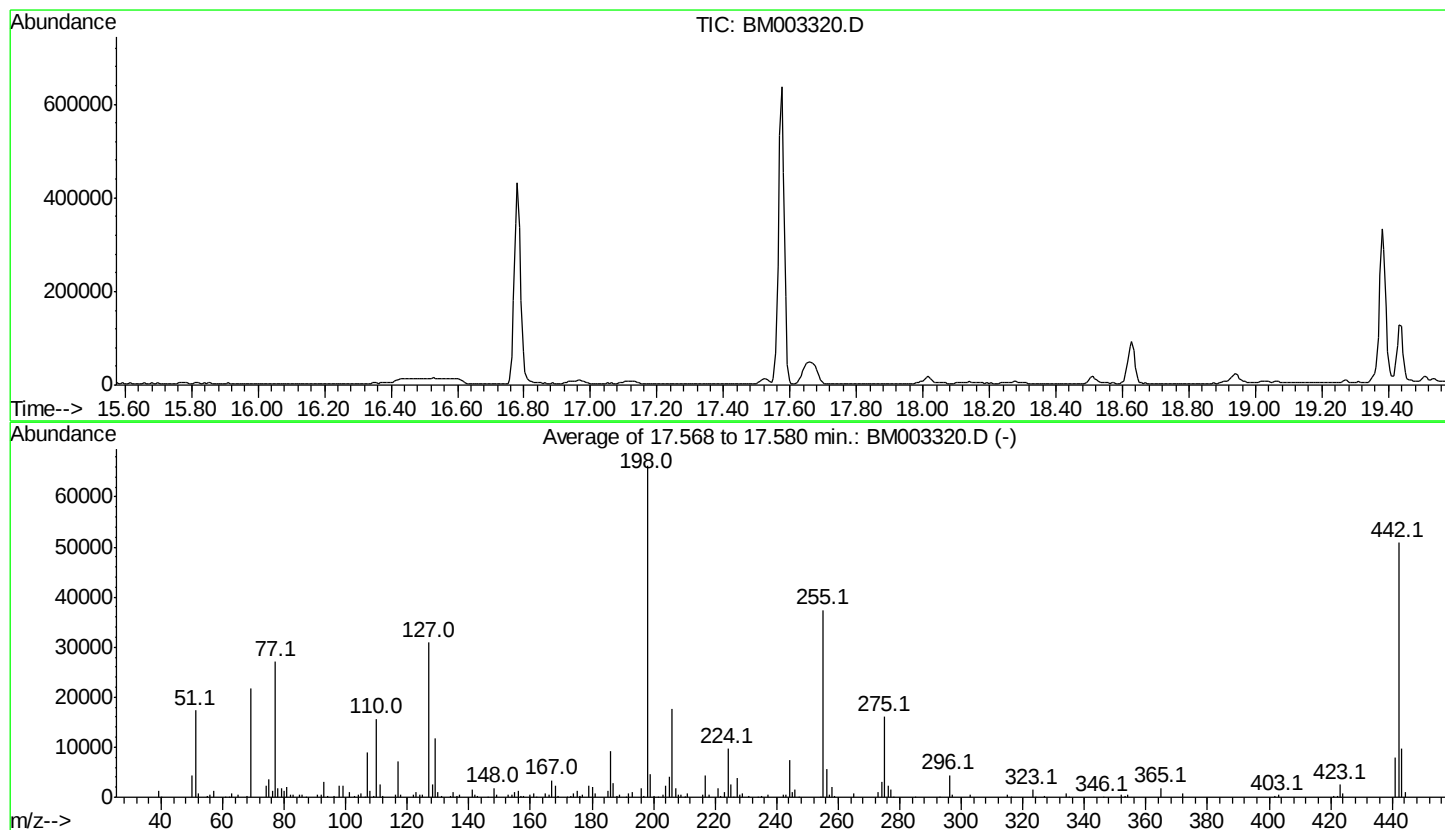

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	17289	PASS
68	69	0.00	2	1.8	389	PASS
69	198	0.00	100	33.0	21853	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	30901	PASS
197	198	0.00	2	0.6	376	PASS
198	198	100	100	100.0	66261	PASS
199	198	5	9	7.0	4612	PASS
275	198	10	60	24.2	16003	PASS
365	198	1	100	2.8	1888	PASS
441	442	0.01	24	15.5	7891	PASS
442	198	50	100	76.7	50816	PASS
443	442	15	24	19.0	9658	PASS