


Data Path : Z:\HPCHEM1\BNA M\DATA\BM113015\
 Data File : BM003327.D
 Acq On : 30 Nov 2015 20:11
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM112715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 13:09:54 2015

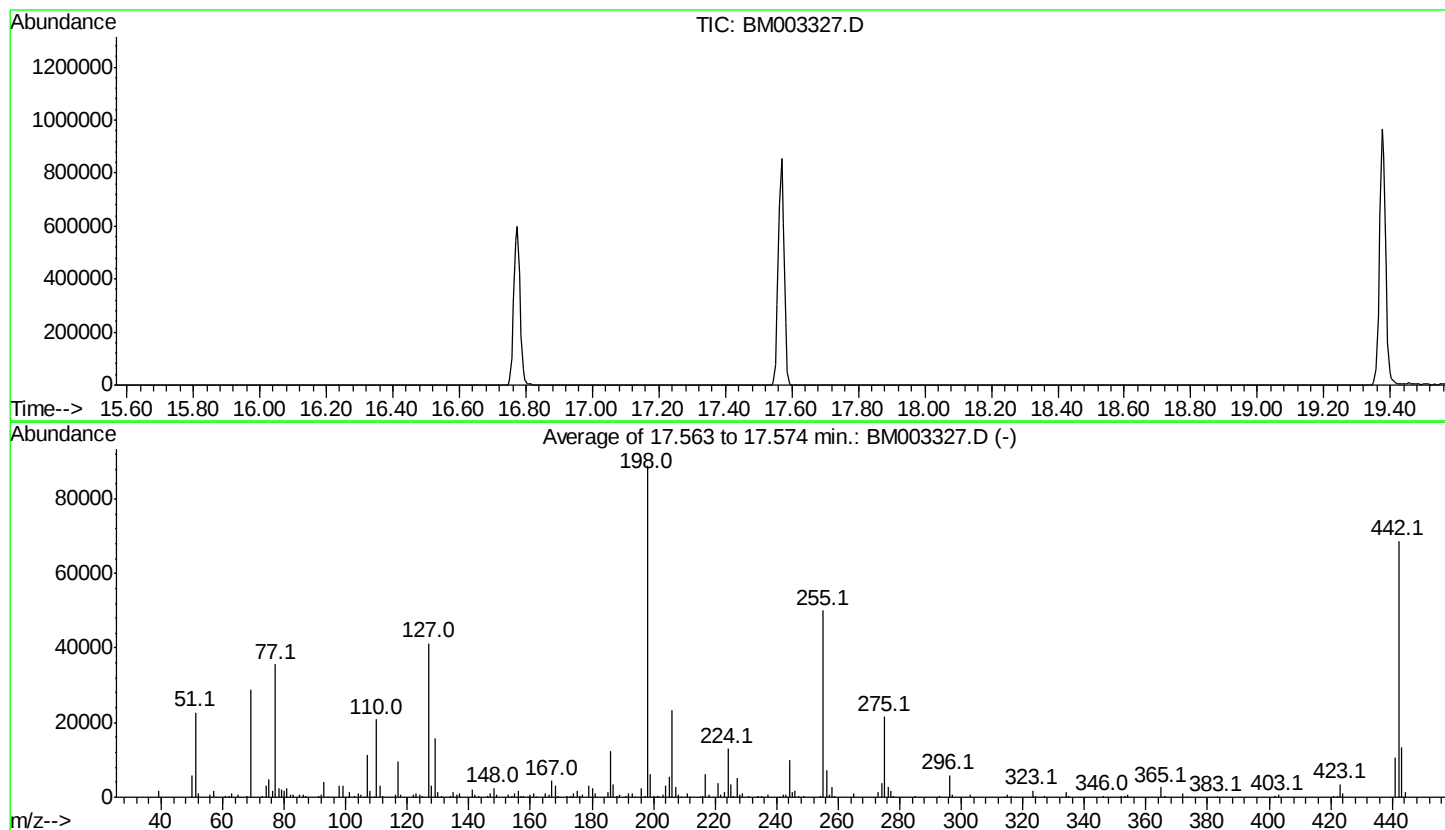

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	22752	PASS
68	69	0.00	2	1.6	450	PASS
69	198	0.00	100	32.3	28701	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	41341	PASS
197	198	0.00	2	0.4	324	PASS
198	198	100	100	100.0	88904	PASS
199	198	5	9	6.8	6044	PASS
275	198	10	60	24.2	21522	PASS
365	198	1	100	3.0	2626	PASS
441	442	0.01	24	15.7	10801	PASS
442	198	50	100	77.3	68712	PASS
443	442	15	24	19.5	13425	PASS