

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM113016\
 Data File : BM008117.D
 Acq On : 30 Nov 2016 18:00
 Operator : UM/SJ
 Sample : H5699-25
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4WF5

Quant Time: Dec 01 02:55:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 01 02:52:19 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	171588	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	710792	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	495906	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	978578	20.00	ng/ul	0.00
75) Chrysene-d12	21.28	240	1022293	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	929464	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	3714	1.07	ng/uL	0.00
5) Phenol-d5	6.89	99	72970	5.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	224431	30.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	235122	23.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	148078	14.89	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	152463	29.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	170538	29.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	275723	26.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	3380	0.33	ng/ul	0.06
43) Dimethylphthalate-d6	13.75	166	1037401	32.46	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1221309	31.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	6336	1.28	ng/ul	0.05
57) Fluorene-d10	15.33	176	884569	32.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	143424	24.68	ng/ul	0.00
70) Anthracene-d10	17.19	188	1319208	31.34	ng/ul	0.00
76) Pyrene-d10	19.49	212	1456093	35.19	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	1239490	32.01	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.76	165	6487	1.04 ng/ul#	36




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM113016\
Data File : BM008117.D
Acq On : 30 Nov 2016 18:00
Operator : UM/SJ
Sample : H5699-25
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4WF5

Quant Time: Dec 01 02:55:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM112916.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 01 02:52:19 2016
Response via : Initial Calibration

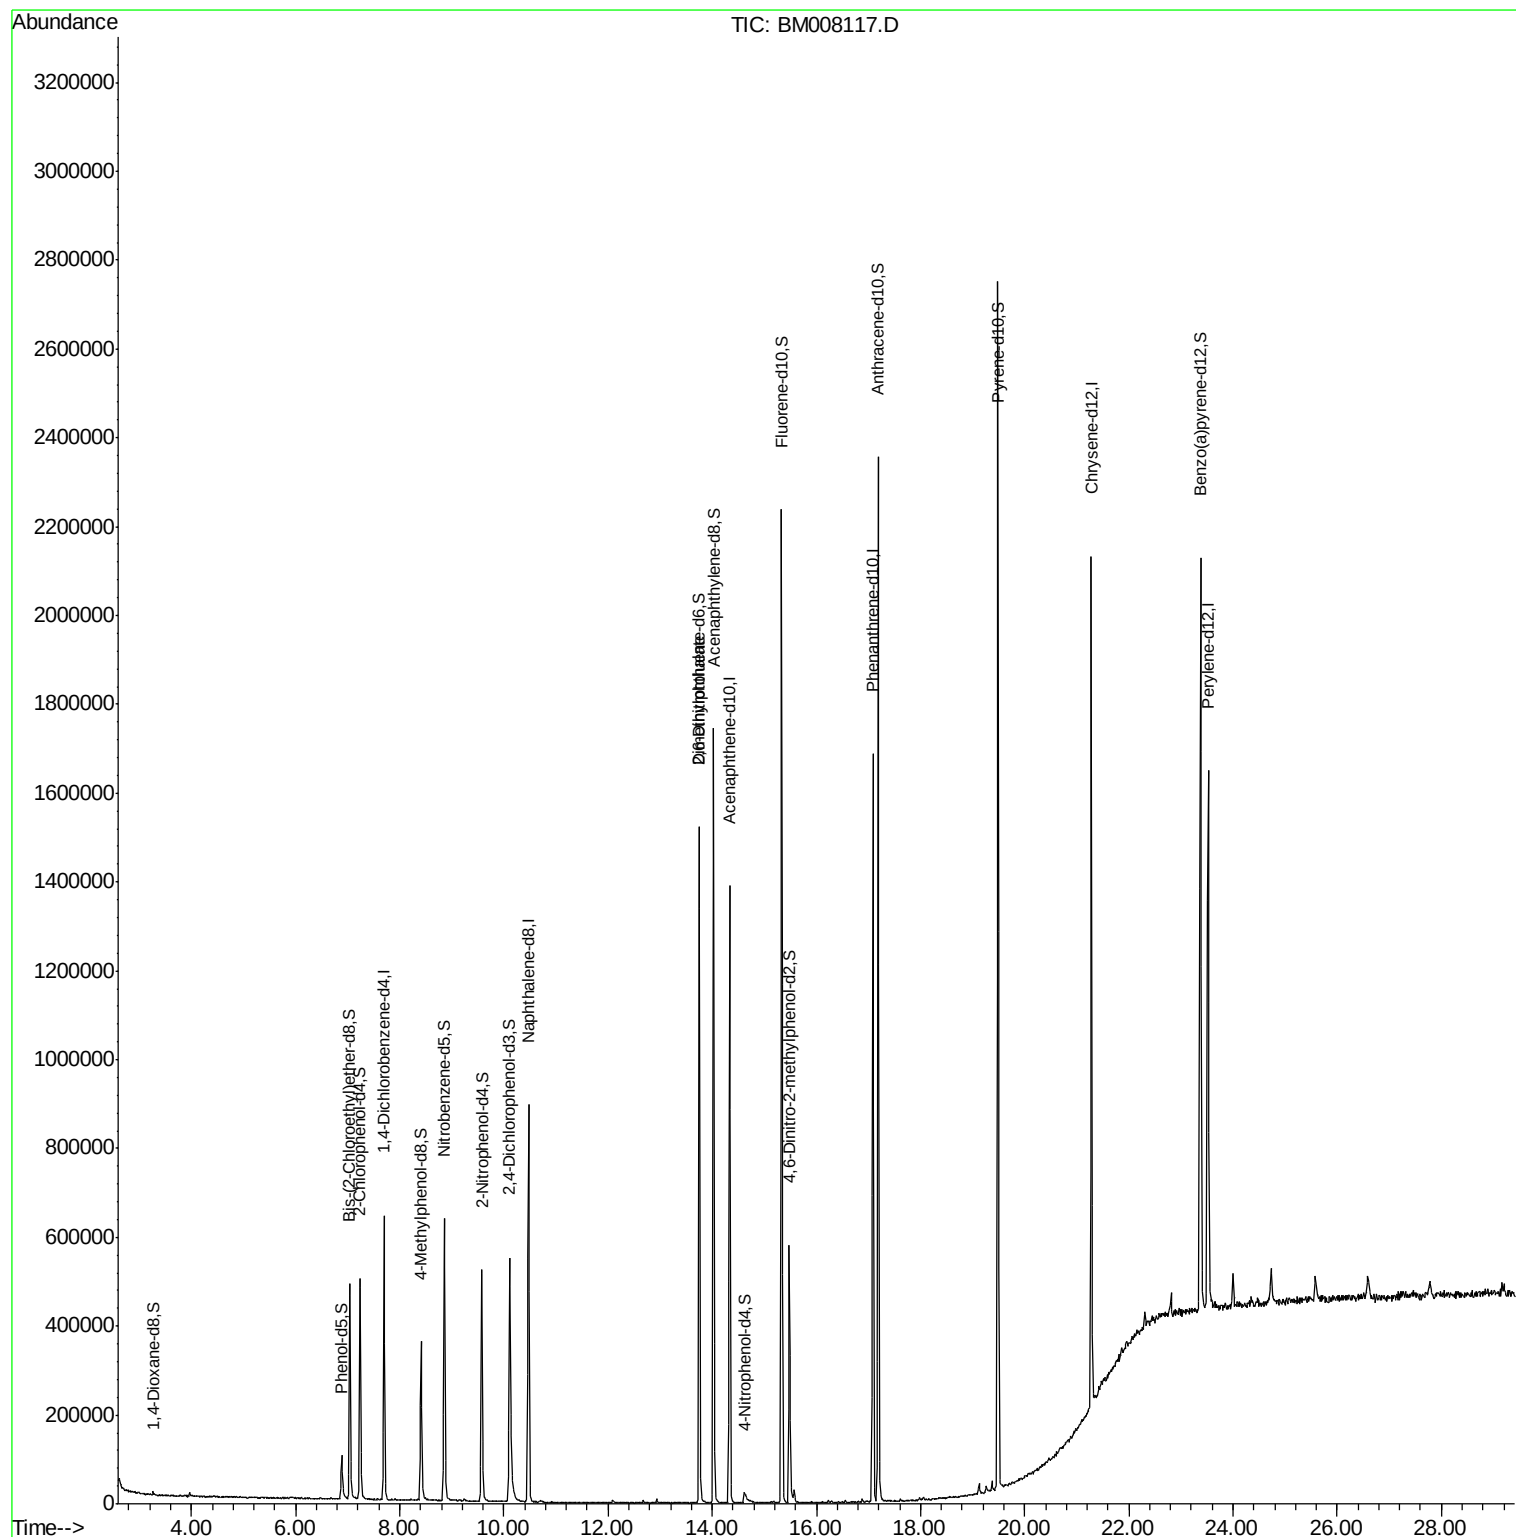

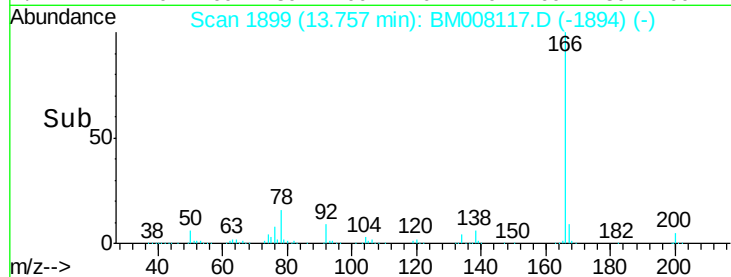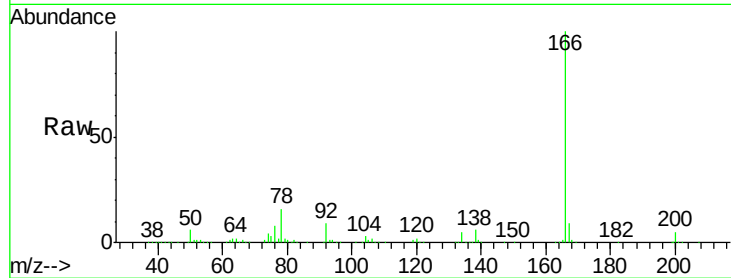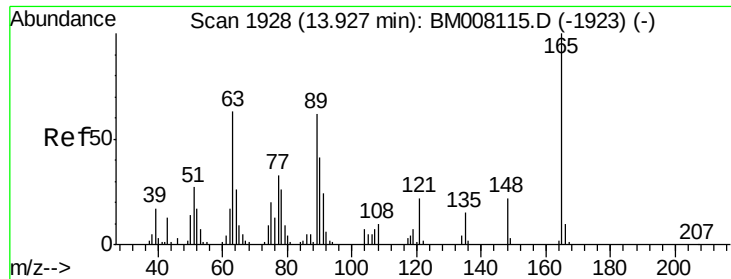

#45

2,6-Dinitrotoluene

Concen: 1.04 ng/ul

RT: 13.76 min Scan# 1899

Delta R.T. -0.17 min

Lab File: BM008117.D

Acq: 30 Nov 2016 18:00

Instrument :

BNA_M

ClientSampleId :

A4WF5

Tgt Ion:165 Resp: 6487

Ion Ratio Lower Upper

165 100

89 0.0 50.6 76.0#

121 29.8 18.2 27.2#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

