
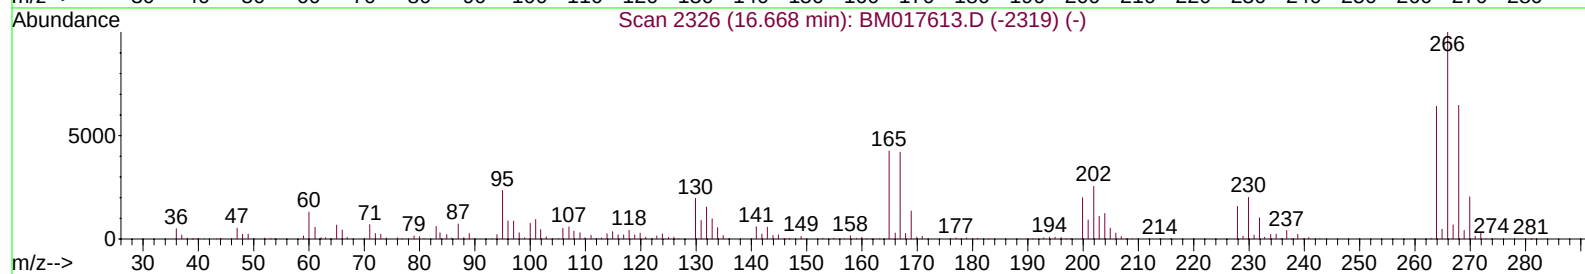
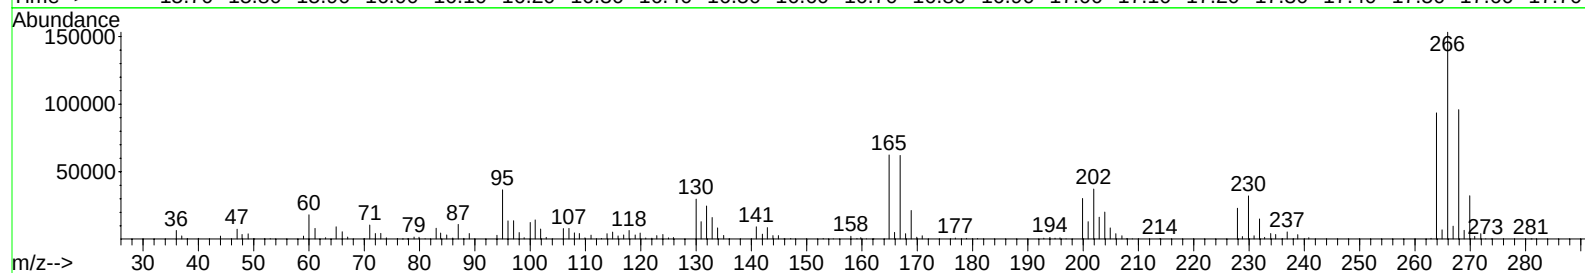


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM113018\
Data File : BM017815.D
Acq On : 30 Nov 2018 09:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 10:50:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

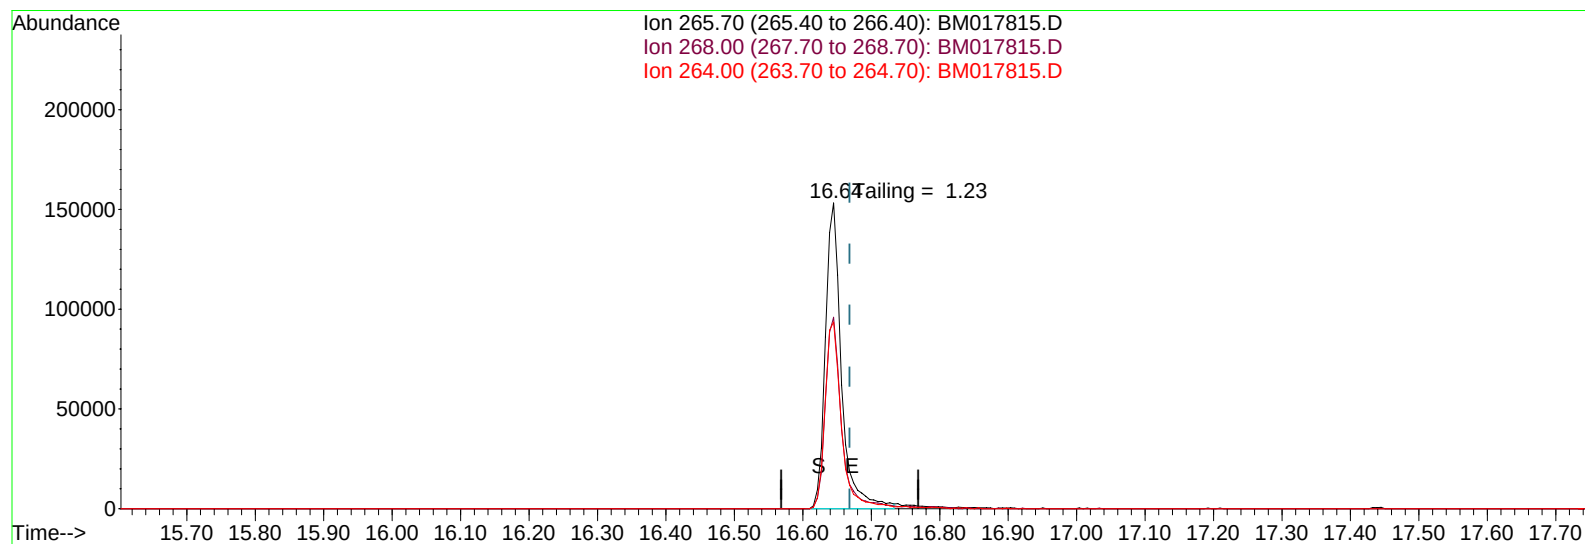

TIC: BM017815.D

(70) Pentachlorophenol (C)




16.645min (-0.024) 0.00ng

response 251905

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	62.65
264.00	64.10	61.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM113018\
Data File : BM017815.D
Acq On : 30 Nov 2018 09:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 10:50:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

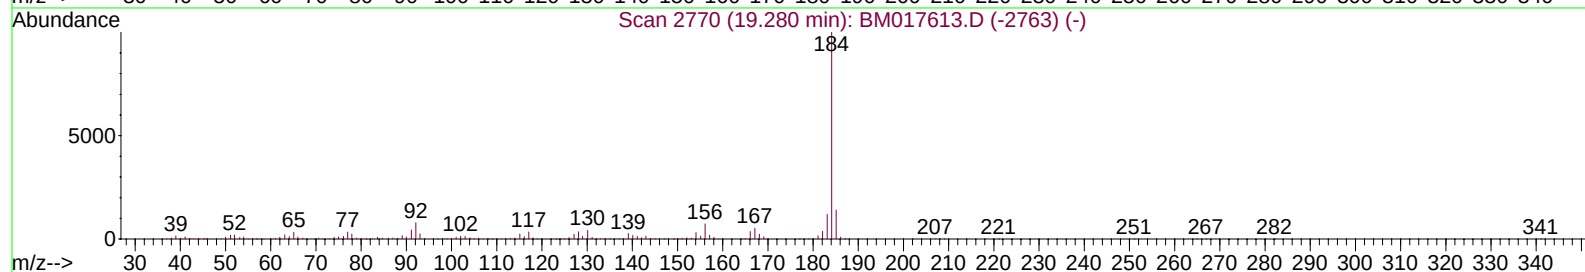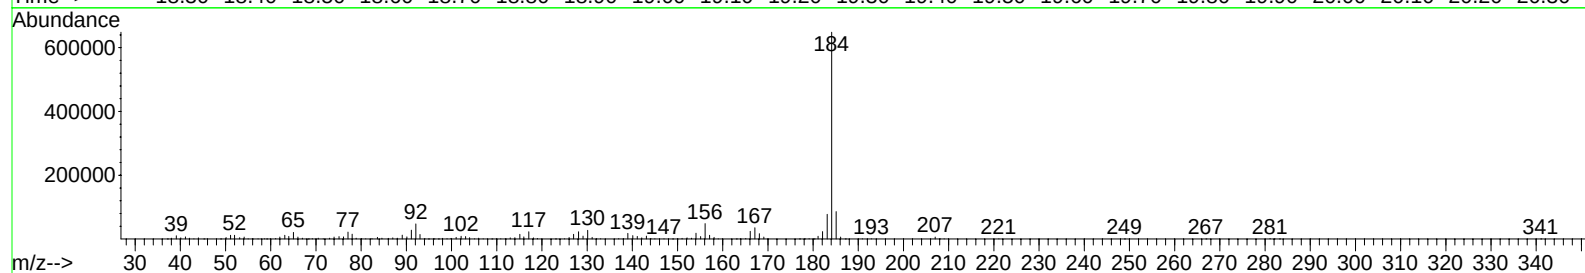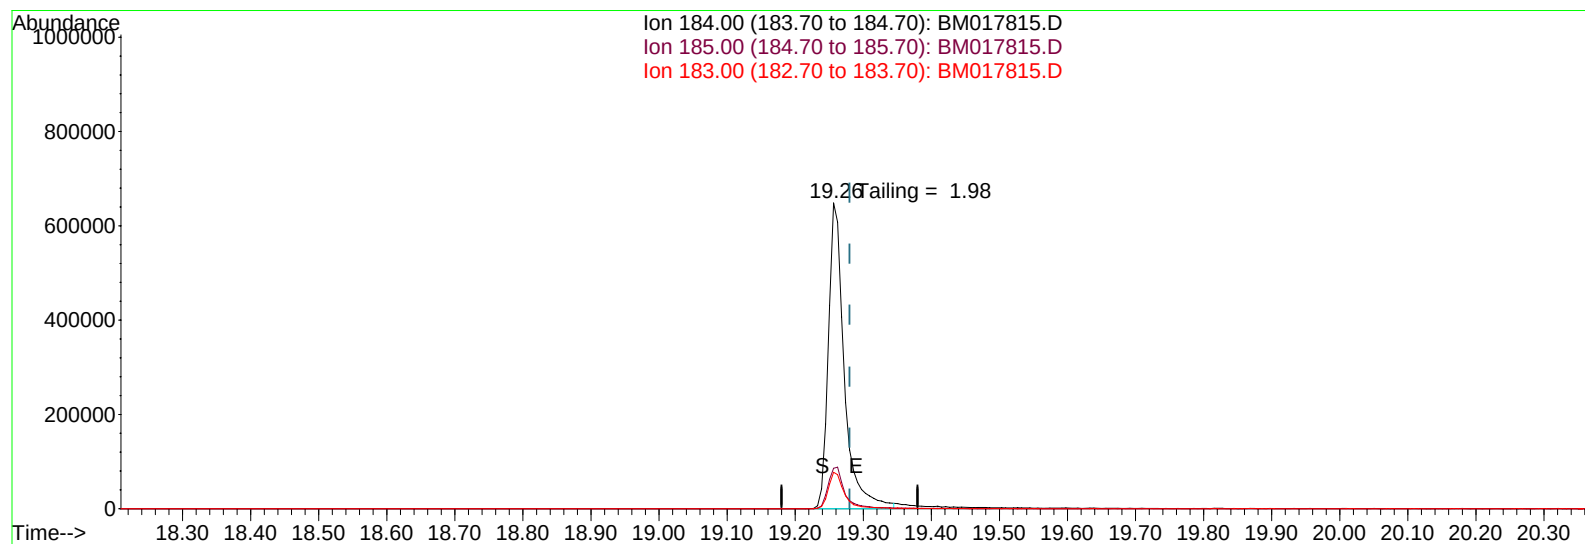

TIC: BM017815.D

(77) Benzidine

19.256min (-0.024) 48293.25ng

response 1069380

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.25
183.00	11.90	11.93
0.00	0.00	0.00