


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM113018\
 Data File : BM017815.D
 Acq On : 30 Nov 2018 09:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

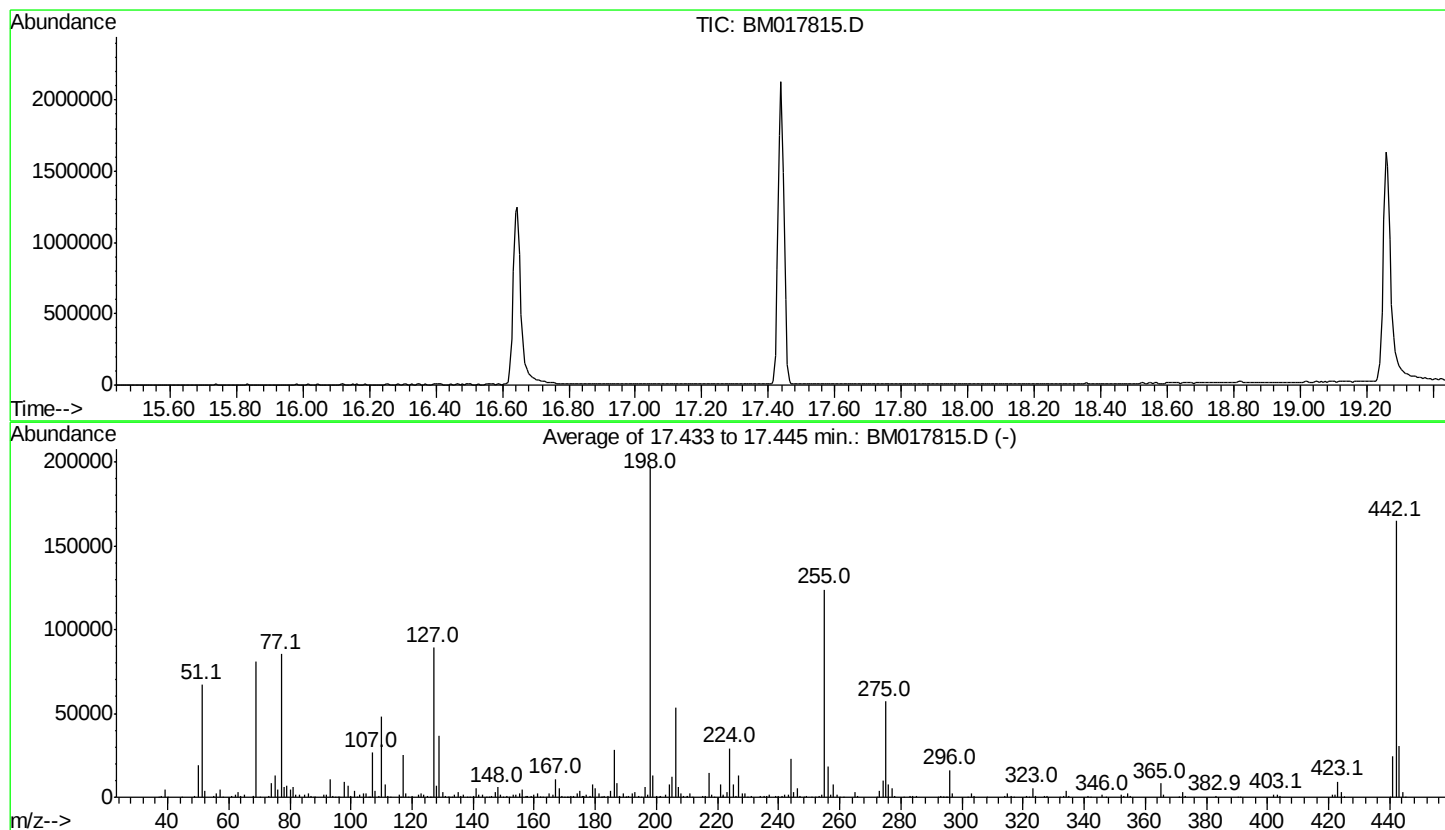

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	67069	PASS
68	69	0.00	2	1.1	859	PASS
69	198	0.00	100	40.9	80840	PASS
70	69	0.00	2	0.5	399	PASS
127	198	10	80	45.0	89104	PASS
197	198	0.00	2	0.6	1279	PASS
198	198	100	100	100.0	197802	PASS
199	198	5	9	6.8	13381	PASS
275	198	10	60	28.9	57109	PASS
365	198	1	100	4.2	8286	PASS
441	198	0.01	100	12.5	24730	PASS
442	198	50	100	83.4	164906	PASS
443	442	15	24	18.4	30416	PASS