

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043086.D
 Acq On : 30 Nov 2023 15:50
 Operator : MA/JU
 Sample : PB157421BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK421

Quant Time: Dec 01 00:43:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 00:42:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	840	0.400	ng/ul	#-0.06
4) Naphthalene-d8	10.601	136	2485	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.451	164	1368	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.302	188	172679	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.423	240	1589	0.400	ng/ul	0.01
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.76
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	4834	3.751	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	689	0.207	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	1534	0.265	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.441	166	302	0.056	ng/ul#	27
20) Pyrene	19.601	202	369	0.039	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043086.D
Acq On : 30 Nov 2023 15:50
Operator : MA/JU
Sample : PB157421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK421

Quant Time: Dec 01 00:43:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 00:42:42 2023
Response via : Initial Calibration




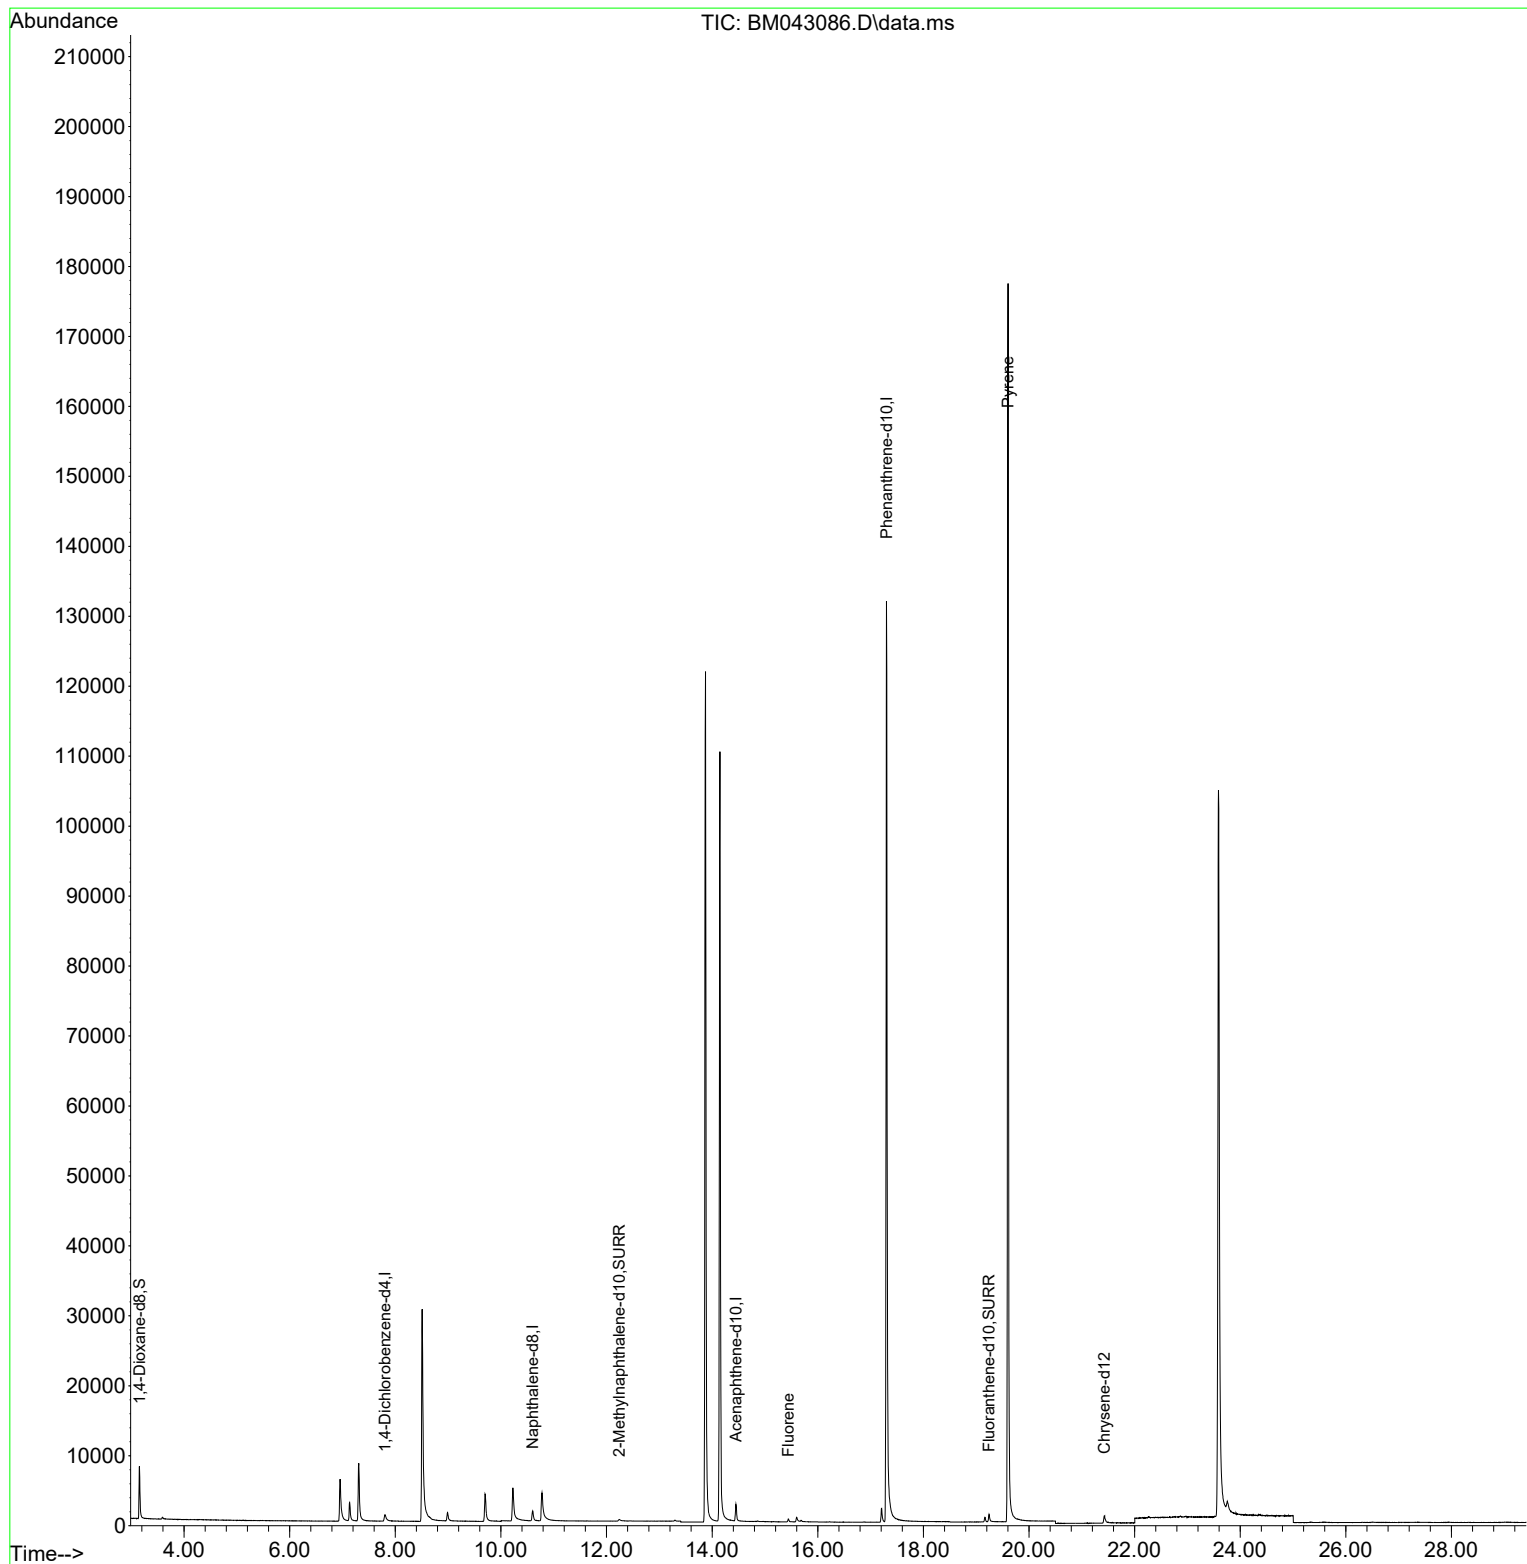


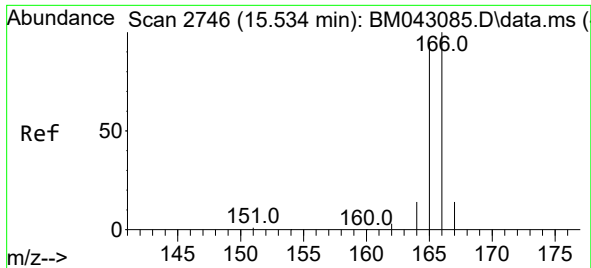

#12
 Fluorene
 Concen: 0.056 ng/ul
 RT: 15.441 min Scan# 21
 Delta R.T. -0.093 min
 Lab File: BM043086.D
 Acq: 30 Nov 2023 15:50

Instrument :
 BNA_M
 ClientSampleId :
 SBLK421

Tgt Ion:166 Resp: 302
 Ion Ratio Lower Upper
 166 100
 165 23.8 79.9 119.9#
 167 43.7 14.2 21.4#

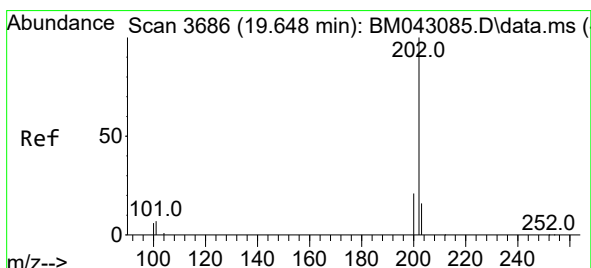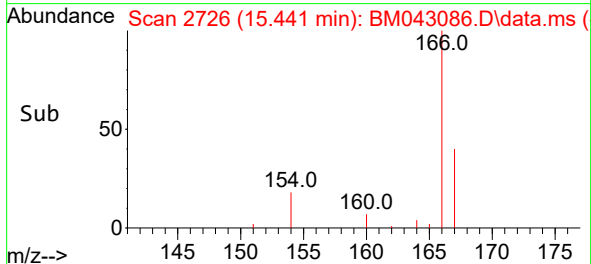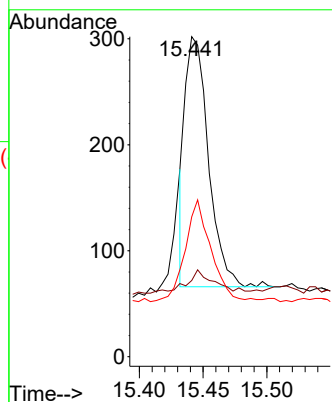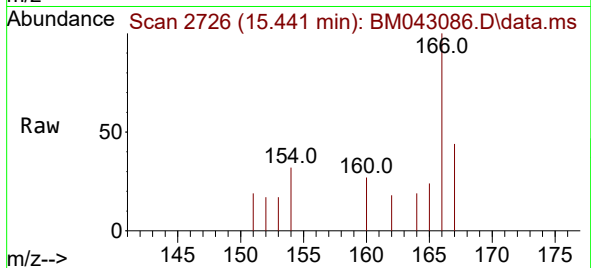

#20
 Pyrene
 Concen: 0.039 ng/ul
 RT: 19.601 min Scan# 3676
 Delta R.T. -0.047 min
 Lab File: BM043086.D
 Acq: 30 Nov 2023 15:50

Tgt Ion:202 Resp: 369
 Ion Ratio Lower Upper
 202 100
 101 181.8 8.7 13.1#
 100 1334.1 7.8 11.8#

