

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043087.D
 Acq On : 30 Nov 2023 16:26
 Operator : MA/JU
 Sample : PB157409BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK409

Quant Time: Dec 01 00:43:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 00:42:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	902	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.601	136	2738	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.451	164	1537	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.302	188	249814	0.400	ng/ul	# 0.07
17) Chrysene-d12	21.420	240	1792	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.76
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	6058	4.377	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	908	0.248	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	2136	0.327	ng/ul	0.00
Target Compounds						
20) Pyrene	19.602	202	514	0.048	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043087.D
Acq On : 30 Nov 2023 16:26
Operator : MA/JU
Sample : PB157409BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK409

Quant Time: Dec 01 00:43:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 00:42:42 2023
Response via : Initial Calibration

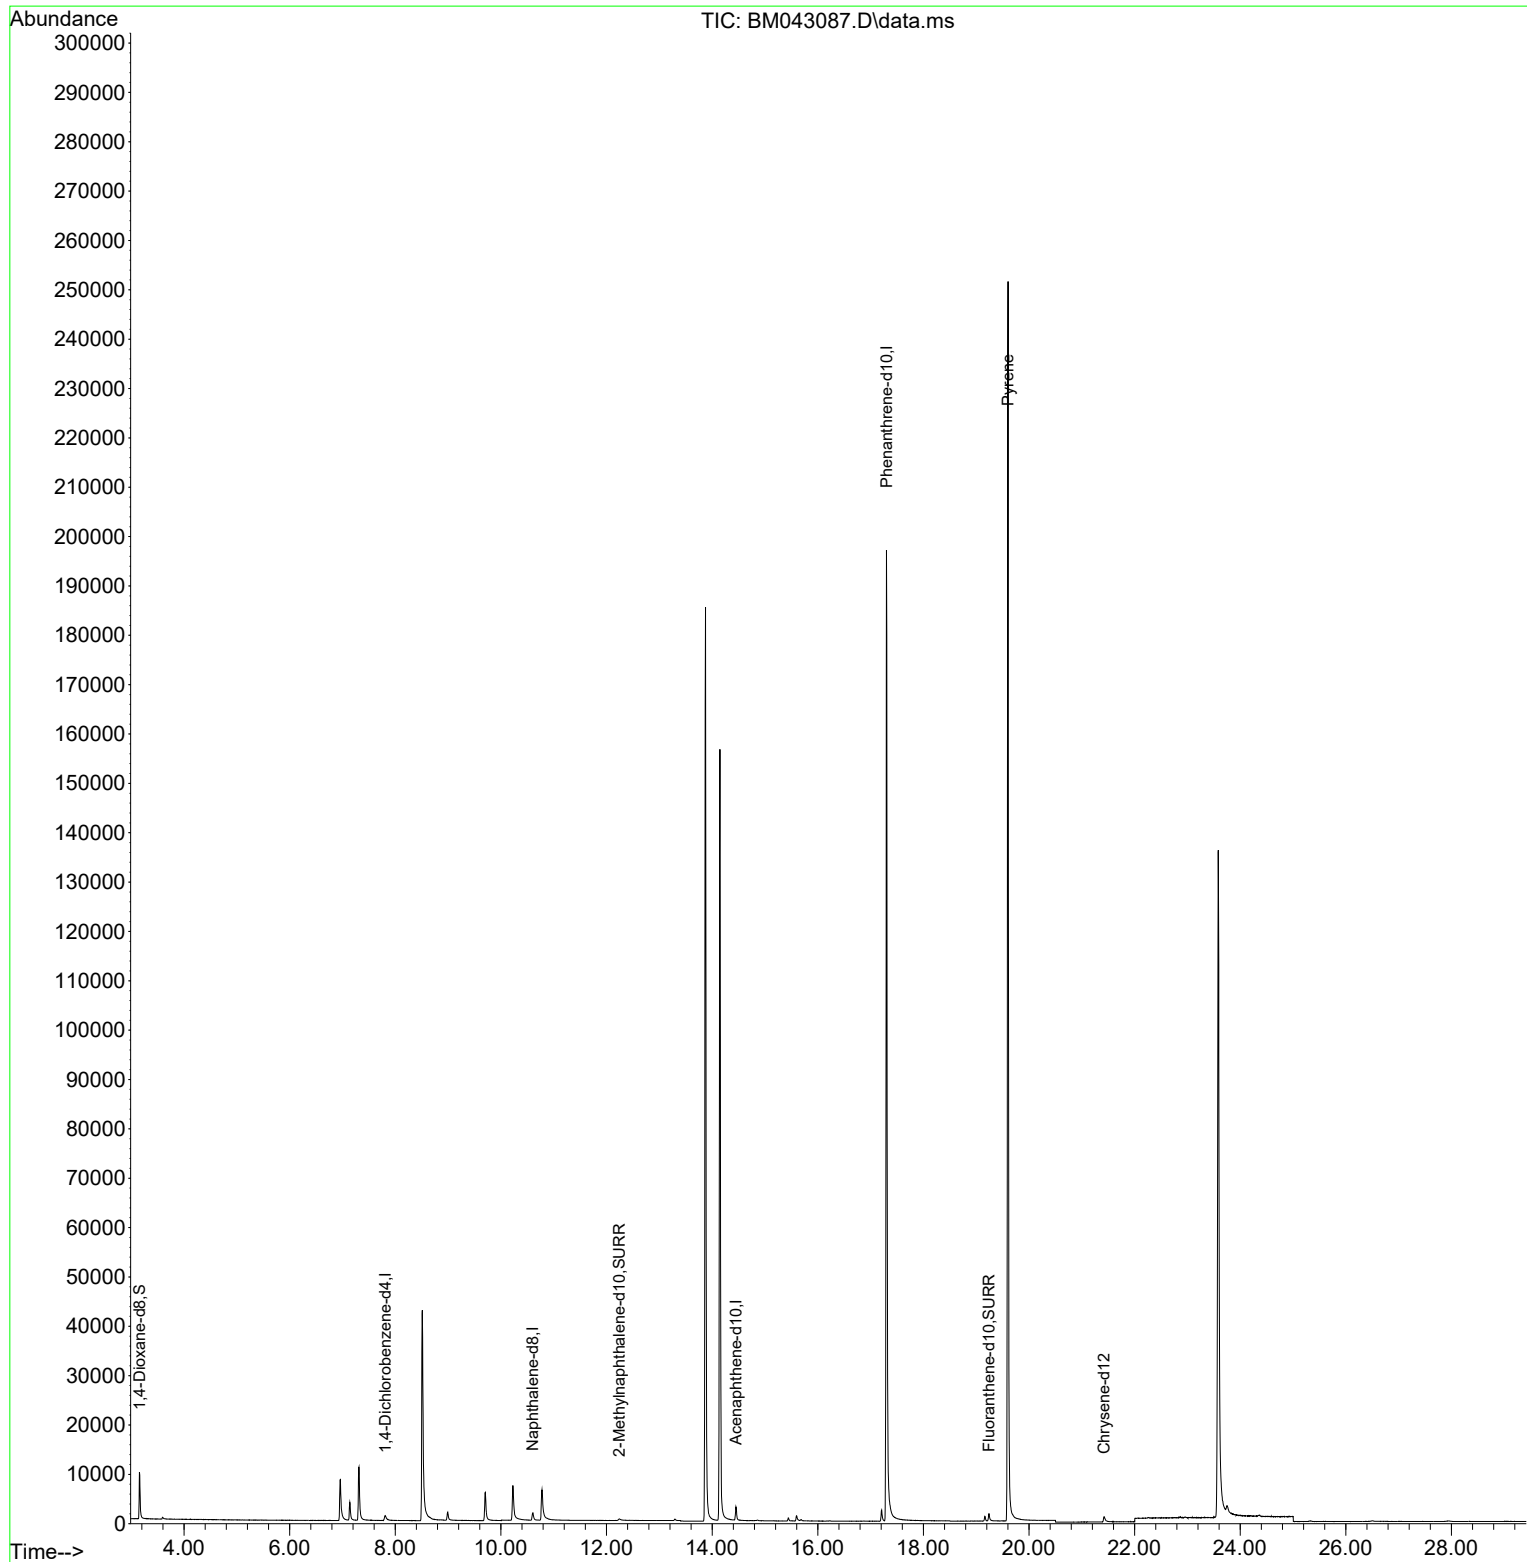

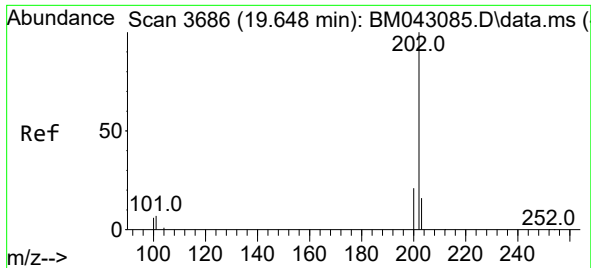

#20

Pyrene

Concen: 0.048 ng/ul

RT: 19.602 min Scan# 30

Delta R.T. -0.046 min

Lab File: BM043087.D


Acq: 30 Nov 2023 16:26

Instrument :

BNA_M

ClientSampleId :

SBLK409

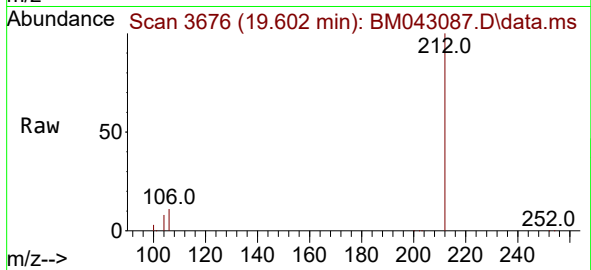

Tgt Ion:202 Resp: 514

Ion	Ratio	Lower	Upper
202	100		
101	173.5	8.7	13.1#
100	1332.7	7.8	11.8#

