

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043127.D
 Acq On : 01 Dec 2023 17:56
 Operator : MA/JU
 Sample : 05439-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Quant Time: Dec 02 00:07:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 00:03:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	958	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.595	136	2766	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.442	164	1498	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.297	188	263255	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.40
23) Perylene-d12	23.741	264	5672	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	4689	3.190	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.218	152	1047	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.234	212	2466	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.197	88	88	0.056	ng/ul#	86
5) Naphthalene	10.650	128	312	0.042	ng/ul#	63
26) Benzo(a)pyrene	23.577	252	1405	0.067	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043127.D
Acq On : 01 Dec 2023 17:56
Operator : MA/JU
Sample : 05439-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Time: Dec 02 00:07:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 00:03:38 2023
Response via : Initial Calibration




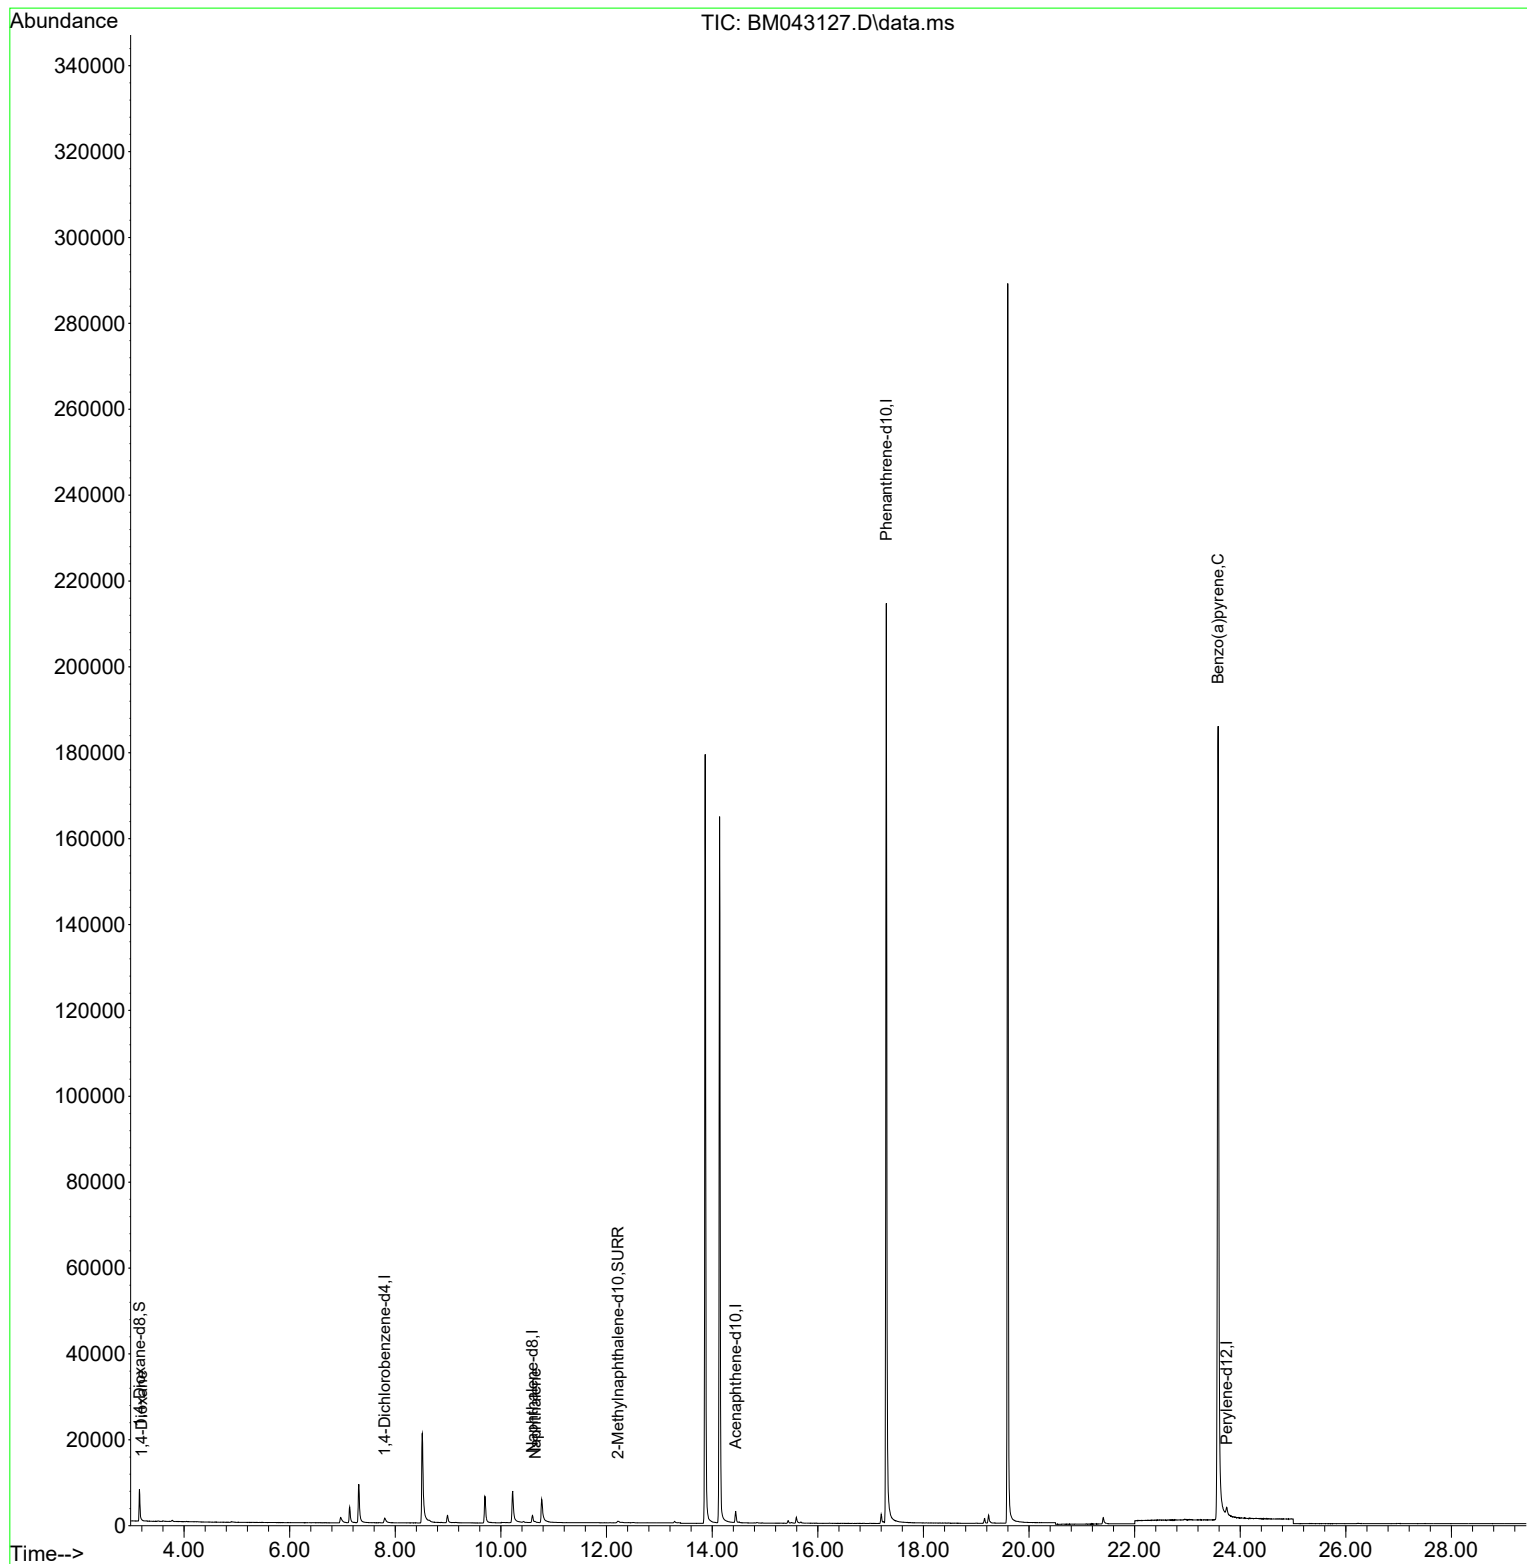


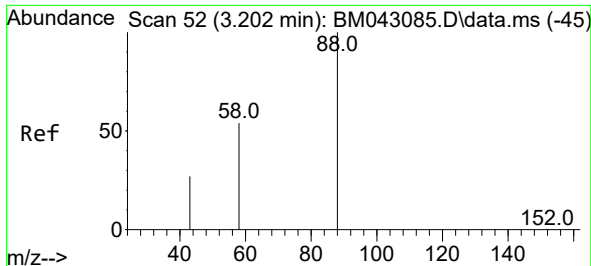

#2
1,4-Dioxane
Concen: 0.056 ng/ul
RT: 3.197 min Scan# 51
Delta R.T. -0.000 min
Lab File: BM043127.D
Acq: 01 Dec 2023 17:56




Instrument :
BNA_M
ClientSampleId :
C0AE1


Tgt Ion: 88 Resp: 88
Ion Ratio Lower Upper
88 100
43 29.1 22.8 34.2
58 19.4 26.8 40.2#

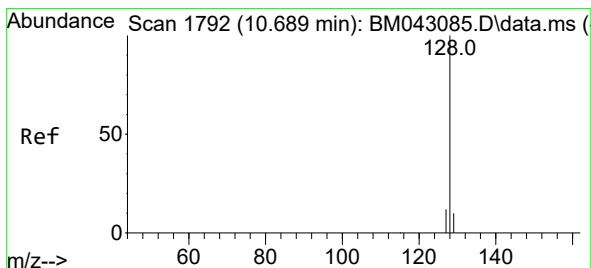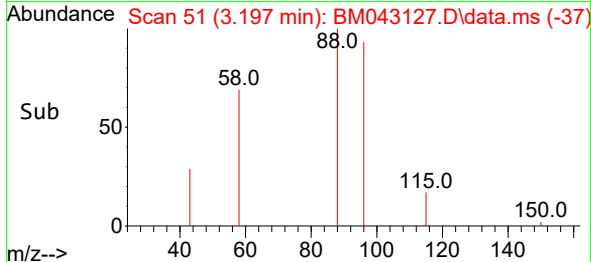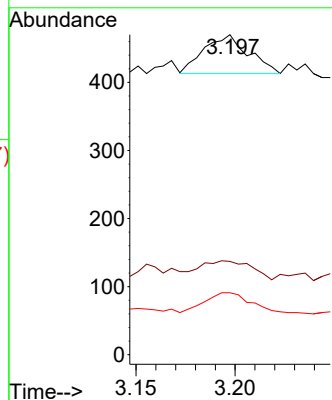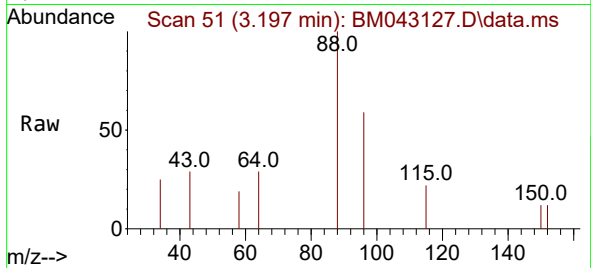

#5
Naphthalene
Concen: 0.042 ng/ul
RT: 10.650 min Scan# 1785
Delta R.T. -0.017 min
Lab File: BM043127.D
Acq: 01 Dec 2023 17:56


Tgt Ion: 128 Resp: 312
Ion Ratio Lower Upper
128 100
129 39.2 16.0 24.0#
127 35.7 16.5 24.7#

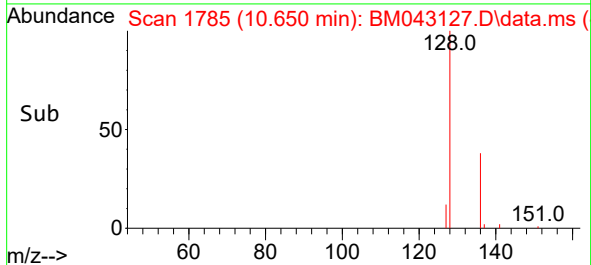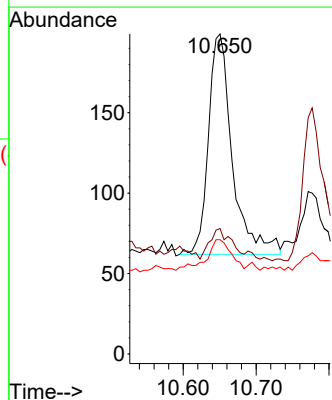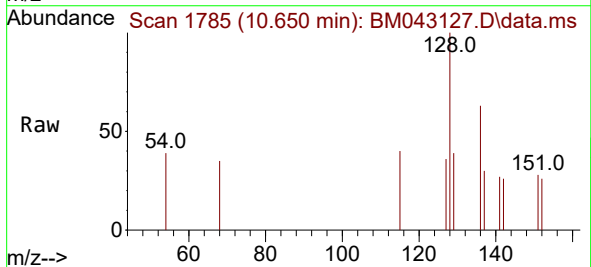

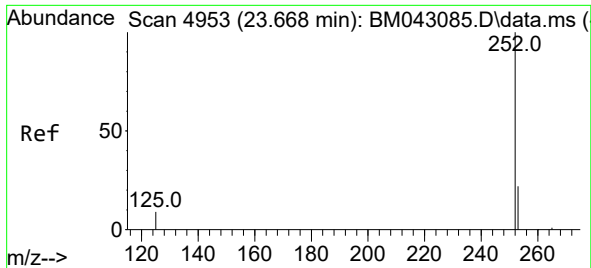

#26
Benzo(a)pyrene
Concen: 0.067 ng/ul
RT: 23.577 min Scan# 49
Delta R.T. -0.073 min
Lab File: BM043127.D
Acq: 01 Dec 2023 17:56

Instrument :
BNA_M
ClientSampleId :
C0AE1

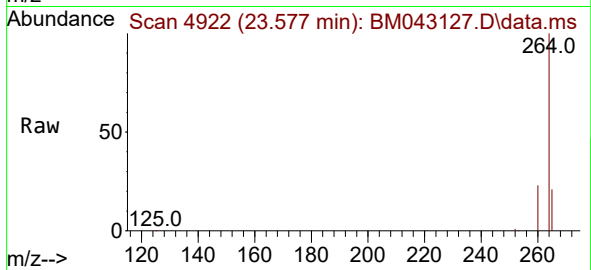

Tgt Ion:252 Resp: 1405
Ion Ratio Lower Upper
252 100
253 60.8 36.6 55.0#
125 38.1 16.2 24.4#

