

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043130.D
 Acq On : 01 Dec 2023 19:45
 Operator : MA/JU
 Sample : 05439-22
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAM0

Quant Time: Dec 02 00:07:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 00:03:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	992	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.595	136	2989	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.446	164	1643	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.297	188	289022	0.400	ng/ul	# 0.08
17) Chrysene-d12	21.414	240	1433	0.400	ng/ul	0.01
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.75
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	4139	2.719	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1126	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.234	212	2490	0.477	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.172	88	40	0.024	ng/ul#	81
20) Pyrene	19.597	202	628	0.073	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043130.D
Acq On : 01 Dec 2023 19:45
Operator : MA/JU
Sample : 05439-22
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COAM0

Quant Time: Dec 02 00:07:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 00:03:38 2023
Response via : Initial Calibration




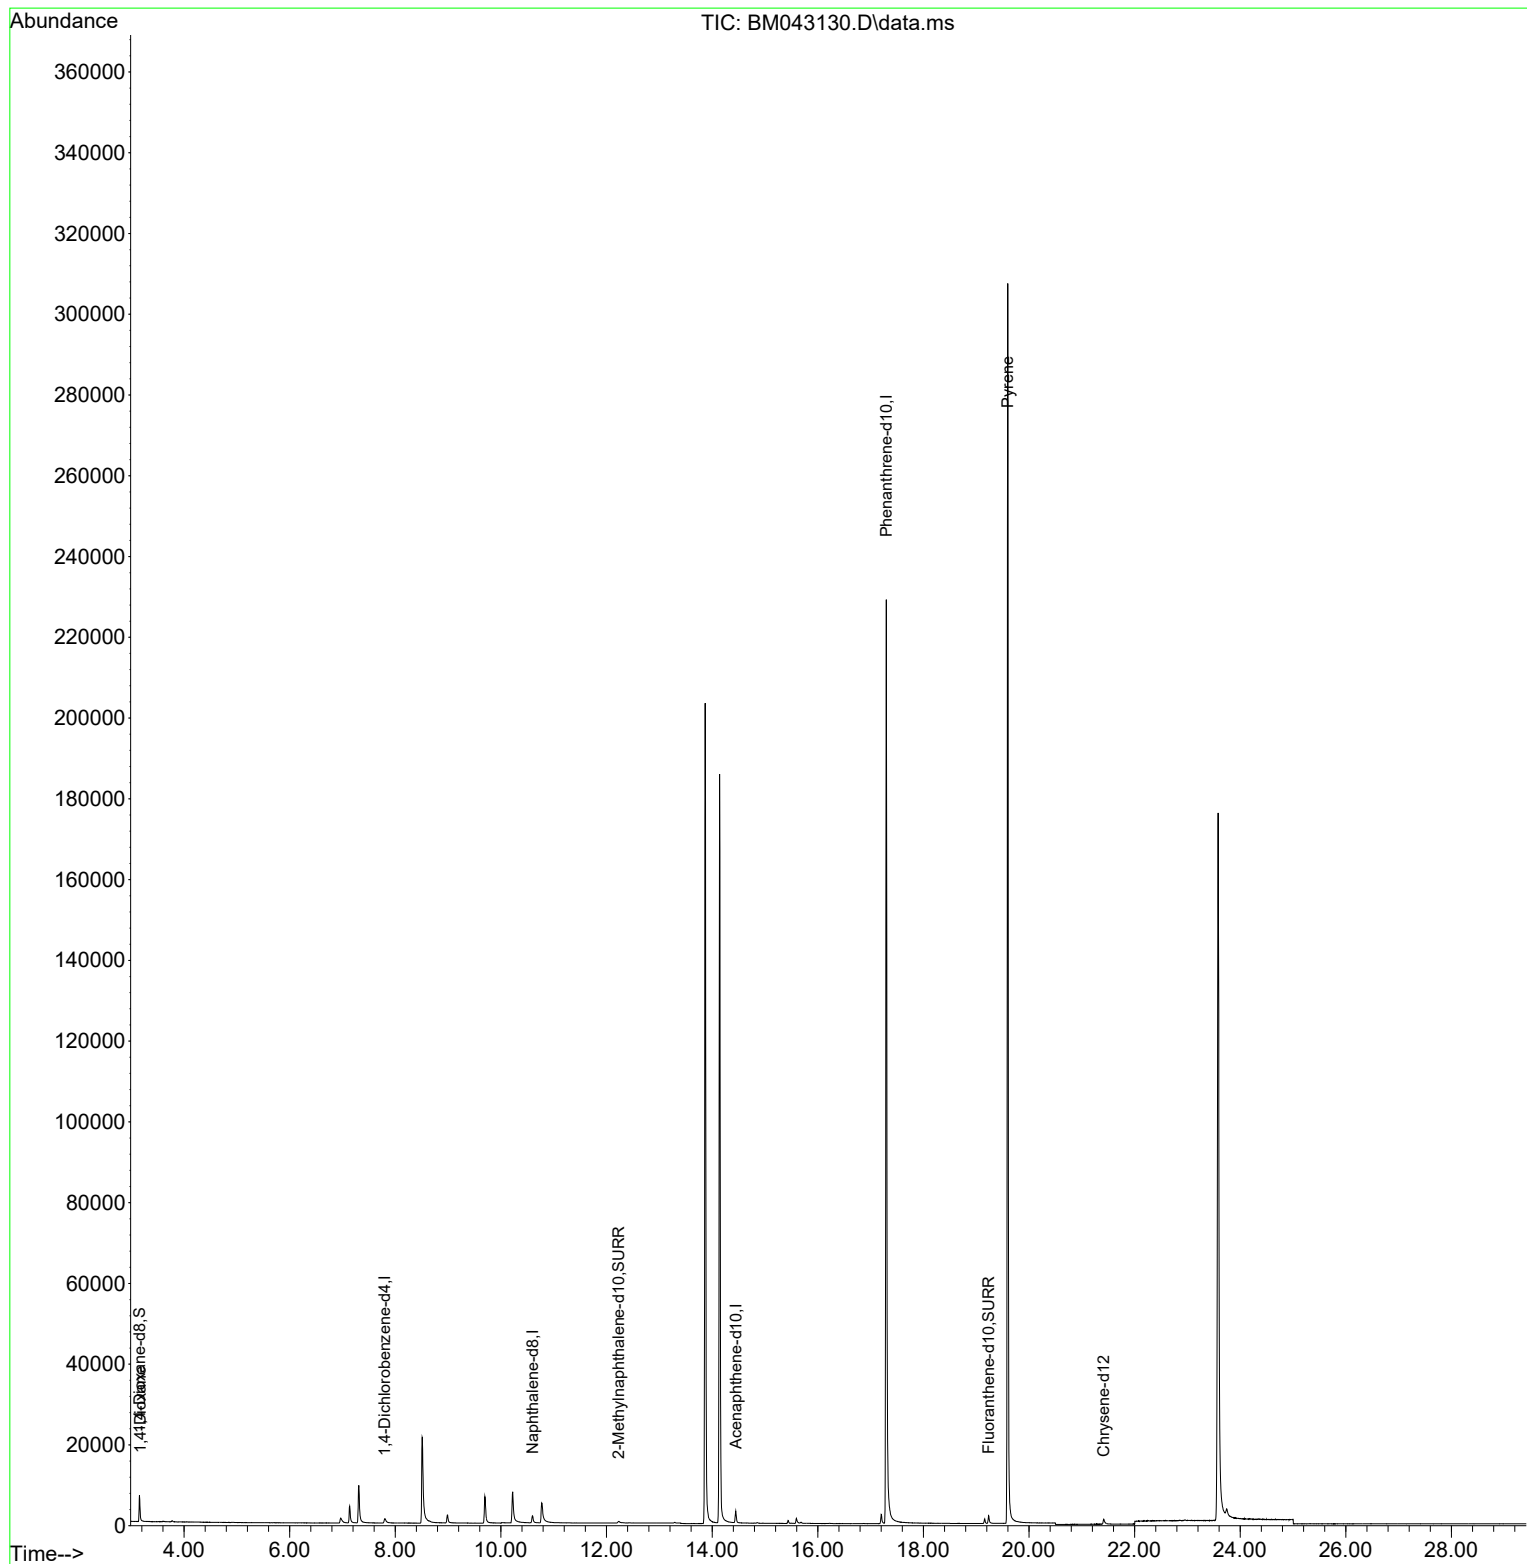


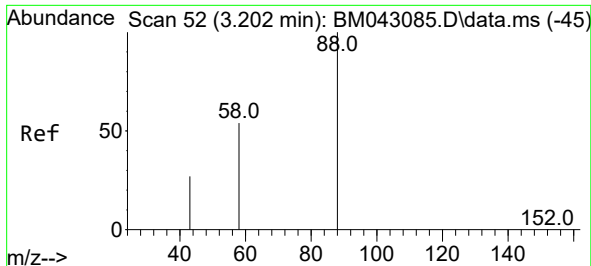

#2
1,4-Dioxane
Concen: 0.024 ng/ul
RT: 3.172 min Scan# 41
Delta R.T. -0.025 min
Lab File: BM043130.D
Acq: 01 Dec 2023 19:45

Instrument :
BNA_M
ClientSampleId :
COAM0

Tgt Ion: 88 Resp: 40
Ion Ratio Lower Upper
88 100
43 29.4 22.8 34.2
58 14.8 26.8 40.2#

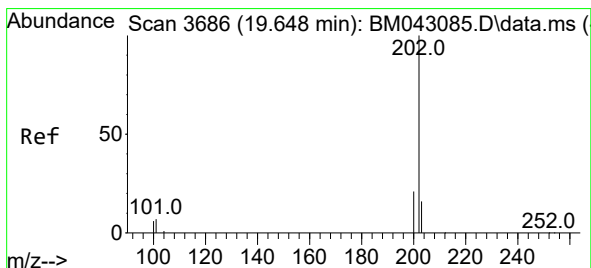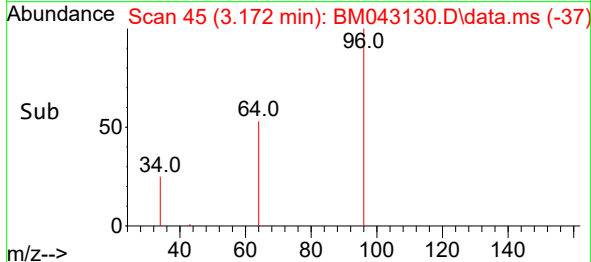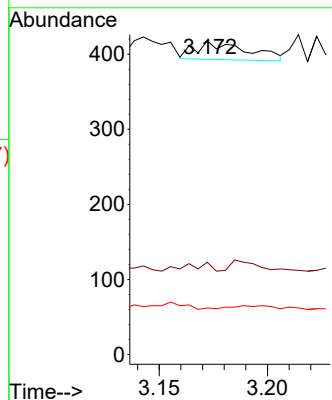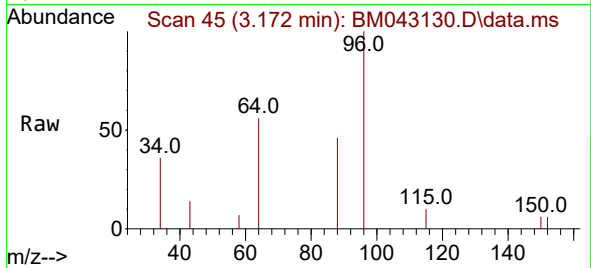

#20
Pyrene
Concen: 0.073 ng/ul
RT: 19.597 min Scan# 3675
Delta R.T. -0.042 min
Lab File: BM043130.D
Acq: 01 Dec 2023 19:45

Tgt Ion: 202 Resp: 628
Ion Ratio Lower Upper
202 100
101 186.9 8.7 13.1#
100 1465.3 7.8 11.8#

