

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043134.D
 Acq On : 01 Dec 2023 22:11
 Operator : MA/JU
 Sample : PB157365BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK365

Quant Time: Dec 02 00:08:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 00:03:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	1014	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.596	136	3010	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.447	164	1715	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.297	188	264315	0.400	ng/ul	# 0.08
17) Chrysene-d12	21.417	240	1486	0.400	ng/ul	0.01
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.75
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	6172	3.967	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1091	0.271	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	2274	0.420	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.441	166	548	0.080	ng/ul#	22
20) Pyrene	19.597	202	538	0.060	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043134.D
Acq On : 01 Dec 2023 22:11
Operator : MA/JU
Sample : PB157365BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK365

Quant Time: Dec 02 00:08:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 00:03:38 2023
Response via : Initial Calibration




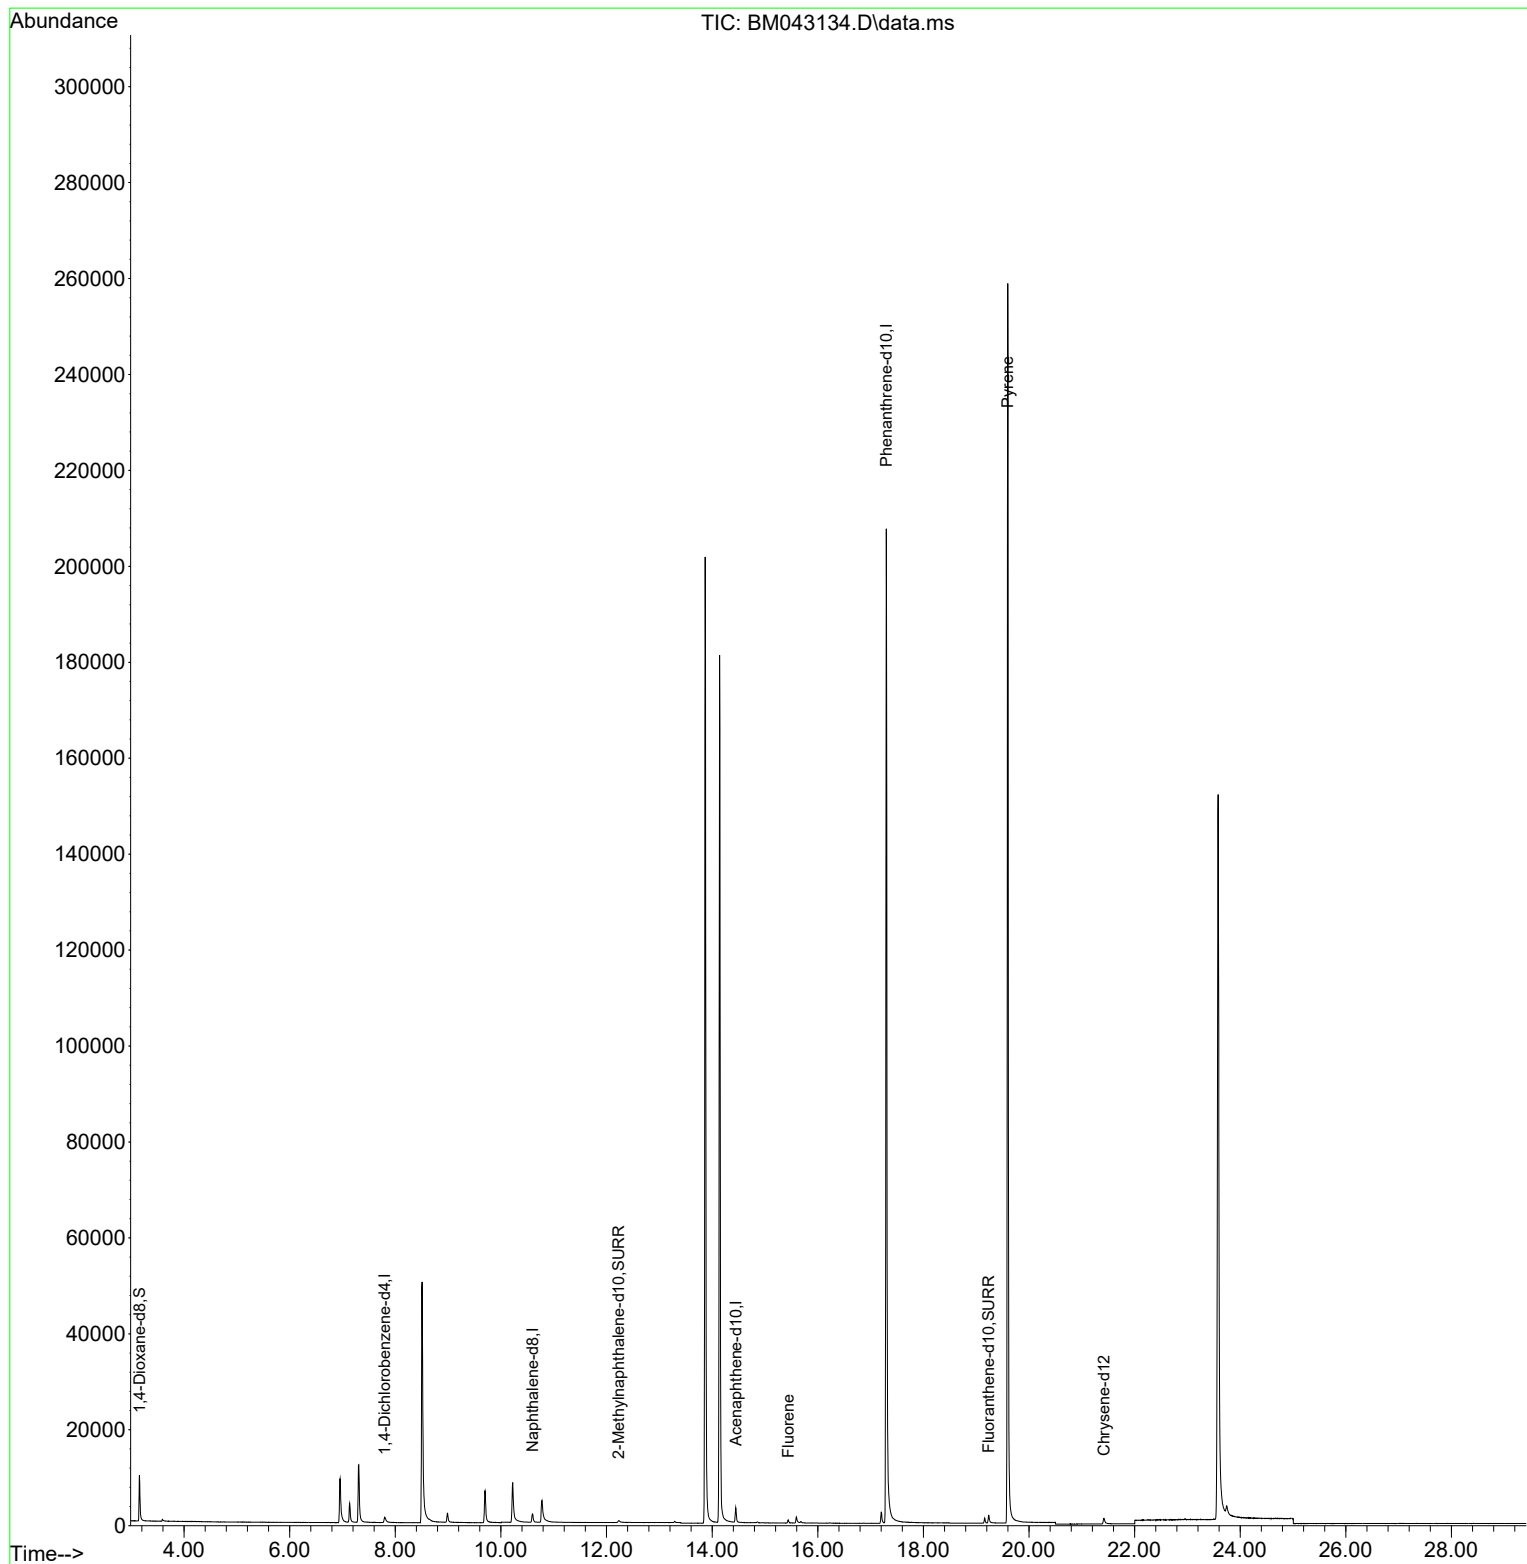


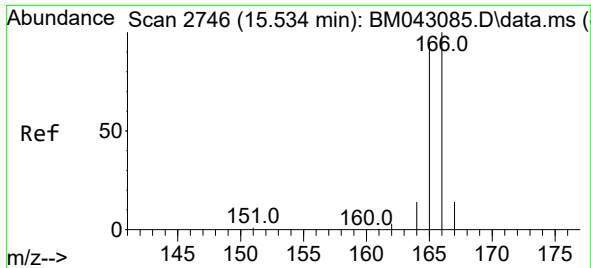

#12
 Fluorene
 Concen: 0.080 ng/ul
 RT: 15.441 min Scan# 21
 Delta R.T. -0.074 min
 Lab File: BM043134.D
 Acq: 01 Dec 2023 22:11

Instrument :
 BNA_M
 ClientSampleId :
 SBLK365

Tgt Ion:166 Resp: 548
 Ion Ratio Lower Upper
 166 100
 165 17.8 79.9 119.9#
 167 41.5 14.2 21.4#

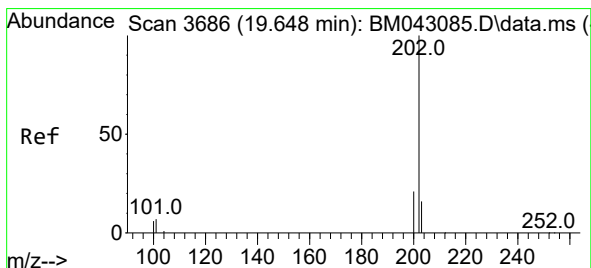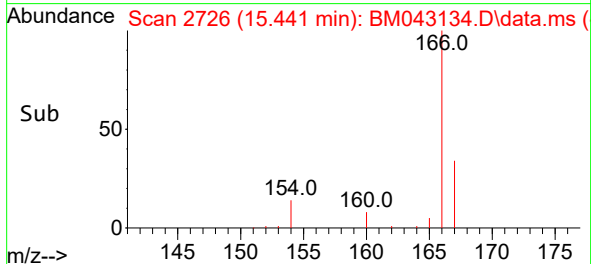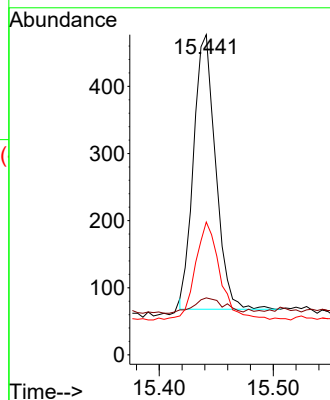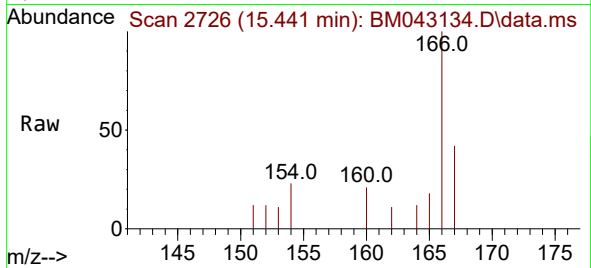

#20
 Pyrene
 Concen: 0.060 ng/ul
 RT: 19.597 min Scan# 3675
 Delta R.T. -0.042 min
 Lab File: BM043134.D
 Acq: 01 Dec 2023 22:11

Tgt Ion:202 Resp: 538
 Ion Ratio Lower Upper
 202 100
 101 180.5 8.7 13.1#
 100 1434.9 7.8 11.8#

