

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043145.D
 Acq On : 02 Dec 2023 05:31
 Operator : MA/JU
 Sample : 05439-11
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC8

Quant Time: Dec 02 22:40:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 01:12:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	849	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.601	136	2446	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.446	164	1506	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.297	188	349786	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.40
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.75
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	4180	3.209	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1043	0.319	ng/ul	0.01
18) Fluoranthene-d10	19.234	212	3203	0.000	ng/ul	0.00
Target Compounds						
12) Fluorene	15.501	166	430	0.072	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043145.D
Acq On : 02 Dec 2023 05:31
Operator : MA/JU
Sample : 05439-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC8

Quant Time: Dec 02 22:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 01:12:12 2023
Response via : Initial Calibration

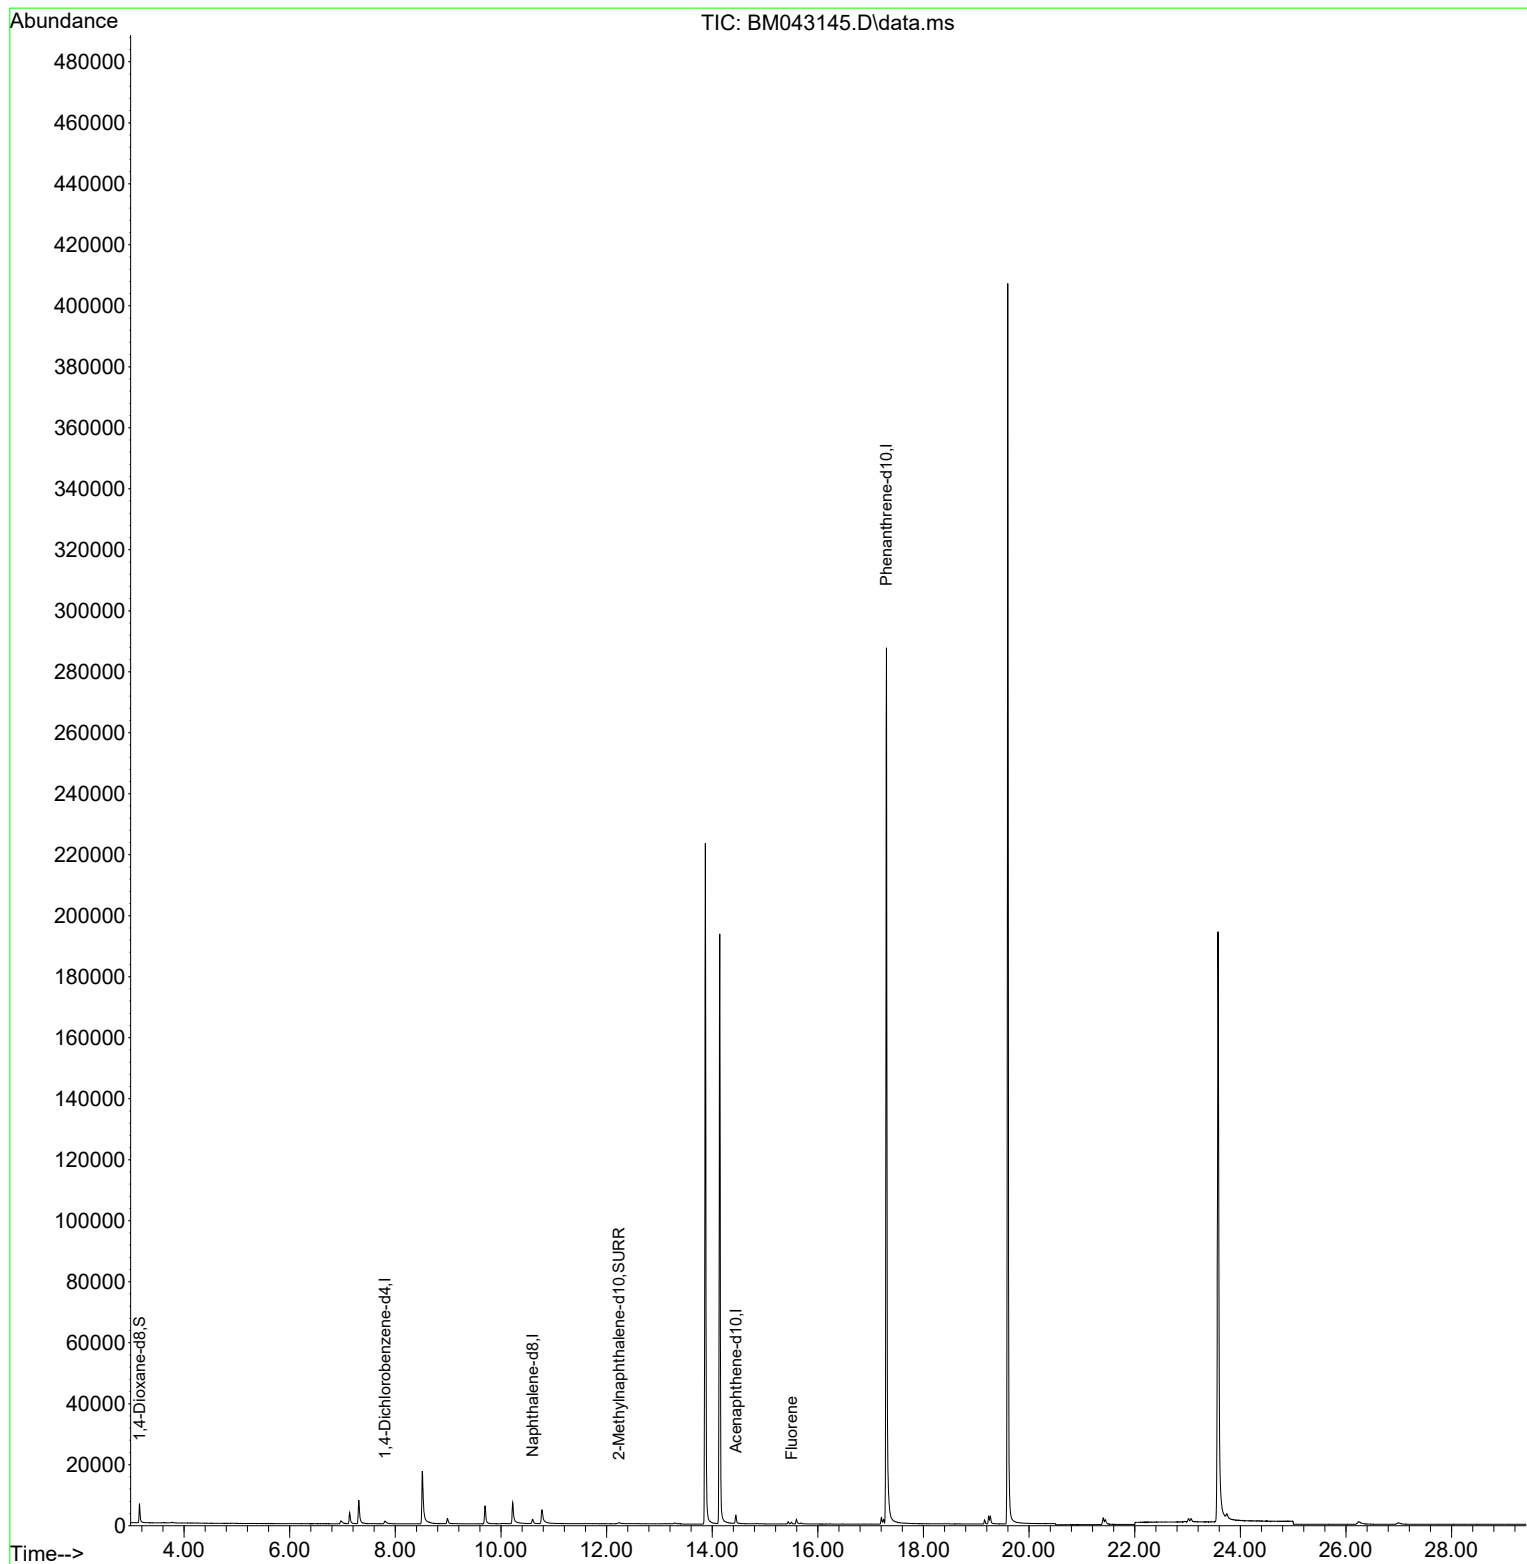

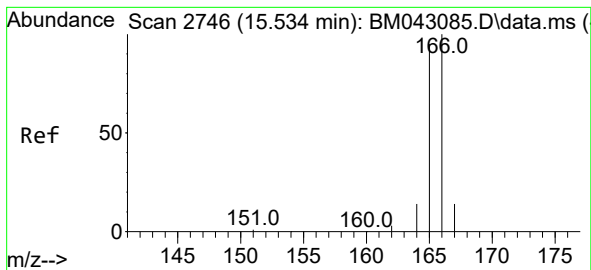

#12

Fluorene

Concen: 0.072 ng/ul

RT: 15.501 min Scan# 21

Delta R.T. -0.014 min

Lab File: BM043145.D


Acq: 02 Dec 2023 05:31

Instrument :

BNA_M

ClientSampleId :

C0AC8

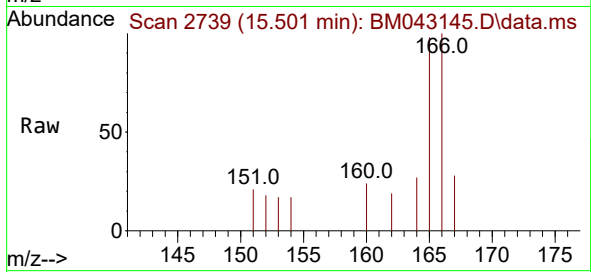

Tgt Ion:166 Resp: 430

Ion	Ratio	Lower	Upper
-----	-------	-------	-------

166	100		
-----	-----	--	--

165	97.7	79.9	119.9
-----	------	------	-------

167	28.5	14.2	21.4#
-----	------	------	-------

