

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043154.D
 Acq On : 02 Dec 2023 11:35
 Operator : MA/JU
 Sample : PB157370BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK370

Quant Time: Dec 02 23:17:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 23:09:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	1228	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.594	136	3628	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.445	164	2175	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188	427254	0.400	ng/ul	# 0.08
17) Chrysene-d12	21.418	240	2494	0.400	ng/ul	# 0.02
23) Perylene-d12	23.741	264	6433	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	7503	3.982	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	1432	0.295	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	3520	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.435	166	860	0.100	ng/ul#	20
20) Pyrene	19.596	202	894	0.059	ng/ul#	1
26) Benzo(a)pyrene	23.575	252	1421	0.060	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043154.D
Acq On : 02 Dec 2023 11:35
Operator : MA/JU
Sample : PB157370BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK370

Quant Time: Dec 02 23:17:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 23:09:32 2023
Response via : Initial Calibration




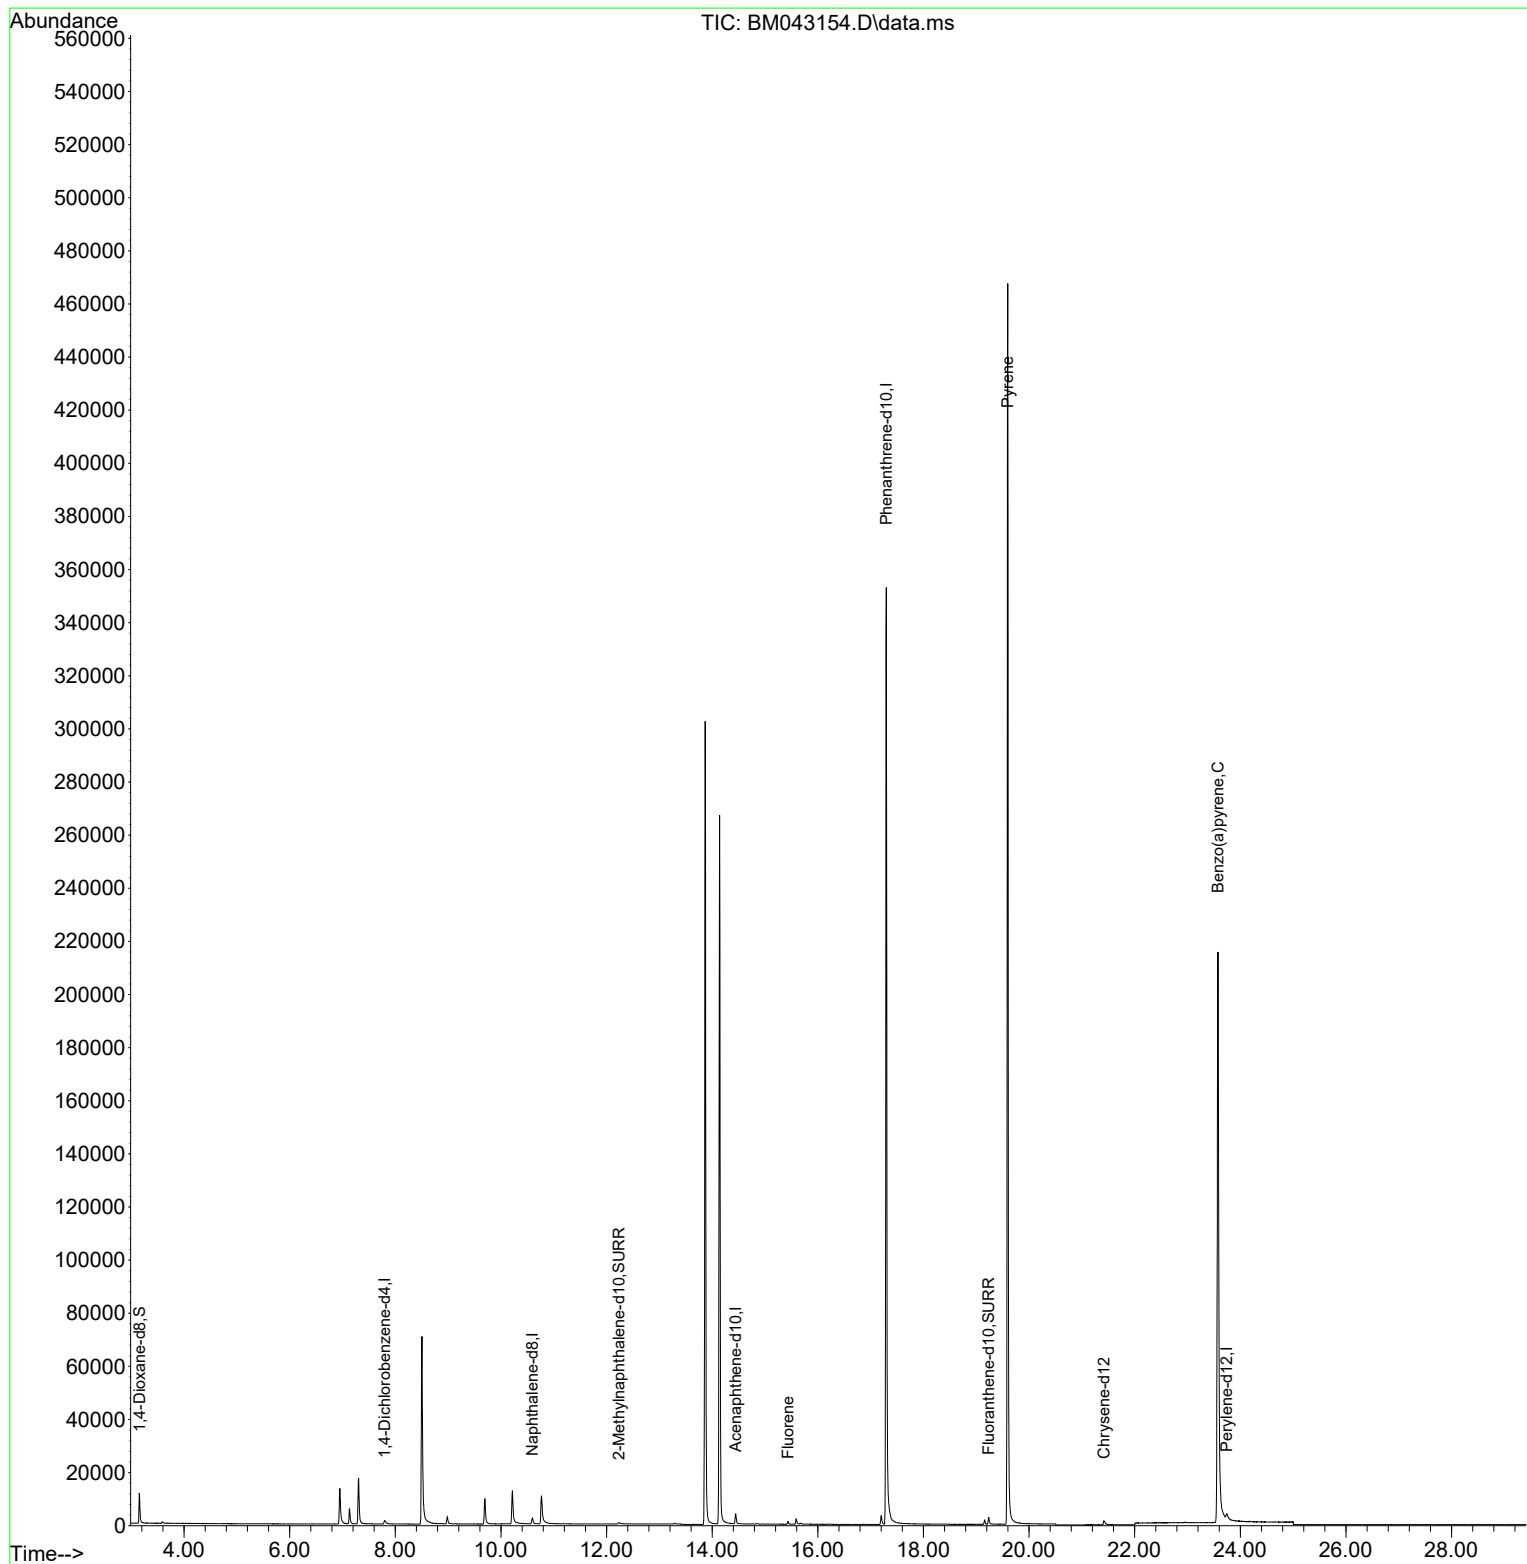


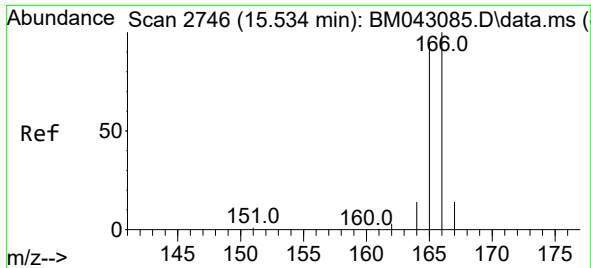

#12
Fluorene
Concen: 0.100 ng/ul
RT: 15.435 min Scan# 21
Delta R.T. -0.080 min
Lab File: BM043154.D
Acq: 02 Dec 2023 11:35




Instrument :
BNA_M
ClientSampleId :
SBLK370


Tgt Ion:166 Resp: 860
Ion Ratio Lower Upper
166 100
165 12.9 79.9 119.9#
167 35.4 14.2 21.4#

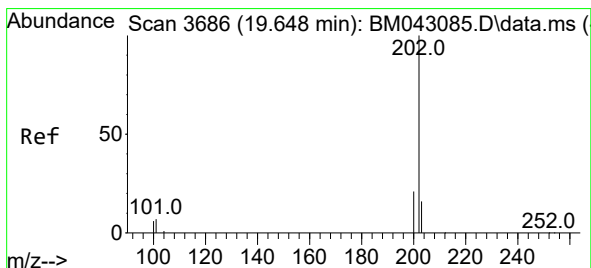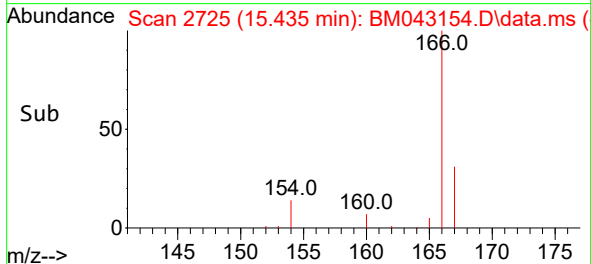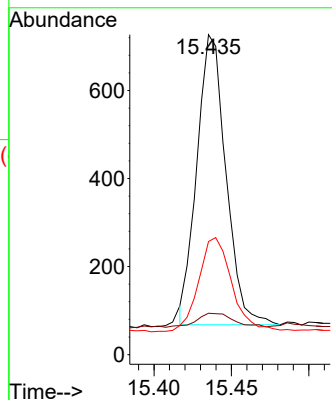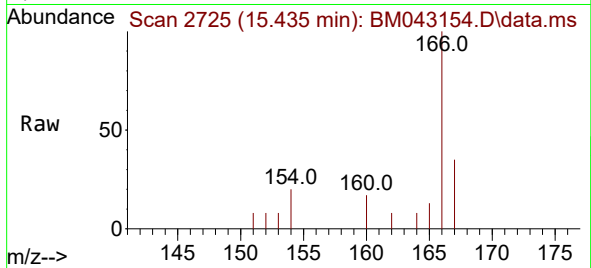

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.596 min Scan# 3675
Delta R.T. -0.043 min
Lab File: BM043154.D
Acq: 02 Dec 2023 11:35


Tgt Ion:202 Resp: 894
Ion Ratio Lower Upper
202 100
101 184.7 8.7 13.1#
100 1459.0 7.8 11.8#

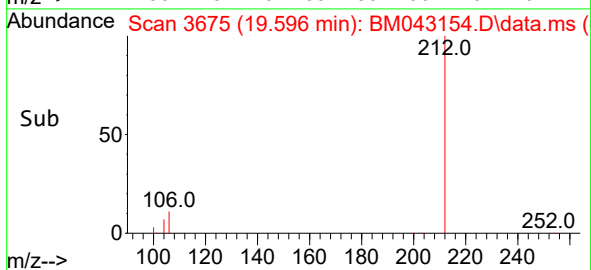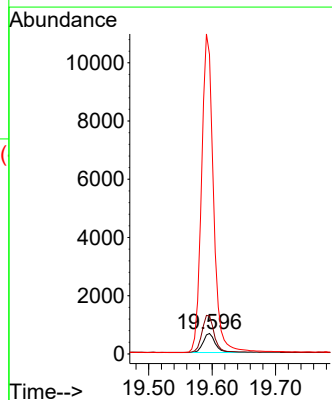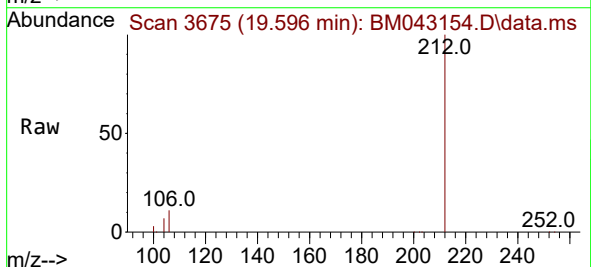

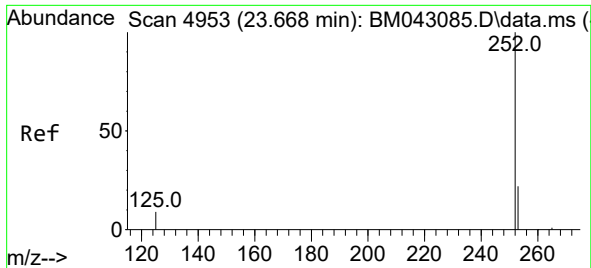

#26
 Benzo(a)pyrene
 Concen: 0.060 ng/ul
 RT: 23.575 min Scan# 49
 Delta R.T. -0.076 min
 Lab File: BM043154.D
 Acq: 02 Dec 2023 11:35

Instrument :
 BNA_M
 ClientSampleId :
 SBLK370

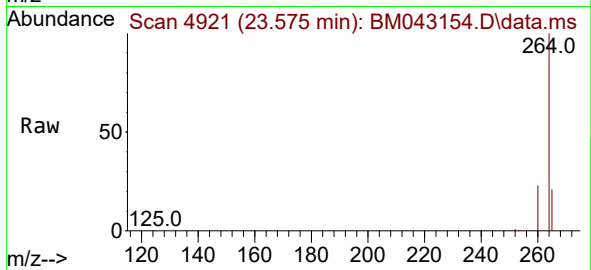

Tgt Ion:252 Resp: 1421
 Ion Ratio Lower Upper
 252 100
 253 57.5 36.6 55.0#
 125 36.7 16.2 24.4#

