

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043160.D
 Acq On : 02 Dec 2023 15:13
 Operator : MA/JU
 Sample : 05473-03
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE7

Quant Time: Dec 02 23:17:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 23:09:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	1195	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.594	136	3829	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.441	164	2324	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.296	188	471902	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.40
23) Perylene-d12	23.744	264	7294	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	4440	2.422	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	1295	0.253	ng/ul	-0.02
18) Fluoranthene-d10	19.233	212	4783	0.000	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.575	252	1751	0.065	ng/ul#	Qvalue 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043160.D
Acq On : 02 Dec 2023 15:13
Operator : MA/JU
Sample : 05473-03
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE7


Quant Time: Dec 02 23:17:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 23:09:32 2023
Response via : Initial Calibration

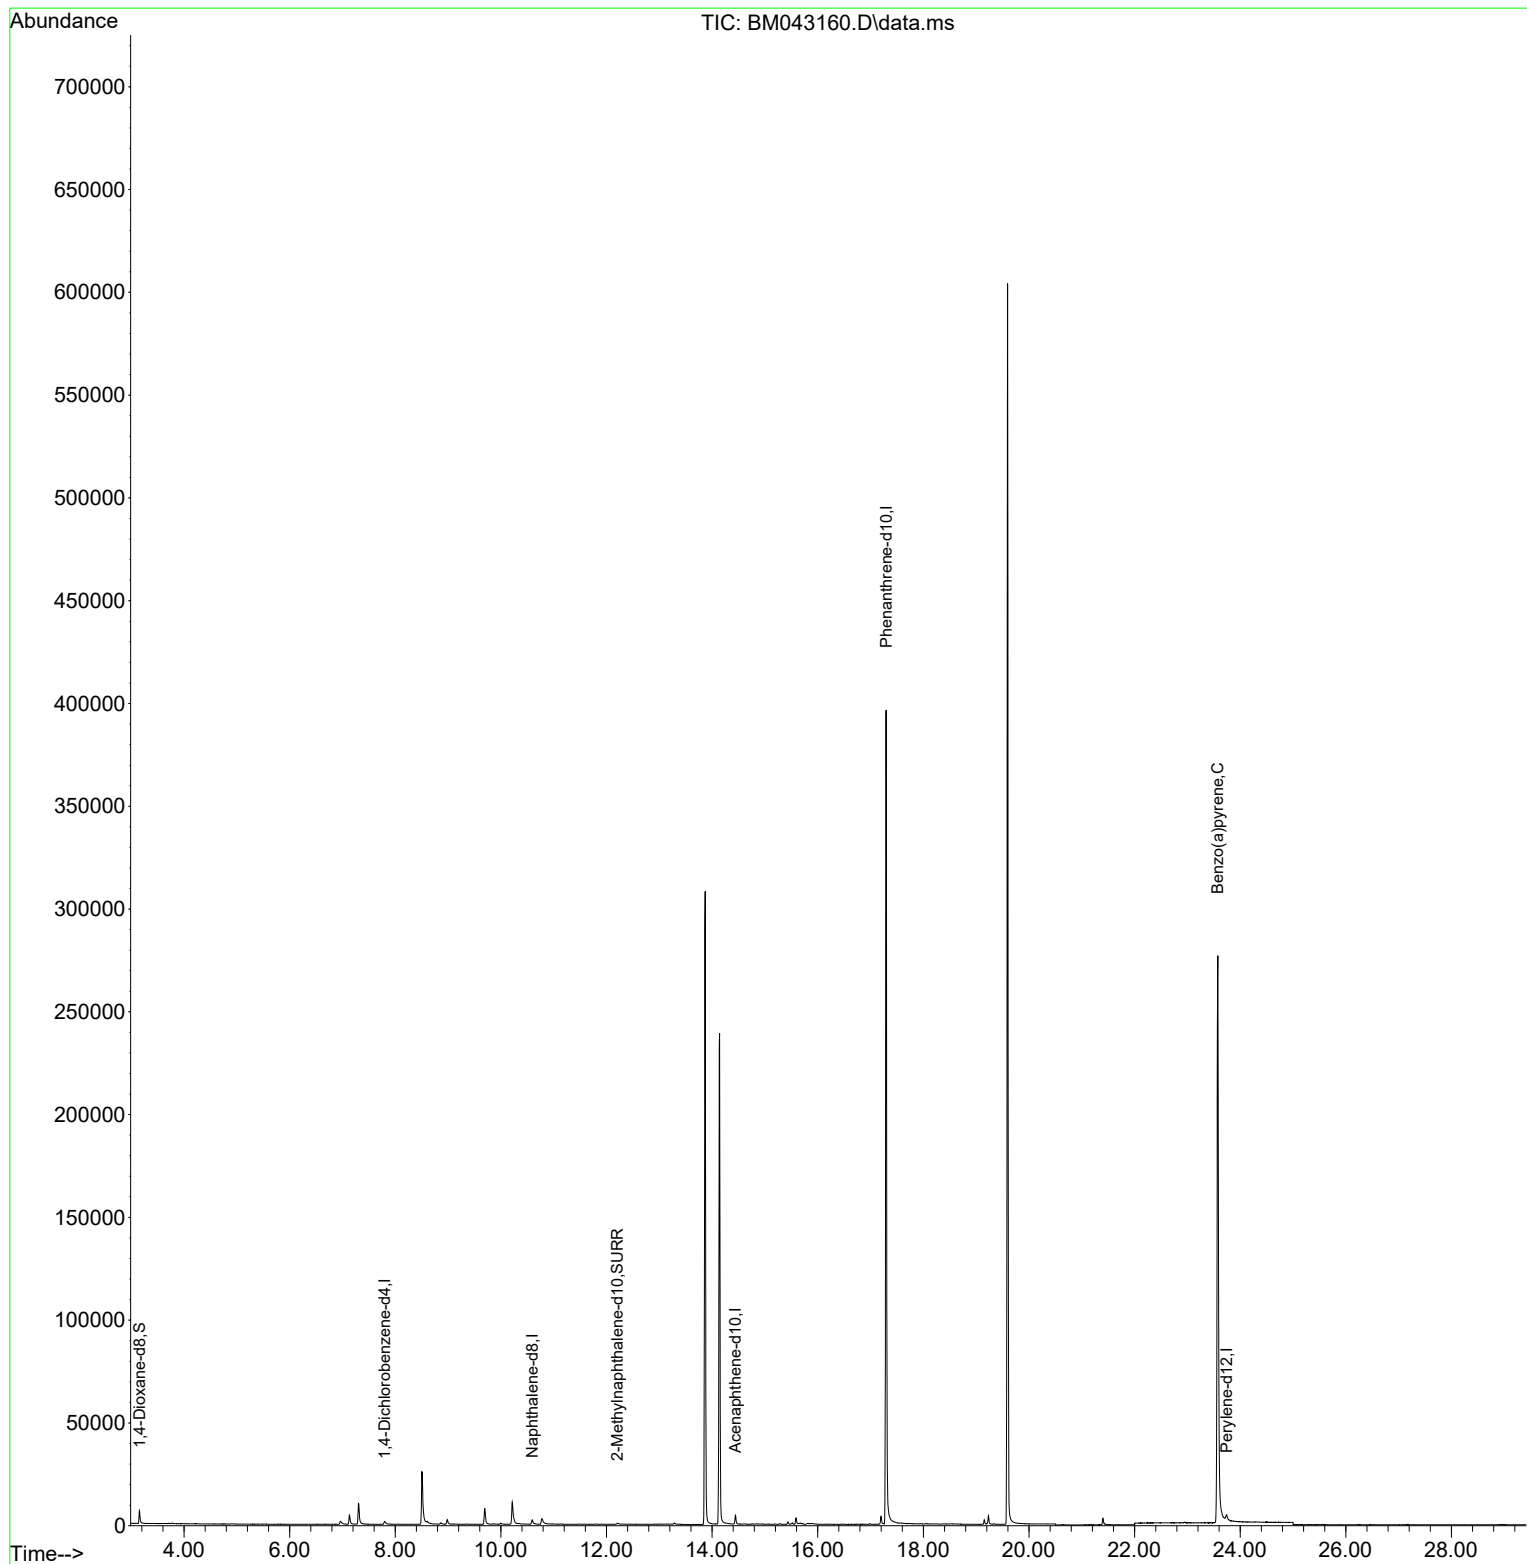

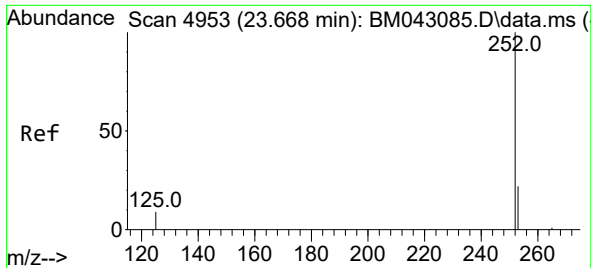

#26
Benzo(a)pyrene
Concen: 0.065 ng/ul
RT: 23.575 min Scan# 4953
Delta R.T. -0.076 min
Lab File: BM043160.D
Acq: 02 Dec 2023 15:13

Instrument :
BNA_M
ClientSampleId :
C0AE7

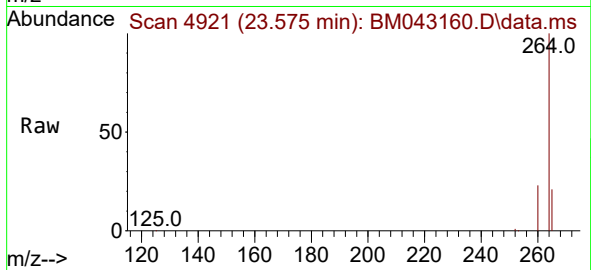

Tgt Ion:252 Resp: 1751
Ion Ratio Lower Upper
252 100
253 59.2 36.6 55.0#
125 37.2 16.2 24.4#

