

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043161.D
 Acq On : 02 Dec 2023 15:49
 Operator : MA/JU
 Sample : 05473-04
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE8

Quant Time: Dec 02 23:18:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 02 23:09:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	1333	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.596	136	4032	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.442	164	2510	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.293	188	509209	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.40
23) Perylene-d12	23.738	264	7418	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	4691	2.294	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	1621	0.300	ng/ul	-0.01
18) Fluoranthene-d10	19.230	212	4974	0.000	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.574	252	1985	0.073	ng/ul#	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043161.D
Acq On : 02 Dec 2023 15:49
Operator : MA/JU
Sample : 05473-04
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8


Quant Time: Dec 02 23:18:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 02 23:09:32 2023
Response via : Initial Calibration

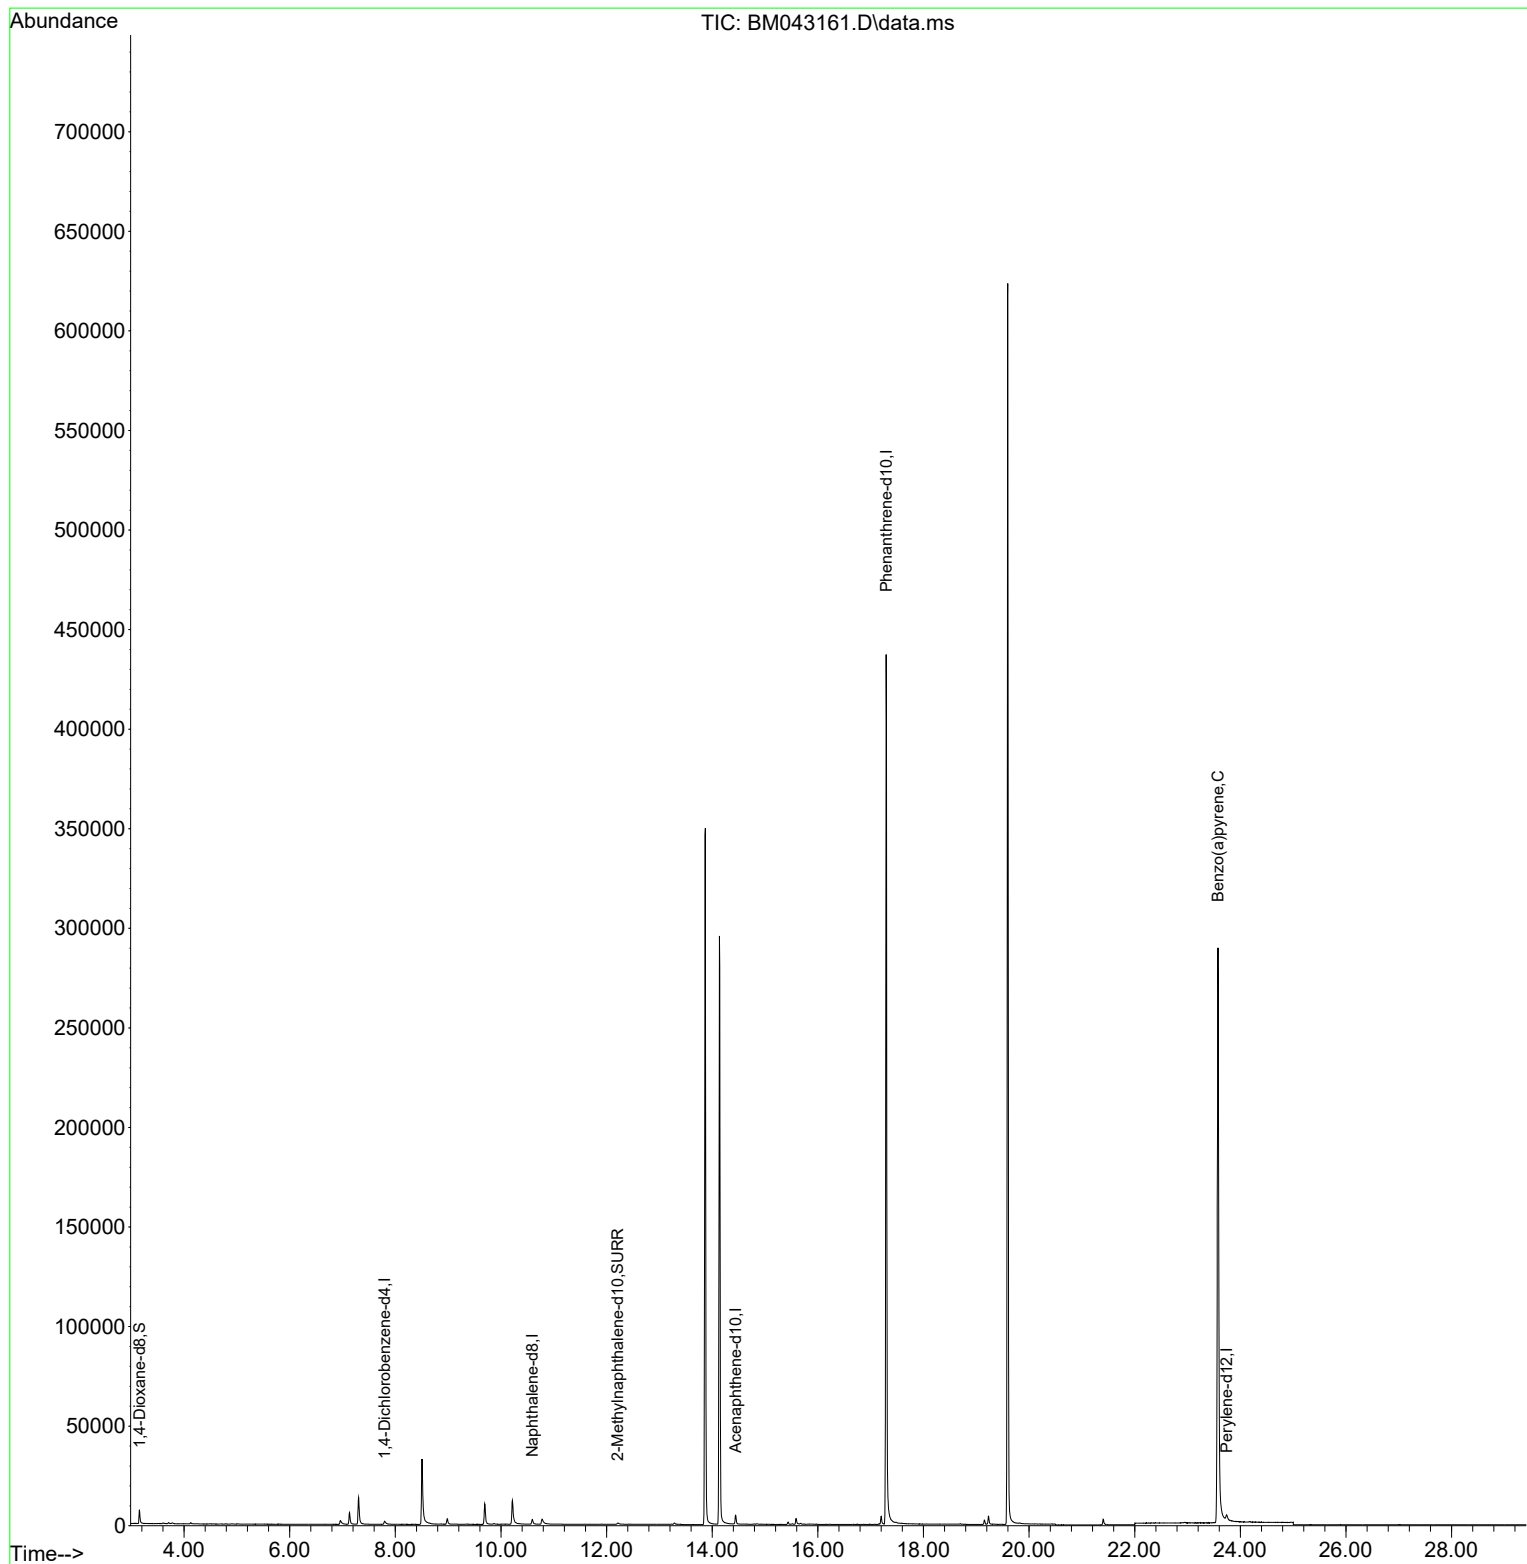

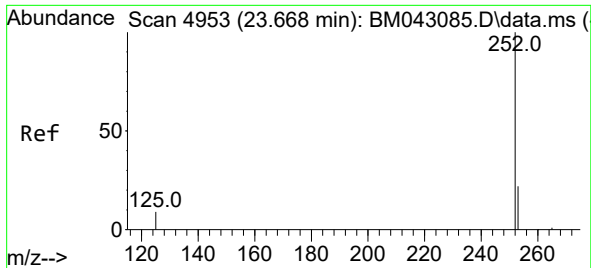

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.574 min Scan# 4953
Delta R.T. -0.076 min
Lab File: BM043161.D
Acq: 02 Dec 2023 15:49

Instrument :
BNA_M
ClientSampleId :
C0AE8

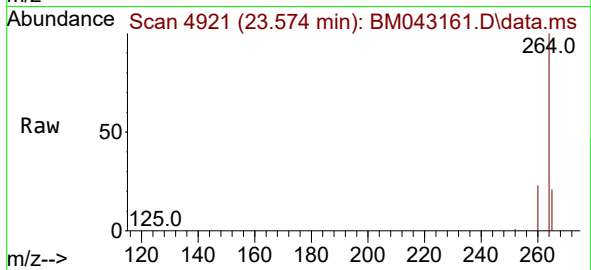

Tgt Ion:252 Resp: 1985
Ion Ratio Lower Upper
252 100
253 54.5 36.6 55.0
125 34.4 16.2 24.4#

