

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043096.D
 Acq On : 30 Nov 2023 21:53
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :mohammad ahmed 12/04/2023

Quant Time: Dec 01 00:44:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 00:42:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	828	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.616	136	2218	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.450	164	1217	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.208	188	2430	0.400	ng/ul	-0.02
17) Chrysene-d12	21.406	240	1703	0.400	ng/ul	0.00
23) Perylene-d12	23.753	264	2179m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	795	0.626	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.222	152	515	0.174	ng/ul	-0.01
18) Fluoranthene-d10	19.238	212	1109	0.179	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.666	128	1048	0.174	ng/ul	94
7) 2-Methylnaphthalene	12.294	142	873	0.246	ng/ul	94
8) 1-Methylnaphthalene	12.503	142	643	0.162	ng/ul	96
15) Phenanthrene	17.250	178	2458	0.354	ng/ul	99
16) Anthracene	17.347	178	354m	0.054	ng/ul	
19) Fluoranthene	19.270	202	3338	0.346	ng/ul	97
20) Pyrene	19.633	202	2603	0.254	ng/ul	97
21) Benzo(a)anthracene	21.395	228	1206	0.218	ng/ul#	90
22) Chrysene	21.441	228	1303	0.127	ng/ul#	91
24) Benzo(b)fluoranthene	23.031	252	1530	0.208	ng/ul	75
25) Benzo(k)fluoranthene	23.072	252	666m	0.066	ng/ul	
26) Benzo(a)pyrene	23.648	252	659	0.082	ng/ul#	60
27) Indeno(1,2,3-cd)pyrene	26.219	276	642	0.059	ng/ul#	100
29) Benzo(g,h,i)perylene	26.983	276	533	0.050	ng/ul#	56

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043096.D
Acq On : 30 Nov 2023 21:53
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AA3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :mohammad ahmed 12/04/2023


Quant Time: Dec 01 00:44:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 00:42:42 2023
Response via : Initial Calibration

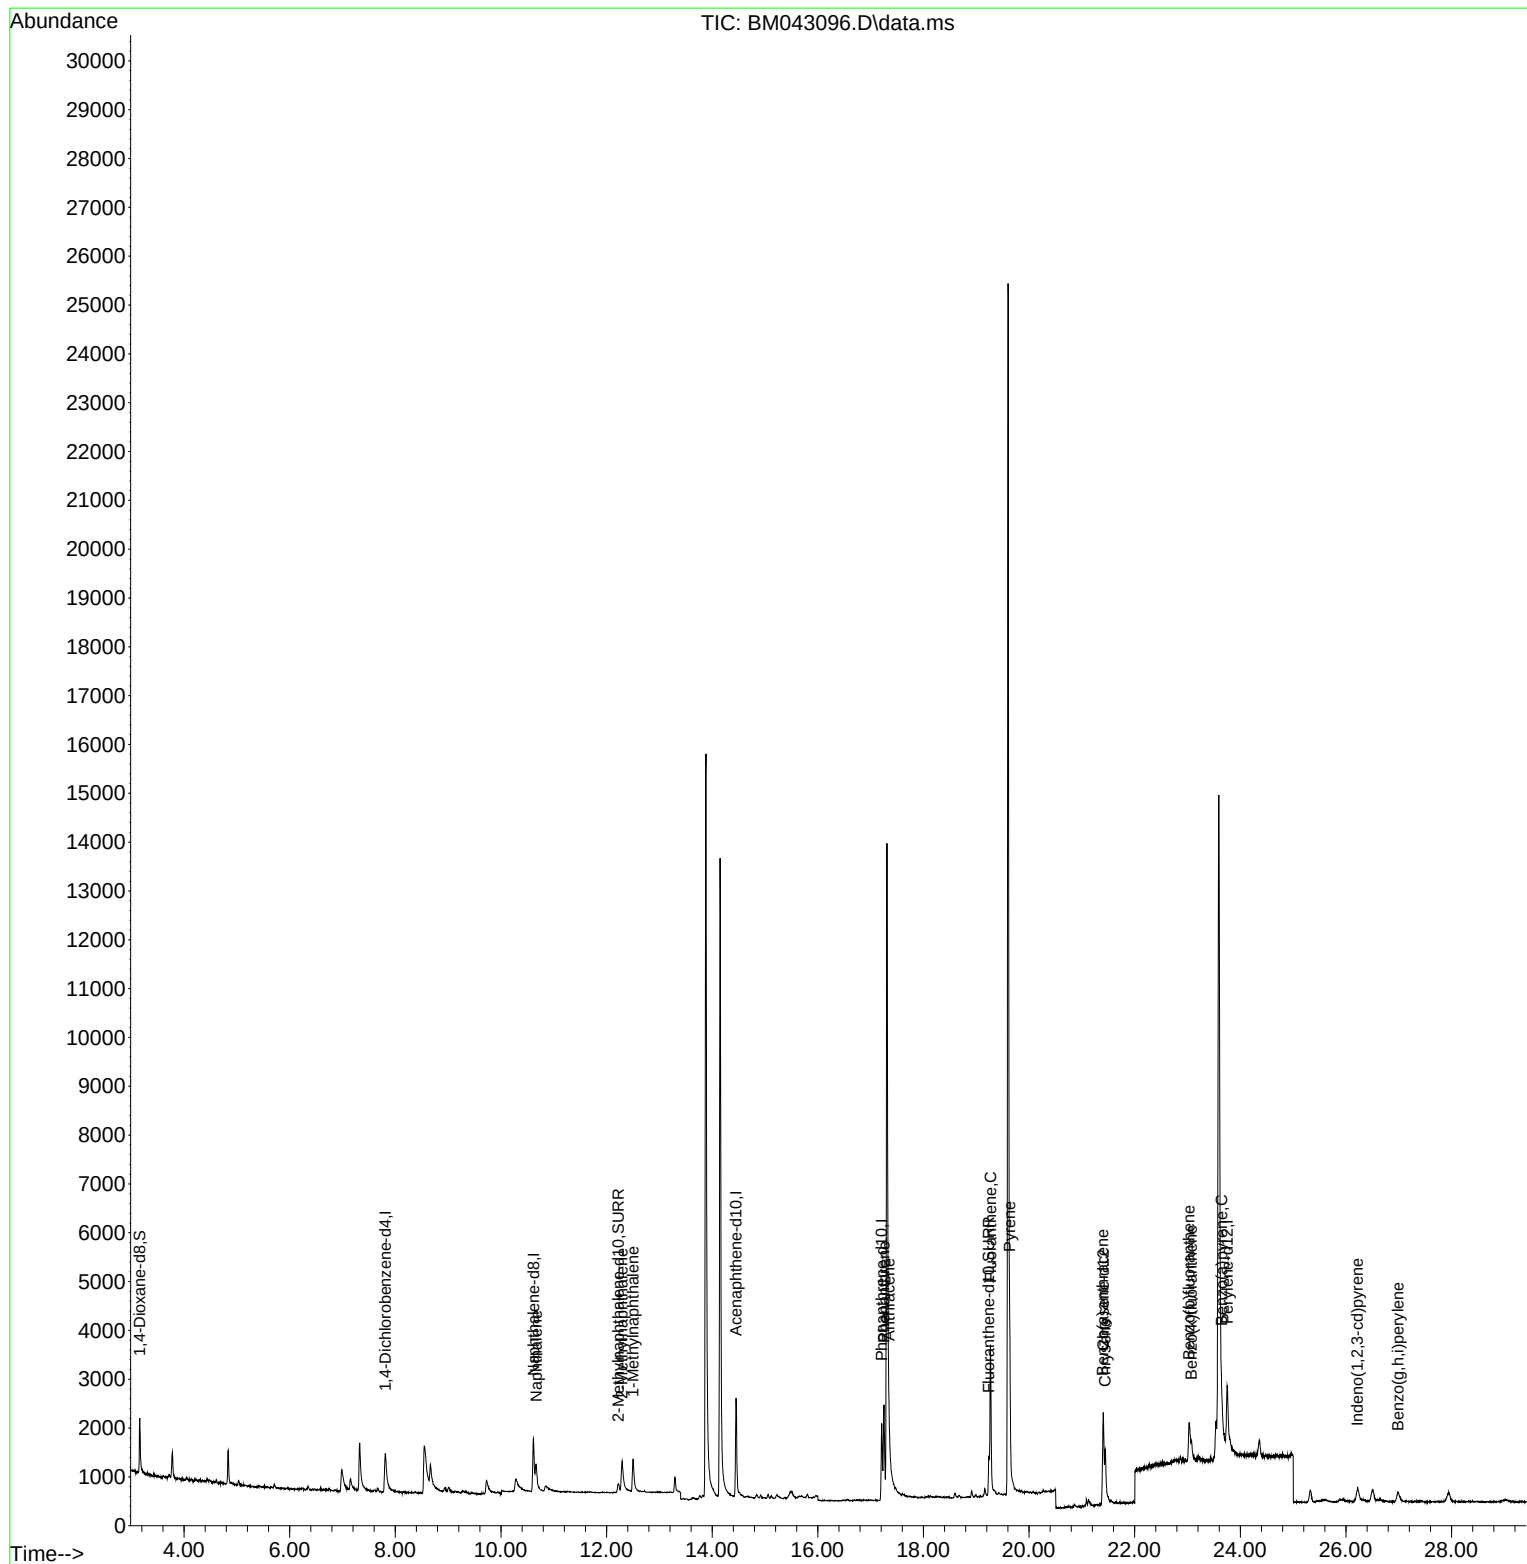

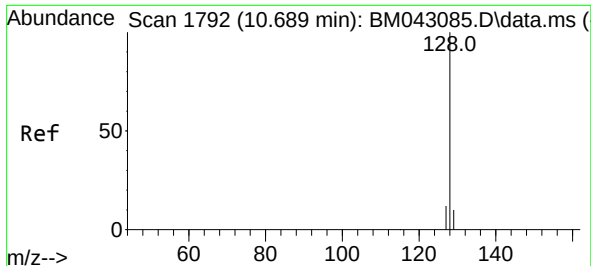

#5
Naphthalene
Concen: 0.174 ng/ul
RT: 10.666 min Scan# 1788
Delta R.T. -0.023 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53




Instrument :
BNA_M
ClientSampleId :
C0AA3



Tgt Ion:128 Resp: 1048
Ion Ratio Lower Upper
128 100
129 21.5 16.0 24.0
127 24.6 16.5 24.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/01/2023
Supervised By :mohammad ahmed 12/04/2023

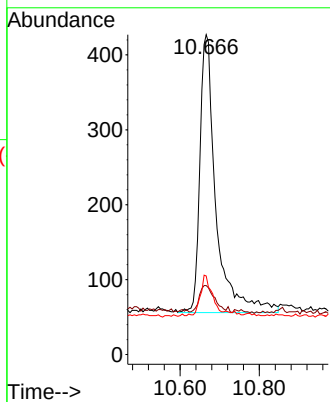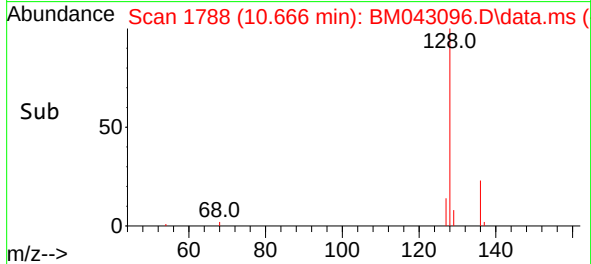

#7
2-Methylnaphthalene
Concen: 0.246 ng/ul
RT: 12.294 min Scan# 2084
Delta R.T. -0.018 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53


Tgt Ion:142 Resp: 873
Ion Ratio Lower Upper
142 100
141 89.1 76.1 114.1

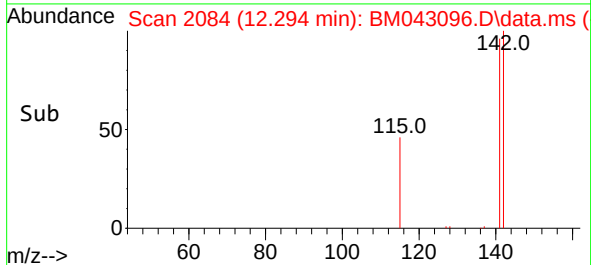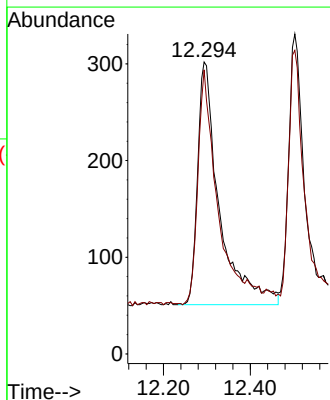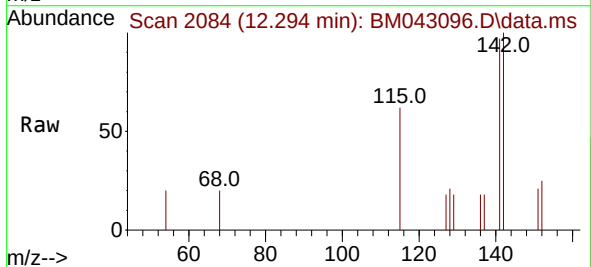



#8
1-Methylnaphthalene
Concen: 0.162 ng/ul
RT: 12.503 min Scan# 2122
Delta R.T. -0.007 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53




Instrument :
BNA_M
ClientSampleId :
C0AA3




Tgt Ion:142 Resp: 64
Ion Ratio Lower Upper
142 100
141 96.6 73.8 110.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/01/2023
Supervised By :mohammad ahmed 12/04/2023

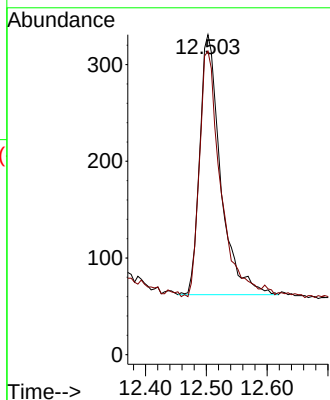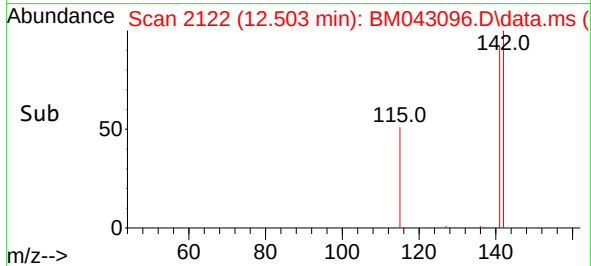


#15
Phenanthrene
Concen: 0.354 ng/ul
RT: 17.250 min Scan# 3143
Delta R.T. -0.022 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53

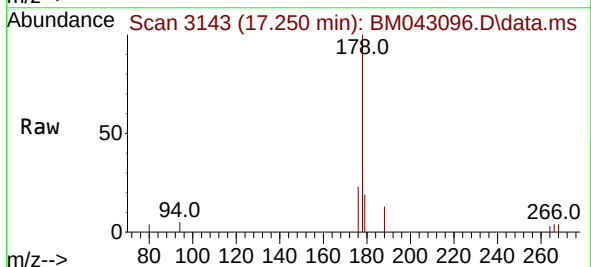


Tgt Ion:178 Resp: 2458
Ion Ratio Lower Upper
178 100
179 19.2 15.7 23.5
176 22.8 18.9 28.3

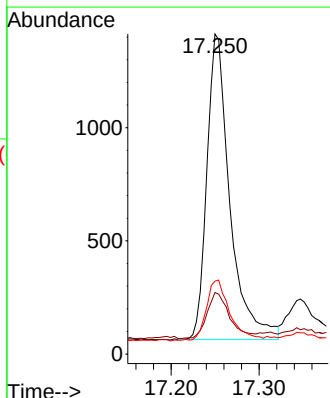



#16
 Anthracene
 Concen: 0.054 ng/ul m
 RT: 17.347 min Scan# 3173
 Delta R.T. -0.031 min
 Lab File: BM043096.D
 Acq: 30 Nov 2023 21:53




Instrument :
 BNA_M
 ClientSampleId :
 C0AA3



Tgt Ion:178 Resp: 354
 Ion Ratio Lower Upper
 178 100
 179 44.0 17.3 25.9
 176 38.7 20.5 30.7




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :mohammad ahmed 12/04/2023

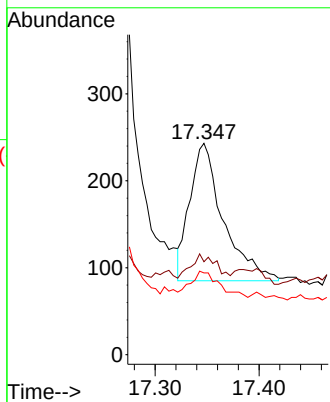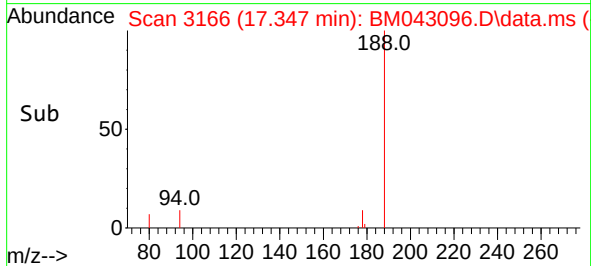

#19
 Fluoranthene
 Concen: 0.346 ng/ul
 RT: 19.270 min Scan# 3605
 Delta R.T. -0.010 min
 Lab File: BM043096.D
 Acq: 30 Nov 2023 21:53


Tgt Ion:202 Resp: 3338
 Ion Ratio Lower Upper
 202 100
 101 8.4 7.8 11.8
 100 7.8 7.1 10.7

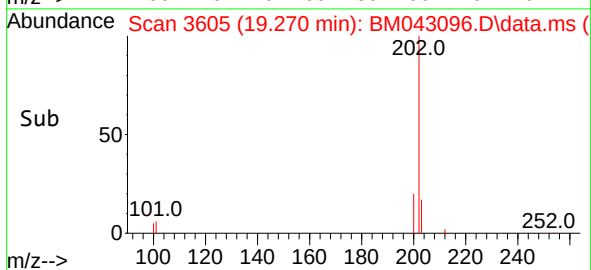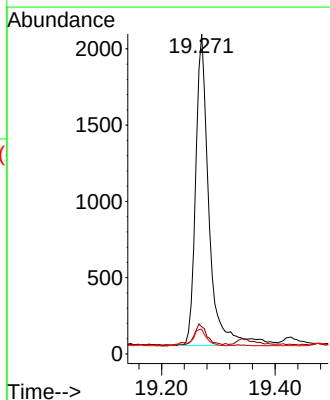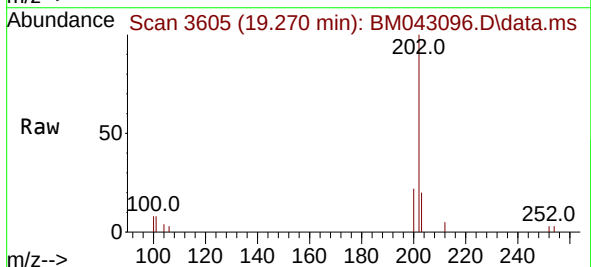

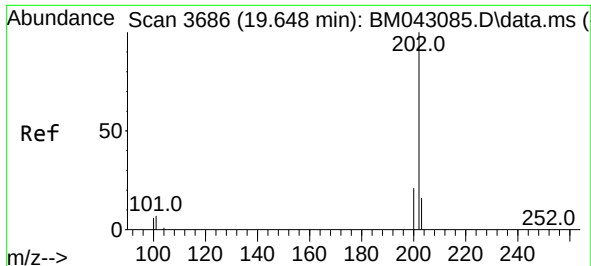

#20
Pyrene
Concen: 0.254 ng/u1
RT: 19.633 min Scan# 30
Delta R.T. -0.015 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53




Instrument :
BNA_M
ClientSampleId :
C0AA3




Tgt Ion:202 Resp: 260
Ion Ratio Lower Upper
202 100
101 11.4 8.7 13.1
100 11.2 7.8 11.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/01/2023
Supervised By :mohammad ahmed 12/04/2023

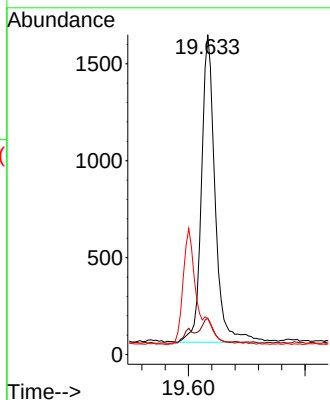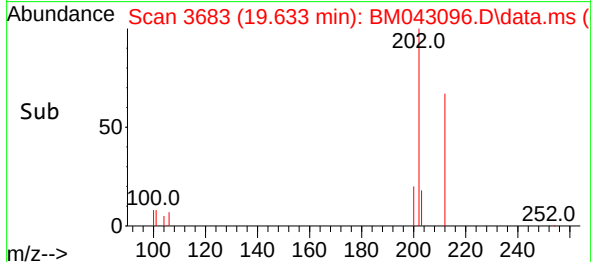


#21
Benzo(a)anthracene
Concen: 0.218 ng/u1
RT: 21.395 min Scan# 4175
Delta R.T. -0.005 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53

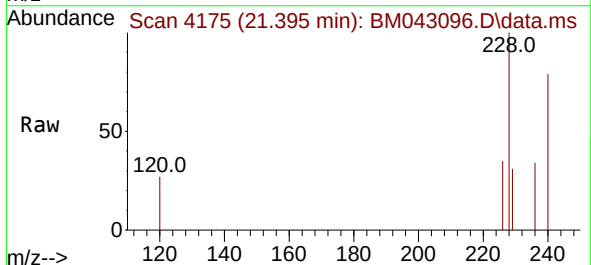


Tgt Ion:228 Resp: 1206
Ion Ratio Lower Upper
228 100
229 30.7 19.4 29.0#
226 35.1 24.9 37.3

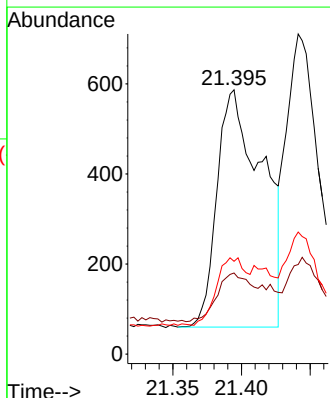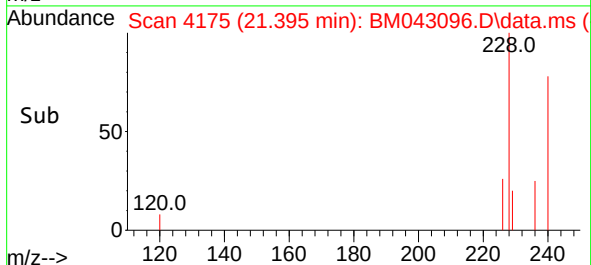

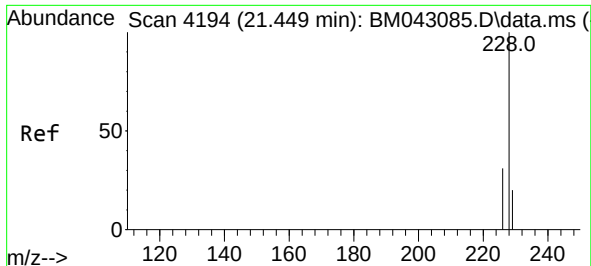

#22
Chrysene
Concen: 0.127 ng/ul
RT: 21.441 min Scan# 4191
Delta R.T. -0.008 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53




Instrument :
BNA_M
ClientSampleId :
C0AA3




Tgt Ion:228 Resp: 1300
Ion Ratio Lower Upper
228 100
226 38.1 27.2 40.8
229 28.0 18.0 27.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/01/2023
Supervised By :mohammad ahmed 12/04/2023

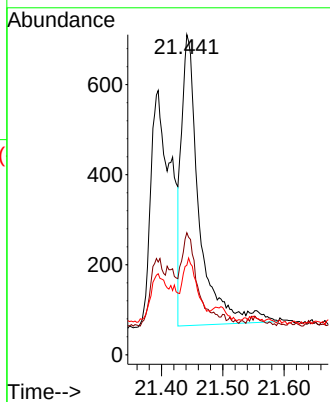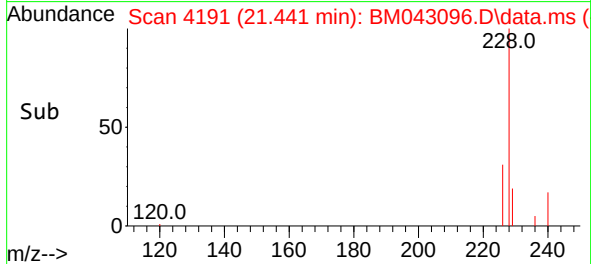


#24
Benzo(b)fluoranthene
Concen: 0.208 ng/ul
RT: 23.031 min Scan# 4735
Delta R.T. -0.005 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53

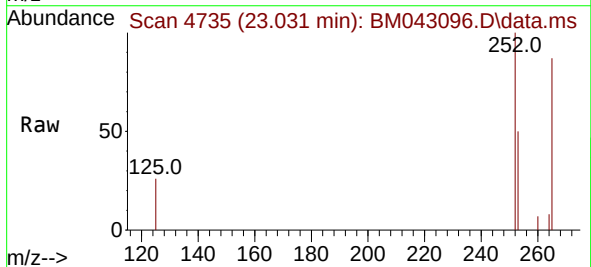


Tgt Ion:252 Resp: 1530
Ion Ratio Lower Upper
252 100
253 49.9 0.0 71.8
125 26.2 0.0 29.0

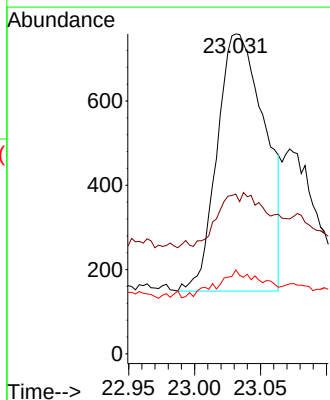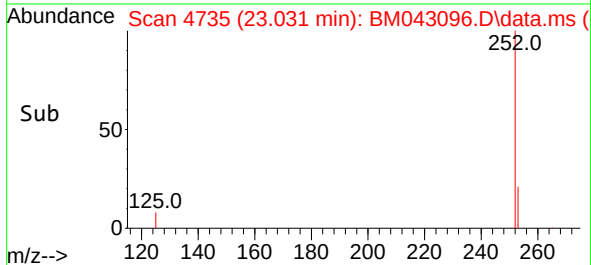



#25
Benzo(k)fluoranthene
Concen: 0.066 ng/ul m
RT: 23.072 min Scan# 4749
Delta R.T. -0.017 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53




Instrument :
BNA_M
ClientSampleId :
C0AA3




Tgt Ion:252 Resp: 660
Ion Ratio Lower Upper
252 100
253 65.8 28.2 42.2
125 34.2 11.0 16.6

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/01/2023
Supervised By :mohammad ahmed 12/04/2023

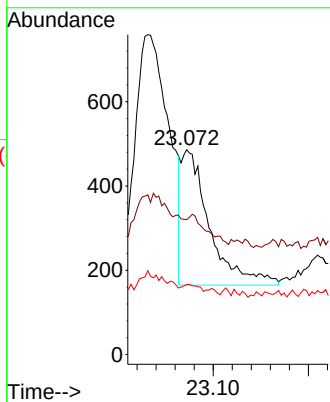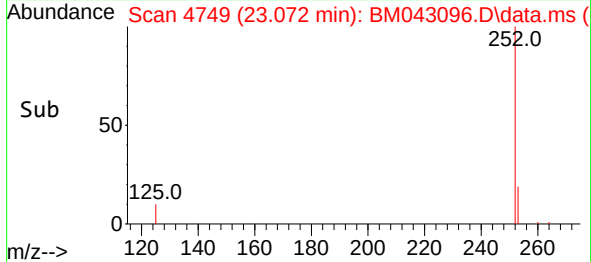


#26
Benzo(a)pyrene
Concen: 0.082 ng/ul
RT: 23.648 min Scan# 4946
Delta R.T. -0.020 min
Lab File: BM043096.D
Acq: 30 Nov 2023 21:53

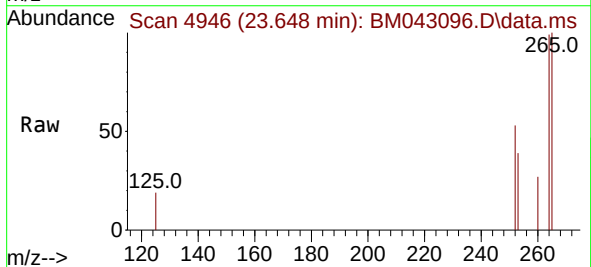

Tgt Ion:252 Resp: 659
Ion Ratio Lower Upper
252 100
253 74.7 36.6 55.0#
125 35.1 16.2 24.4#

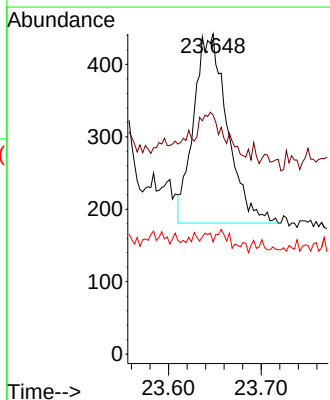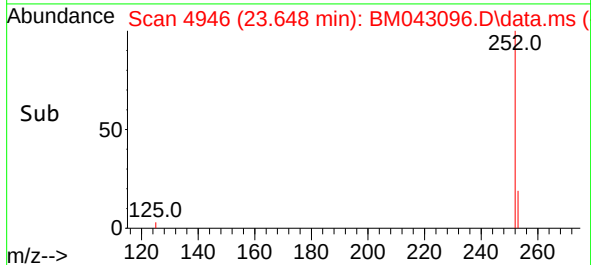



#27

Indeno(1,2,3-cd)pyrene

Concen: 0.059 ng/ul

RT: 26.219 min Scan# 51

Delta R.T. -0.009 min

Lab File: BM043096.D

Acq: 30 Nov 2023 21:53

Instrument :

BNA_M

ClientSampleId :

C0AA3





Tgt Ion:	276	Resp:	64
Ion Ratio	Lower	Upper	
276	100		
138	0.0	0.0	0.0
227	0.2	0.2	0.2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/01/2023

Supervised By :mohammad ahmed 12/04/2023

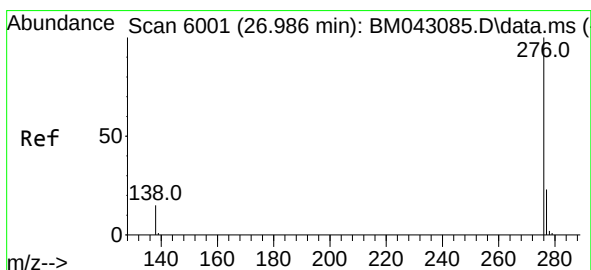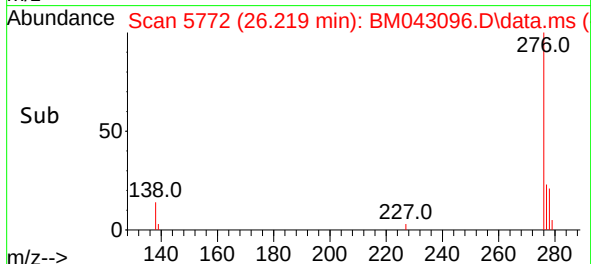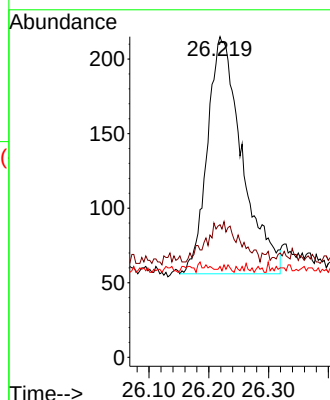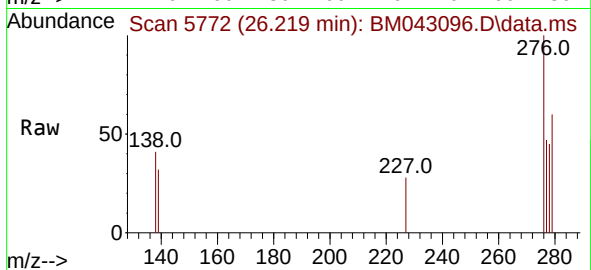

#29

Benzo(g,h,i)perylene

Concen: 0.050 ng/ul

RT: 26.983 min Scan# 6000

Delta R.T. -0.003 min

Lab File: BM043096.D

Acq: 30 Nov 2023 21:53

Tgt Ion:	276	Resp:	533
Ion Ratio	Lower	Upper	
276	100		
138	43.7	17.8	26.8#
277	53.0	23.8	35.8#

