

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
 Data File : BM043117.D
 Acq On : 01 Dec 2023 11:11
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/04/2023
 Supervised By :mohammad ahmed 12/04/2023

Quant Time: Dec 01 23:18:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 00:42:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	1137m	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.601	136	3169	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.447	164	1666m	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.205	188	3246	0.400	ng/ul	#-0.03
17) Chrysene-d12	21.397	240	2245	0.400	ng/ul	-0.01
23) Perylene-d12	23.744	264	3070m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	1604	0.919	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.207	152	772	0.182	ng/ul	-0.03
18) Fluoranthene-d10	19.230	212	1566	0.191	ng/ul	-0.02
Target Compounds						
					Qvalue	
5) Naphthalene	10.656	128	947	0.110	ng/ul	96
7) 2-Methylnaphthalene	12.278	142	697	0.137	ng/ul	96
8) 1-Methylnaphthalene	12.493	142	462	0.082	ng/ul	94
10) Acenaphthylene	14.174	152	295	0.035	ng/ul#	67
15) Phenanthrene	17.247	178	3535	0.382	ng/ul	97
16) Anthracene	17.340	178	576m	0.066	ng/ul	
19) Fluoranthene	19.262	202	5456	0.429	ng/ul#	96
20) Pyrene	19.625	202	4846	0.358	ng/ul	98
21) Benzo(a)anthracene	21.385	228	2307	0.317	ng/ul	99
22) Chrysene	21.435	228	2092	0.154	ng/ul	95
24) Benzo(b)fluoranthene	23.022	252	3269	0.316	ng/ul	95
25) Benzo(k)fluoranthene	23.063	252	1352m	0.095	ng/ul	
26) Benzo(a)pyrene	23.636	252	2100	0.186	ng/ul	98
27) Indeno(1,2,3-cd)pyrene	26.191	276	2068	0.135	ng/ul#	100
29) Benzo(g,h,i)perylene	26.959	276	1778	0.119	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM113023\
Data File : BM043117.D
Acq On : 01 Dec 2023 11:11
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023


Quant Time: Dec 01 23:18:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 00:42:42 2023
Response via : Initial Calibration

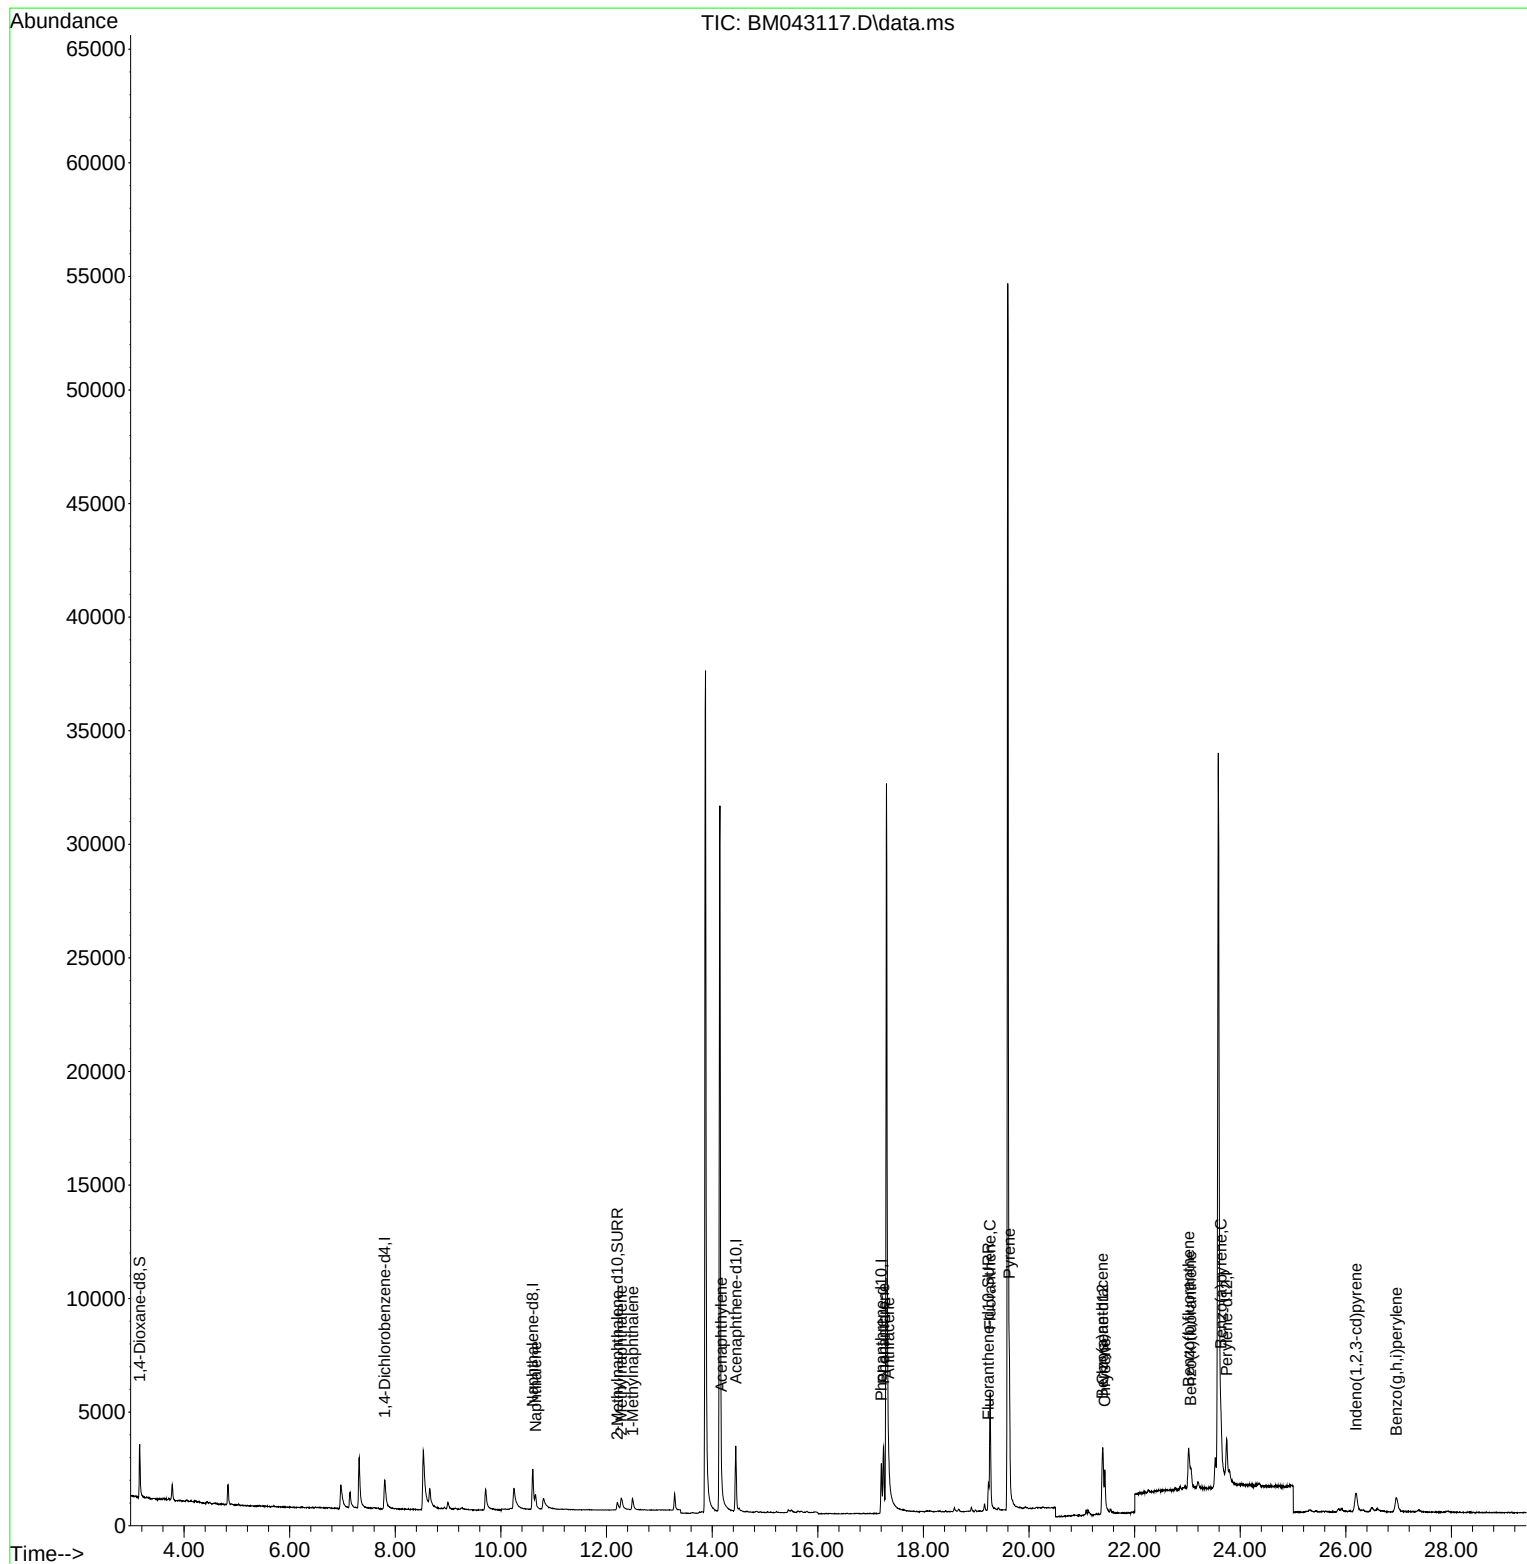



#5
Naphthalene
Concen: 0.110 ng/ul
RT: 10.656 min Scan# 1786
Delta R.T. -0.033 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6

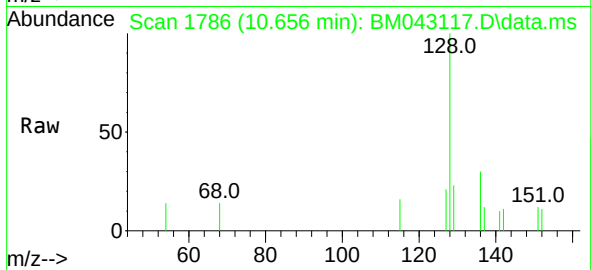


Tgt Ion:128 Resp: 947
Ion Ratio Lower Upper
128 100
129 23.1 16.0 24.0
127 21.3 16.5 24.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

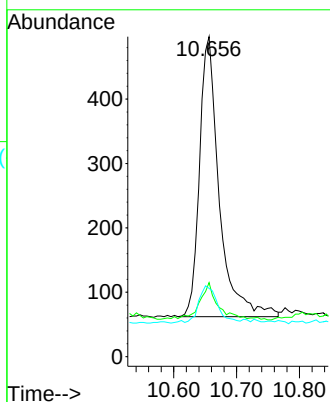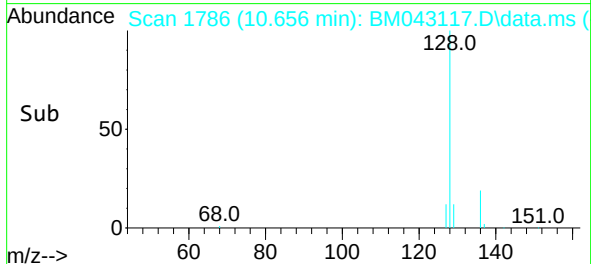


#7
2-Methylnaphthalene
Concen: 0.137 ng/ul
RT: 12.278 min Scan# 2081
Delta R.T. -0.033 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11

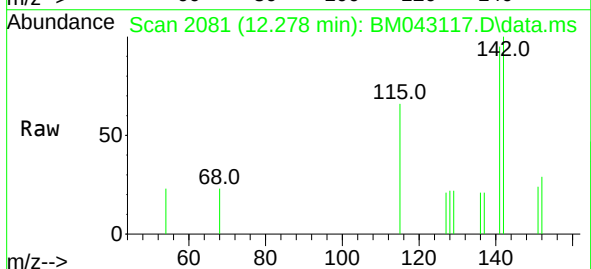


Tgt Ion:142 Resp: 697
Ion Ratio Lower Upper
142 100
141 90.8 76.1 114.1

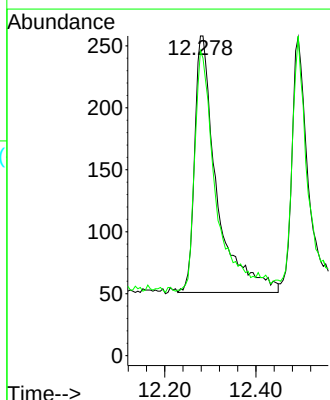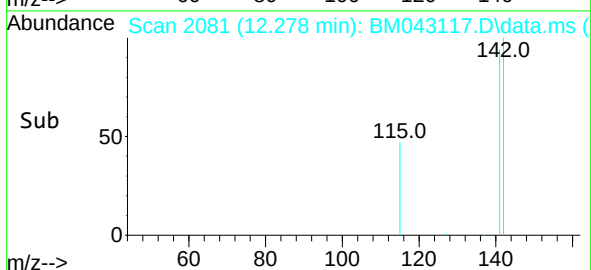

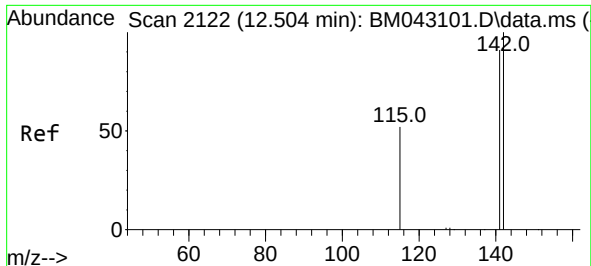

#8
1-Methylnaphthalene
Concen: 0.082 ng/ul
RT: 12.493 min Scan# 2122
Delta R.T. -0.016 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6

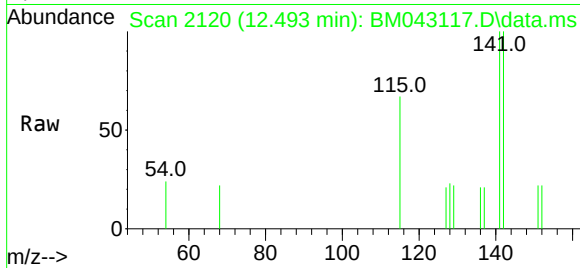


Tgt Ion:142 Resp: 462
Ion Ratio Lower Upper
142 100
141 97.8 73.8 110.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

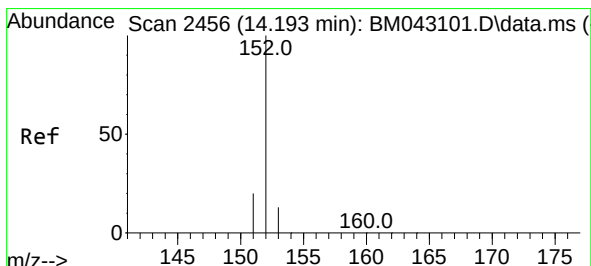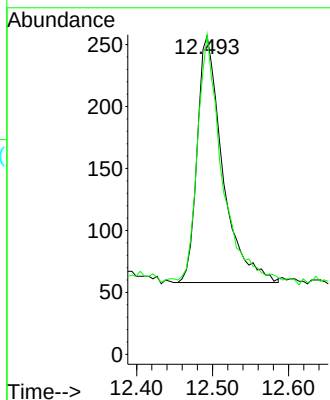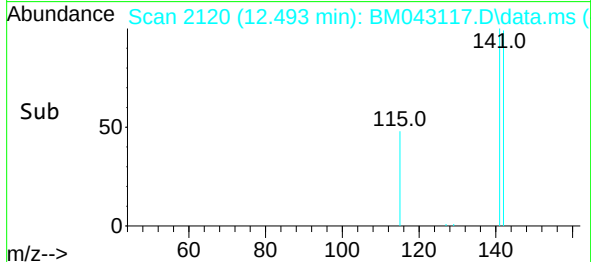


#10
Acenaphthylene
Concen: 0.035 ng/ul
RT: 14.174 min Scan# 2452
Delta R.T. -0.023 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11

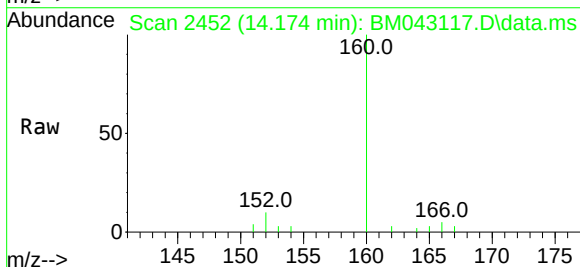


Tgt Ion:152 Resp: 295
Ion Ratio Lower Upper
152 100
151 40.9 19.4 29.0#
153 32.7 14.6 21.8#

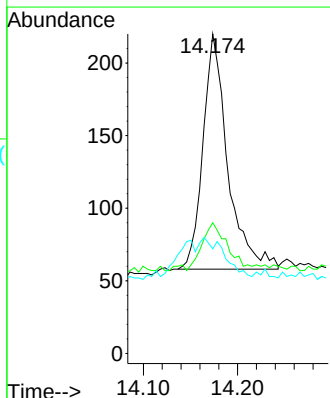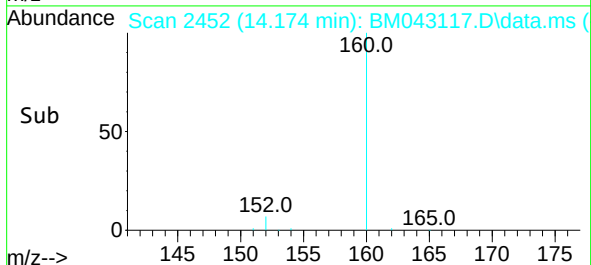

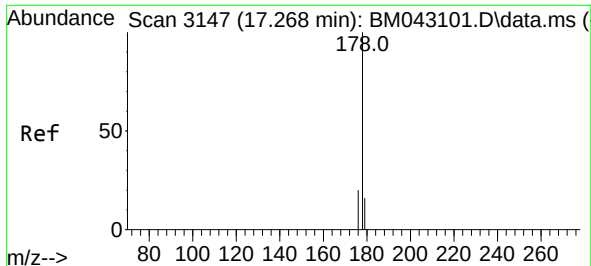

#15
Phenanthrene
Concen: 0.382 ng/ul
RT: 17.247 min Scan# 3142
Delta R.T. -0.025 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6

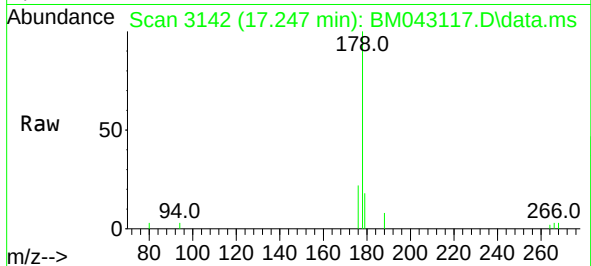


Tgt Ion:178 Resp: 353
Ion Ratio Lower Upper
178 100
179 18.4 15.7 23.5
176 22.5 18.9 28.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

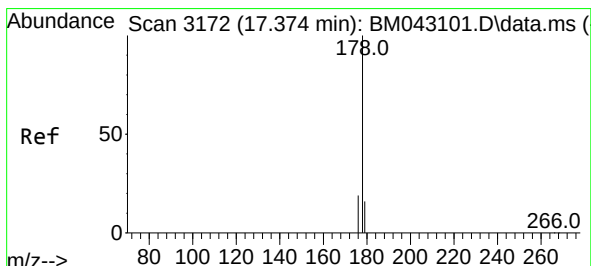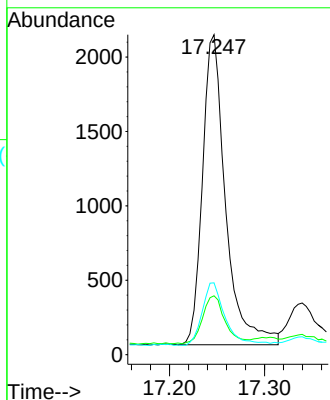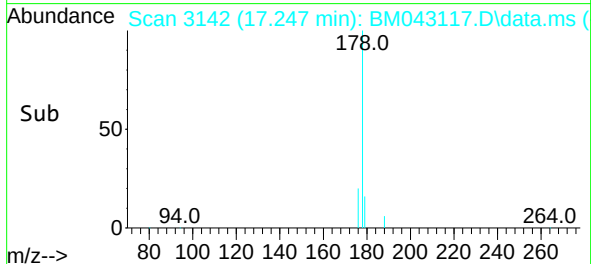


#16
Anthracene
Concen: 0.066 ng/ul m
RT: 17.340 min Scan# 3164
Delta R.T. -0.038 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11

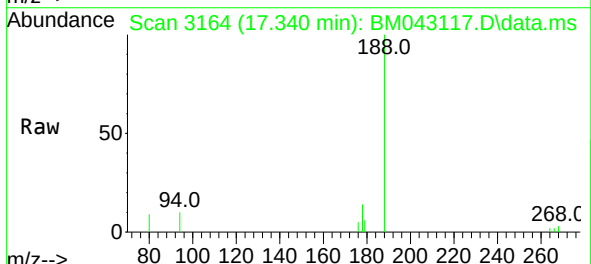


Tgt Ion:178 Resp: 576
Ion Ratio Lower Upper
178 100
179 39.2 17.3 25.9#
176 34.6 20.5 30.7#

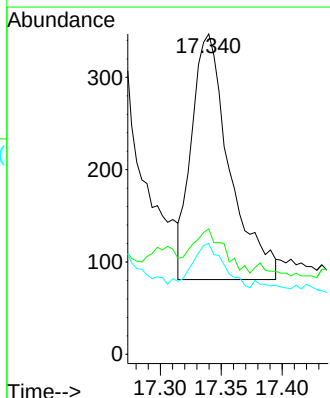



#19
Fluoranthene
Concen: 0.429 ng/u1
RT: 19.262 min Scan# 30
Delta R.T. -0.018 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6



Tgt Ion:202 Resp: 5450
Ion Ratio Lower Upper
202 100
101 8.7 7.8 11.8
100 7.0 7.1 10.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

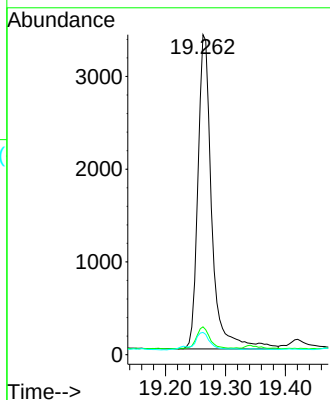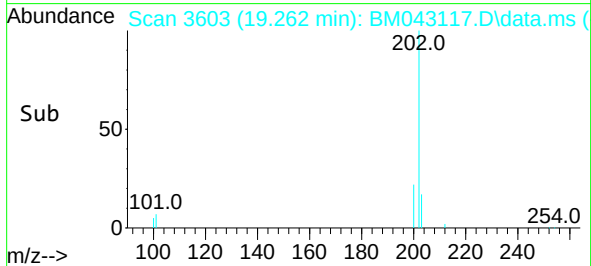

#20
Pyrene
Concen: 0.358 ng/u1
RT: 19.625 min Scan# 3681
Delta R.T. -0.023 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11


Tgt Ion:202 Resp: 4846
Ion Ratio Lower Upper
202 100
101 10.1 8.7 13.1
100 10.1 7.8 11.8

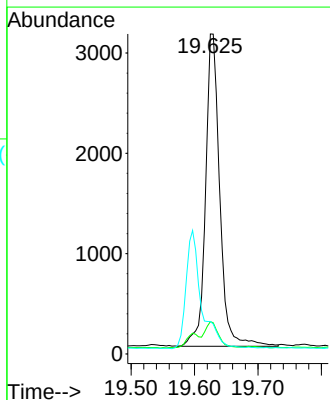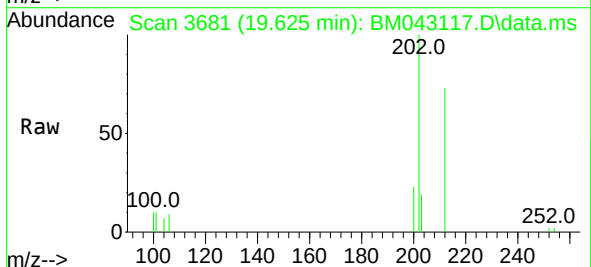



#21
Benzo(a)anthracene
Concen: 0.317 ng/ul
RT: 21.385 min Scan# 4172
Delta R.T. -0.014 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6




Tgt Ion:228 Resp: 2307
Ion Ratio Lower Upper
228 100
229 24.7 19.4 29.0
226 31.5 24.9 37.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

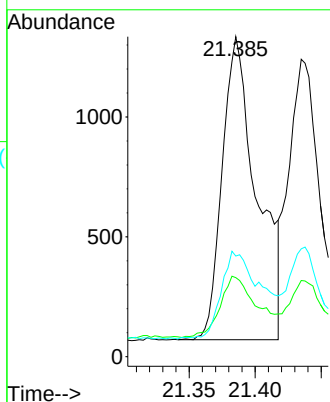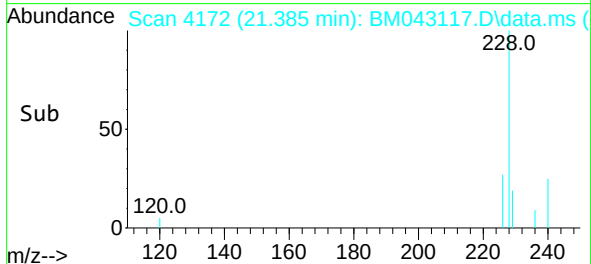


#22
Chrysene
Concen: 0.154 ng/ul
RT: 21.435 min Scan# 4189
Delta R.T. -0.014 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11

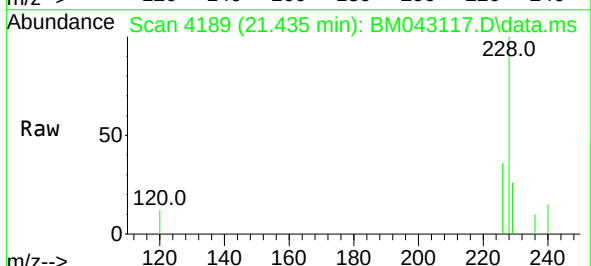


Tgt Ion:228 Resp: 2092
Ion Ratio Lower Upper
228 100
226 36.3 27.2 40.8
229 25.6 18.0 27.0

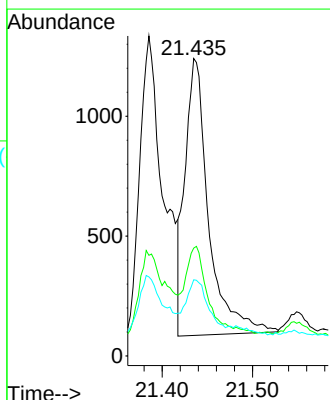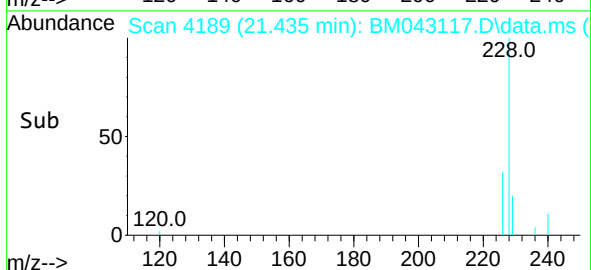



#24
Benzo(b)fluoranthene
Concen: 0.316 ng/ul
RT: 23.022 min Scan# 4732
Delta R.T. -0.014 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6




Tgt Ion:252 Resp: 3269
Ion Ratio Lower Upper
252 100
253 37.1 0.0 71.8
125 19.3 0.0 29.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

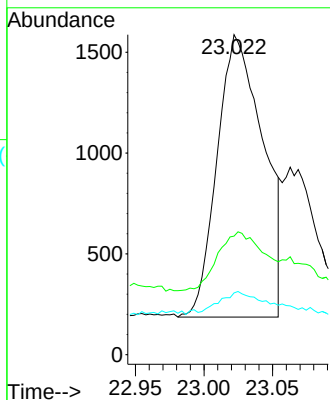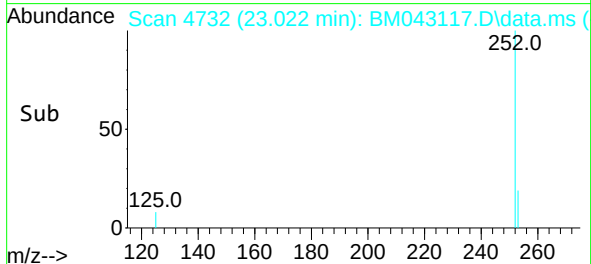


#25
Benzo(k)fluoranthene
Concen: 0.095 ng/ul m
RT: 23.063 min Scan# 4746
Delta R.T. -0.026 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11

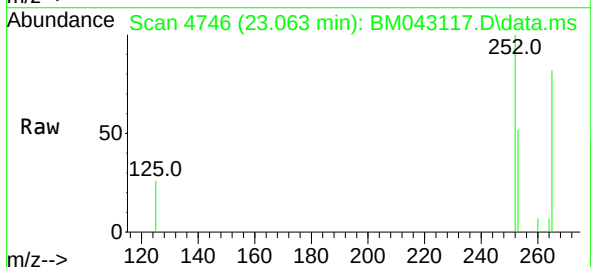


Tgt Ion:252 Resp: 1352
Ion Ratio Lower Upper
252 100
253 52.2 28.2 42.2#
125 26.0 11.0 16.6#

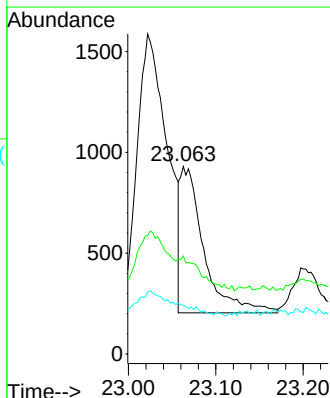



#26
Benzo(a)pyrene
Concen: 0.186 ng/ul
RT: 23.636 min Scan# 4952
Delta R.T. -0.032 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11




Instrument :
BNA_M
ClientSampleId :
C0AA6



Tgt Ion:252 Resp: 2100
Ion Ratio Lower Upper
252 100
253 46.2 36.6 55.0
125 22.3 16.2 24.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

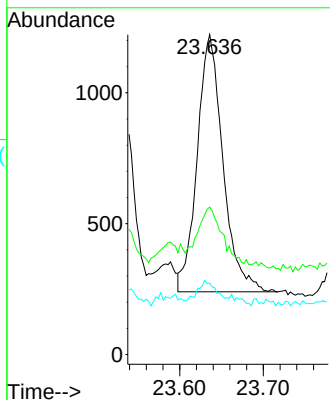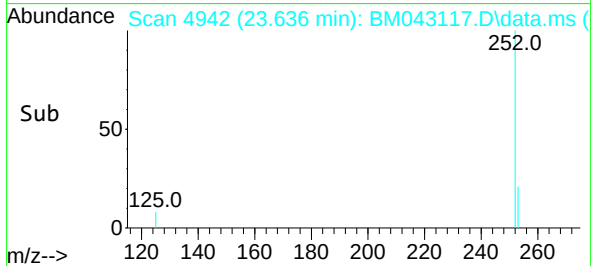

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.135 ng/ul
RT: 26.191 min Scan# 5764
Delta R.T. -0.037 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11


Tgt Ion:276 Resp: 2068
Ion Ratio Lower Upper
276 100
138 13.8 0.0 0.0#
227 0.2 0.2 0.2#

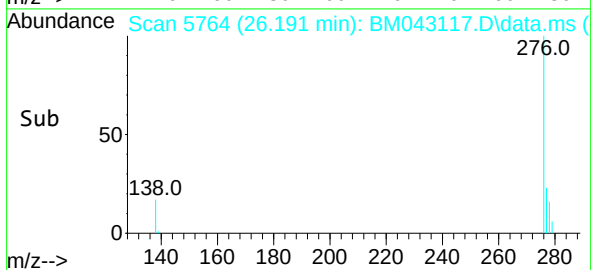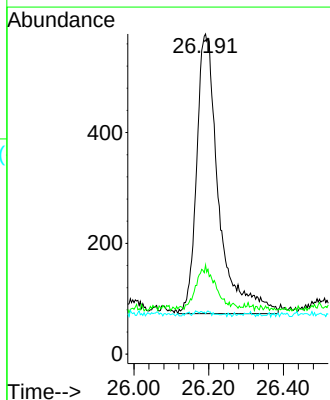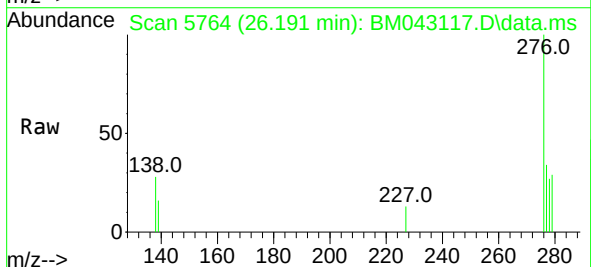



#29
Benzo(g,h,i)perylene
Concen: 0.119 ng/ul
RT: 26.959 min Scan# 5993
Delta R.T. -0.027 min
Lab File: BM043117.D
Acq: 01 Dec 2023 11:11

Instrument :
BNA_M
ClientSampleId :
C0AA6



Tgt Ion:276 Resp: 1778
Ion Ratio Lower Upper
276 100
138 26.6 17.8 26.8
277 36.5 23.8 35.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/04/2023
Supervised By :mohammad ahmed 12/04/2023

